

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051622\
 Data File : FB027206.D
 Signal(s) : FID2B.CH
 Acq On : 16 May 2022 15:41
 Operator : AJ/MA
 Sample : BSF0516S2
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 16 21:15:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
 Quant Title :
 QLast Update : Tue May 10 13:42:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	210473	20.050 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.718	450241	28.293 ng/ml
2) t 2,2,4-Trimethylpentane	7.435	507981	31.485 ng/ml
3) t n-Heptane	7.755	136879	8.376 ng/ml
4) t Benzene	7.892	174654	9.418 ng/ml
6) t Toluene	10.626	510465	28.752 ng/ml
7) t Ethylbenzene	13.062	169745	10.279 ng/ml
8) t m-Xylene	13.195	327160	19.883 ng/ml
9) t O-Xylene	13.923	341881	20.843 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	387497	23.210 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051622\
Data File : FB027206.D
Signal(s) : FID2B.CH
Acq On : 16 May 2022 15:41
Operator : AJ/MA
Sample : BSF0516S2
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 16 21:15:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
Quant Title :
QLast Update : Tue May 10 13:42:12 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

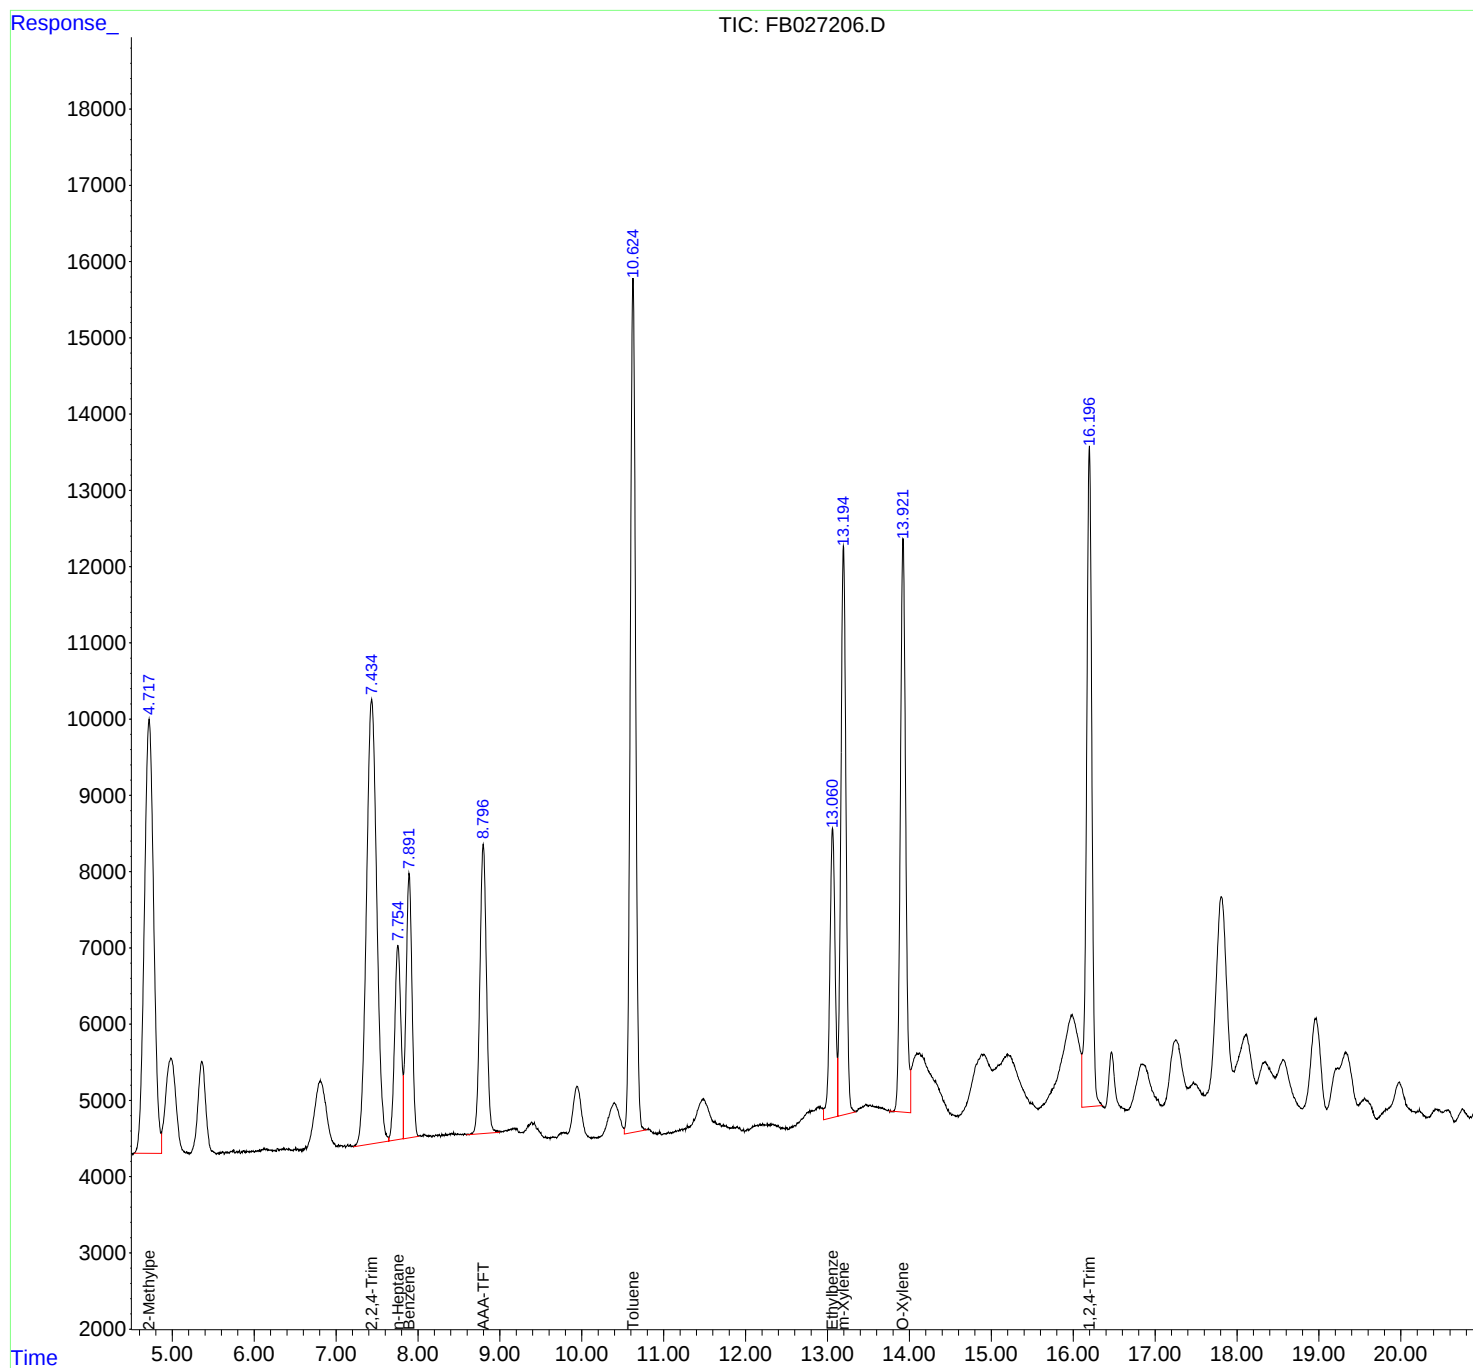

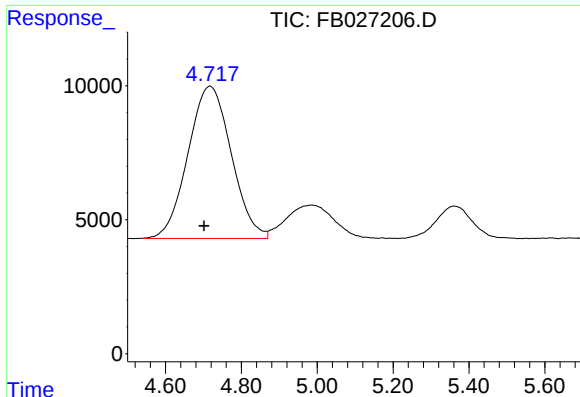


#1 2-Methylpentane

R.T.: 4.718 min
Delta R.T.: 0.016 min
Response: 450241
Conc: 28.29 ng/ml

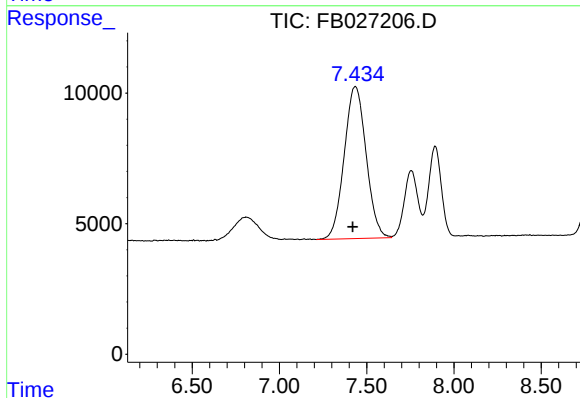


#2 2,2,4-Trimethylpentane

R.T.: 7.435 min
Delta R.T.: 0.015 min
Response: 507981
Conc: 31.49 ng/ml

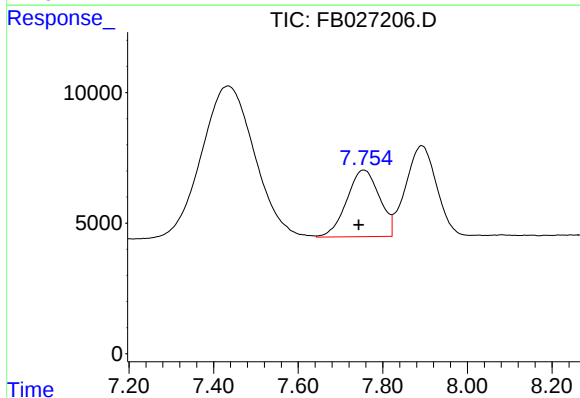


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.012 min
Response: 136879
Conc: 8.38 ng/ml

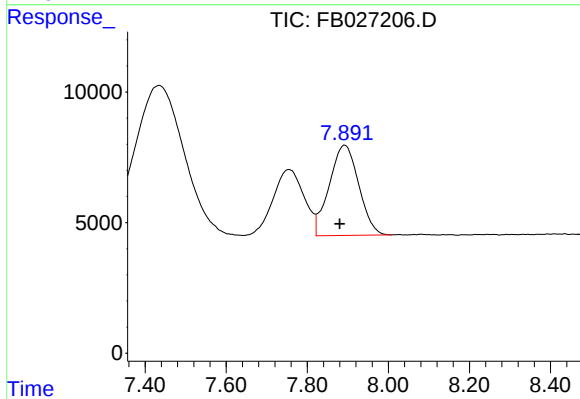


#4 Benzene

R.T.: 7.892 min
Delta R.T.: 0.012 min
Response: 174654
Conc: 9.42 ng/ml

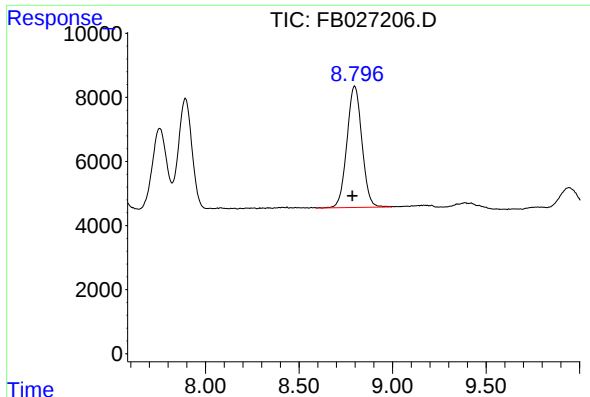


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.012 min
Response: 210473
Conc: 20.05 ng/ml

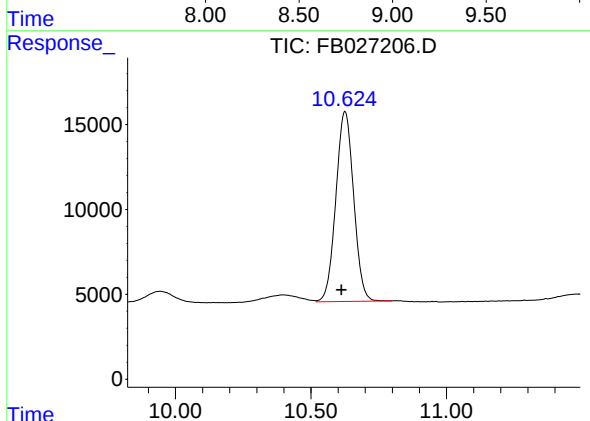


#6 Toluene

R.T.: 10.626 min
Delta R.T.: 0.013 min
Response: 510465
Conc: 28.75 ng/ml

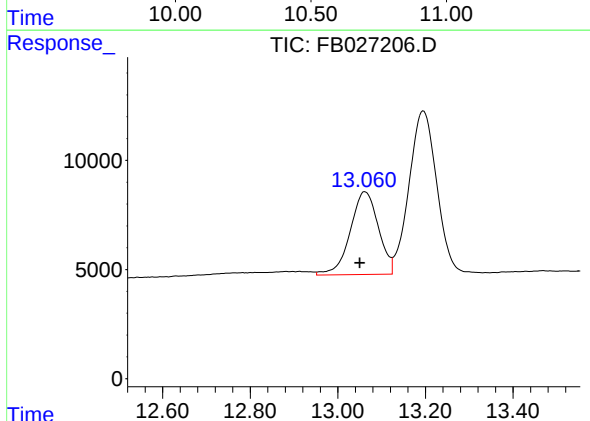


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: 0.012 min
Response: 169745
Conc: 10.28 ng/ml

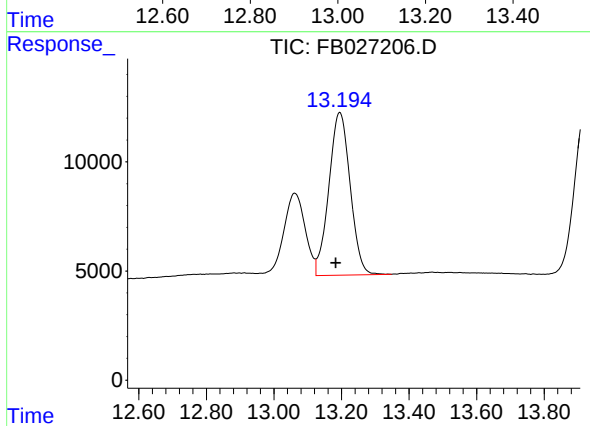


#8 m-Xylene

R.T.: 13.195 min
Delta R.T.: 0.013 min
Response: 327160
Conc: 19.88 ng/ml

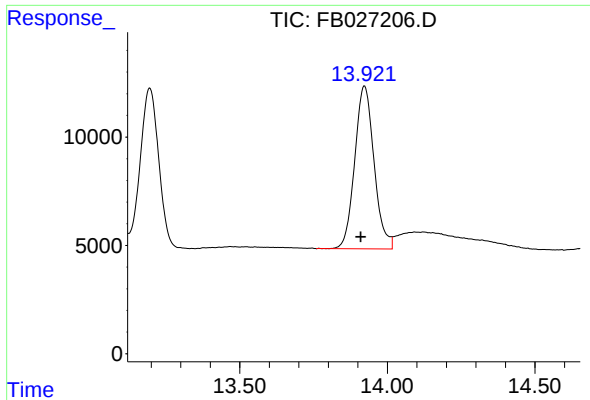

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: 0.013 min
Response: 341881
Conc: 20.84 ng/ml

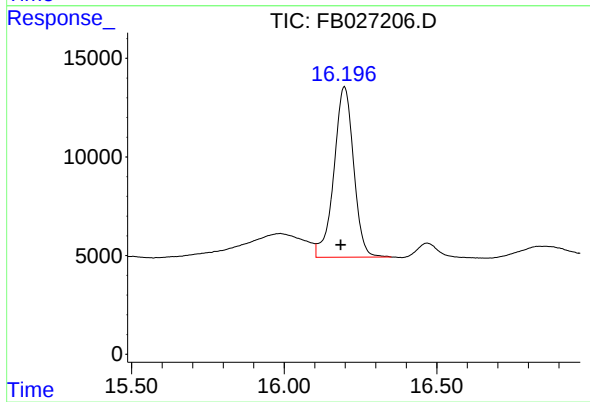

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.012 min
Response: 387497
Conc: 23.21 ng/ml