

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051722\
 Data File : FB027244.D
 Signal(s) : FID2B.CH
 Acq On : 17 May 2022 15:12
 Operator : AJ/MA
 Sample : BSF0517S2
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: May 18 00:26:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
 Quant Title :
 QLast Update : Tue May 10 13:42:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	221910	21.140 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	487685	30.646 ng/ml
2) t 2,2,4-Trimethylpentane	7.430	517433	32.071 ng/ml
3) t n-Heptane	7.752	166393	10.182 ng/ml
4) t Benzene	7.889	204864	11.047 ng/ml
6) t Toluene	10.622	593248	33.415 ng/ml
7) t Ethylbenzene	13.059	180743	10.945 ng/ml
8) t m-Xylene	13.191	360221	21.892 ng/ml
9) t O-Xylene	13.919	352742	21.505 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	353605	21.180 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051722\
Data File : FB027244.D
Signal(s) : FID2B.CH
Acq On : 17 May 2022 15:12
Operator : AJ/MA
Sample : BSF0517S2
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 18 00:26:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
Quant Title :
QLast Update : Tue May 10 13:42:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

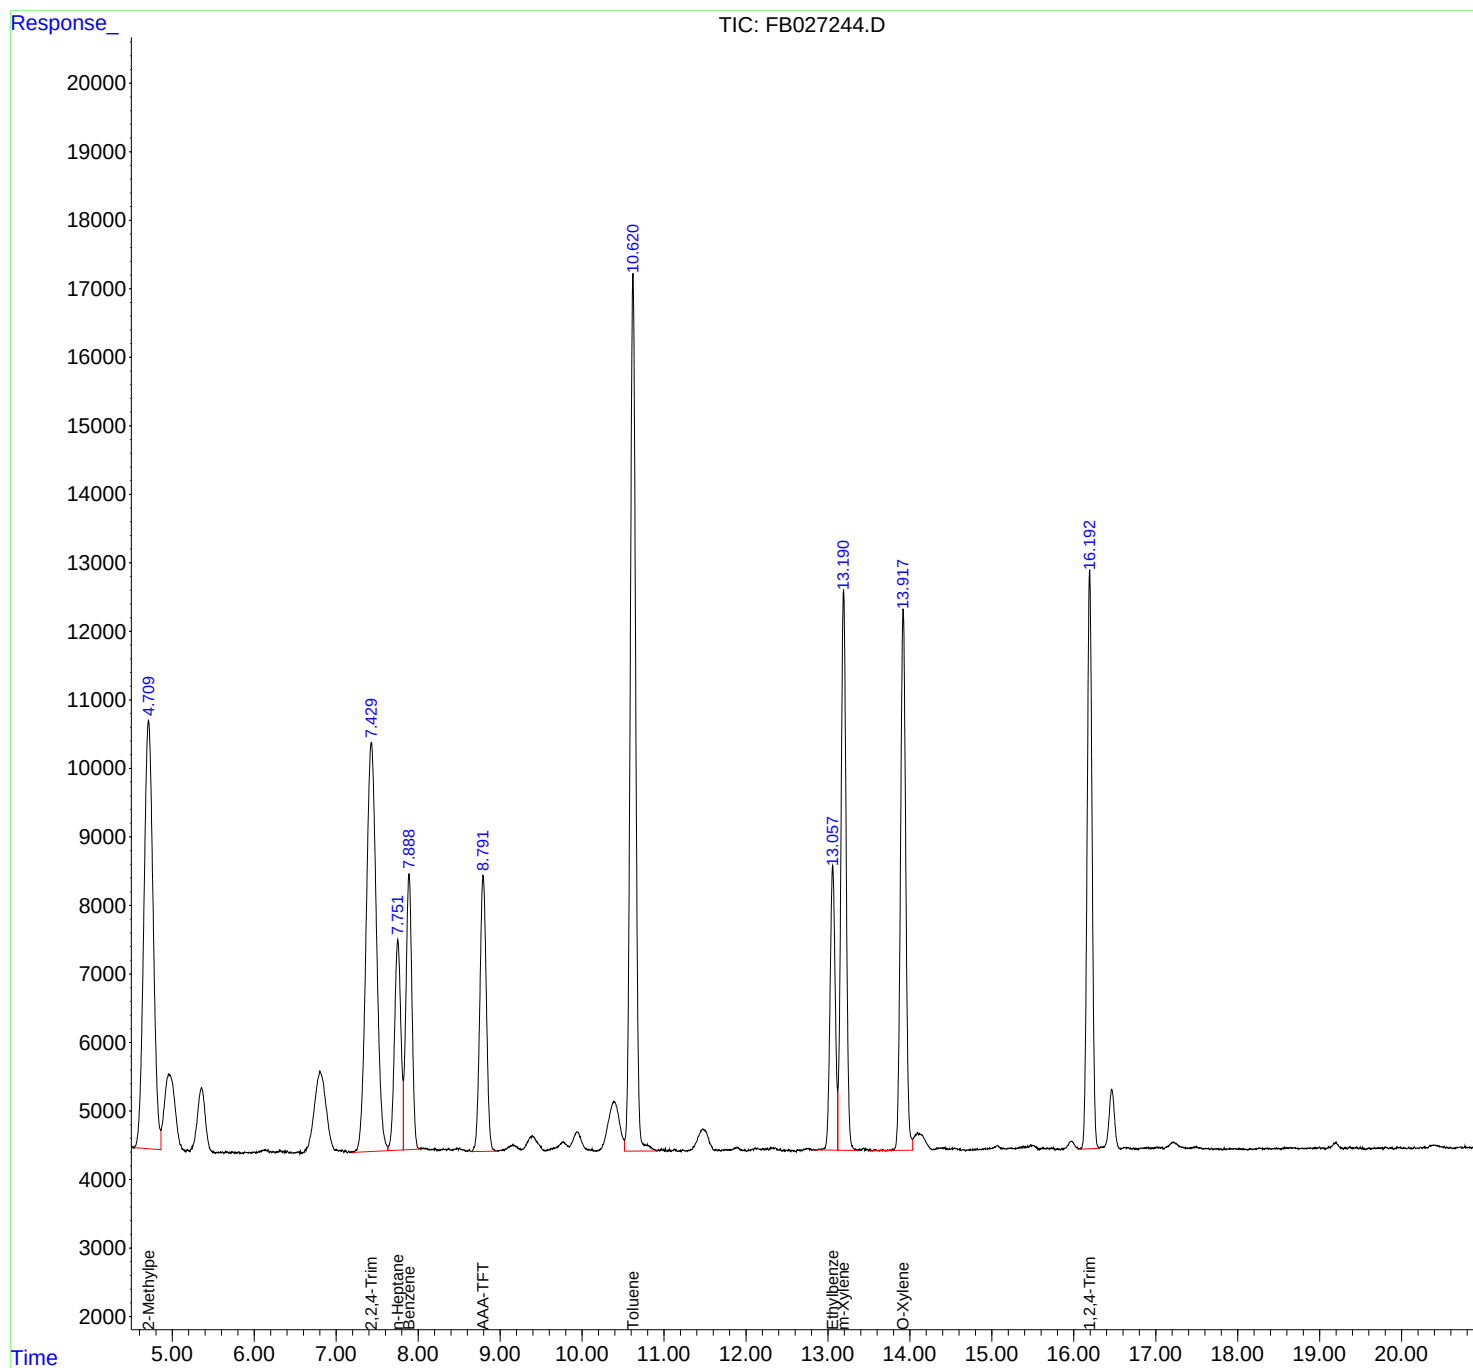


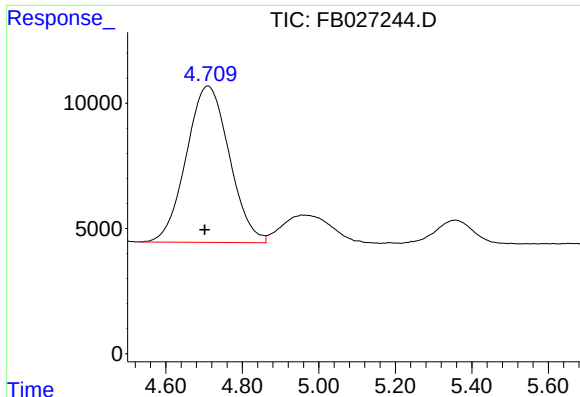

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.009 min
Response: 487685
Conc: 30.65 ng/ml

Instrument :
FID_B
ClientSampleId :

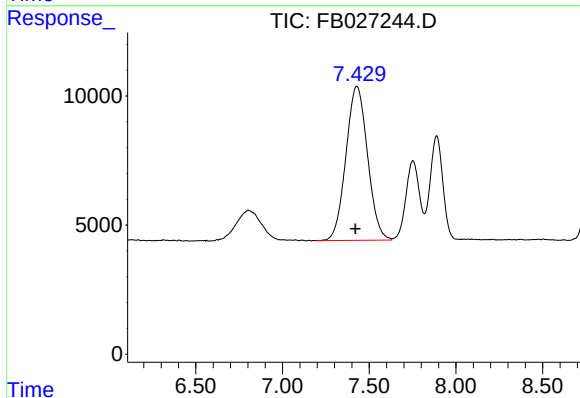


#2 2,2,4-Trimethylpentane

R.T.: 7.430 min
Delta R.T.: 0.010 min
Response: 517433
Conc: 32.07 ng/ml

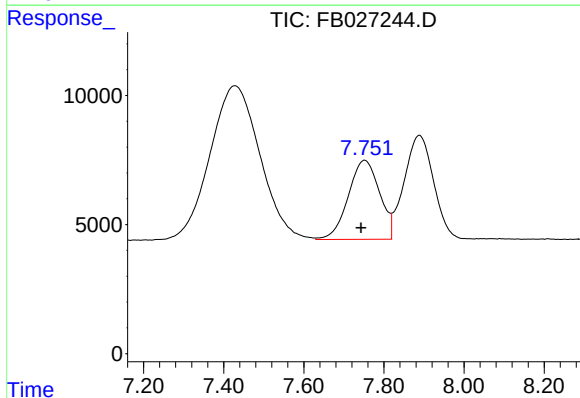


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.008 min
Response: 166393
Conc: 10.18 ng/ml

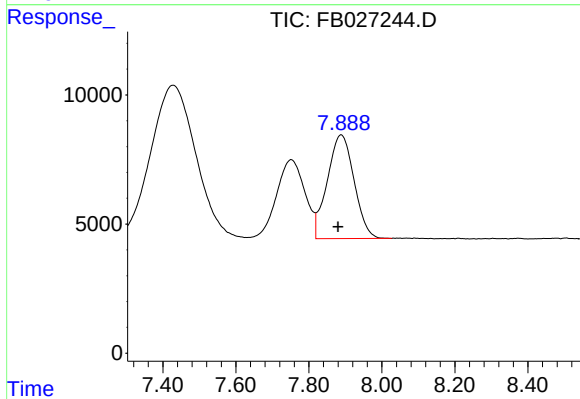

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.009 min
Response: 204864
Conc: 11.05 ng/ml

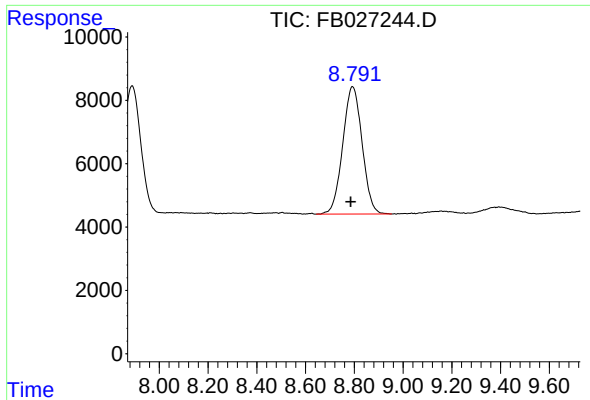

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.008 min
Response: 221910
Conc: 21.14 ng/ml

Instrument :
FID_B
ClientSampleId :

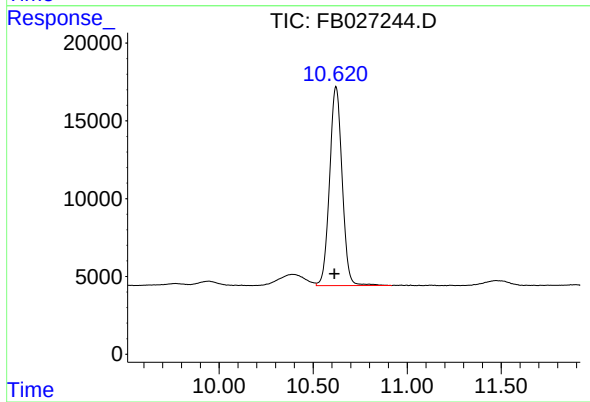


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.008 min
Response: 593248
Conc: 33.41 ng/ml

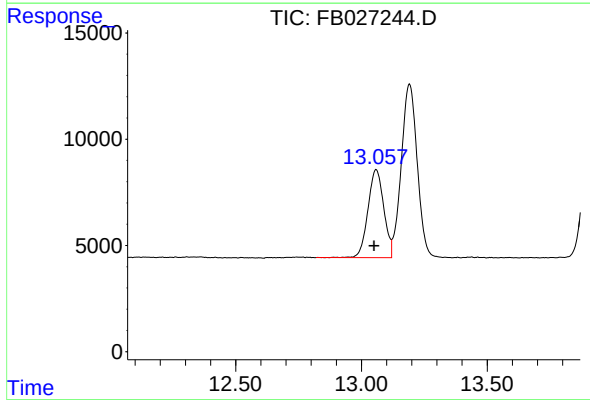


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.009 min
Response: 180743
Conc: 10.95 ng/ml

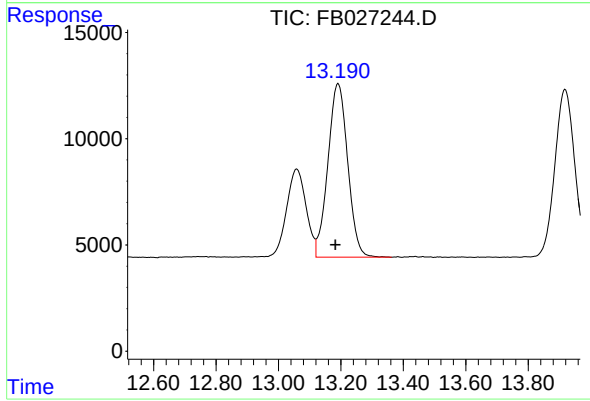

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.009 min
Response: 360221
Conc: 21.89 ng/ml

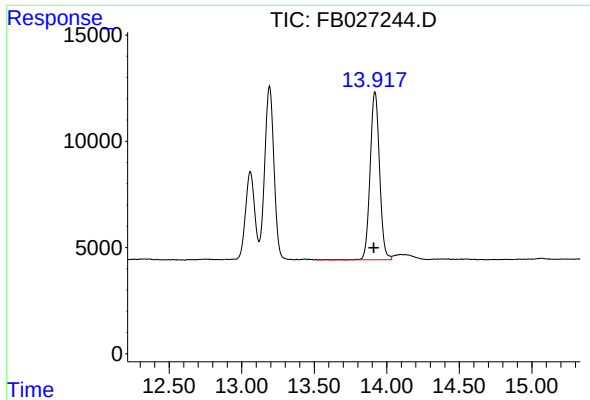

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.008 min
Response: 352742
Conc: 21.51 ng/ml

Instrument :
FID_B
ClientSampleId :

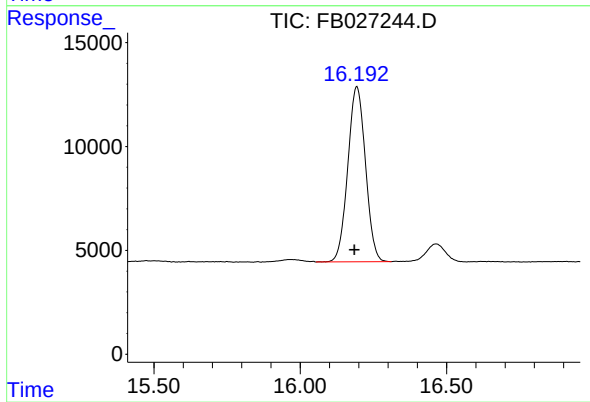

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.008 min
Response: 353605
Conc: 21.18 ng/ml