

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051722\
 Data File : PS019437.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 May 2022 23:37
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 00:52:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
 Quant Title : 8080.M
 QLast Update : Wed May 04 16:27:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.247	0.000	1584428	0	<MDL	N.D.	#
Target Compounds								
2) T	3,5-DICHL...	6.471f	5.908f	4422911	358424	1.251	<MDL	#
3) T	4-Nitroph...	7.056	0.000	543941	0	<MDL	N.D.	#
5) T	DICAMBA	7.418	6.976	917797	126715	<MDL	<MDL	#
6) T	MCP	0.000	7.074	0	133155	N.D.	<MDL	#
7) T	MCPA	7.729	0.000	529393	0	<MDL	N.D.	#
8) T	DICHLORPROP	8.099	7.638f	-51091	670064	N.D.	<MDL	#
9) T	2,4-D	8.326	0.000	579726	0	<MDL	N.D.	#
10) T	Pentachlo...	8.655	8.308	1184550	383088	<MDL	<MDL	#
11) T	2,4,5-TP ...	9.166	8.645	104887	929968	<MDL	<MDL	#
12) T	2,4,5-T	9.474	9.079	1018089	1157615	<MDL	<MDL	#
13) T	2,4-DB	10.010	9.586	224259	135700	<MDL	<MDL	#
14) T	DINOSEB	11.120f	0.000	56247679	0	3.407	N.D.	#
15) T	Picloram	11.016	10.807f	11992282	4901168	<MDL	<MDL	#
16) T	DCPA	11.463	10.807	1389400	4901168	<MDL	<MDL	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051722\
Data File : PS019437.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2022 23:37
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 00:52:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
Quant Title : 8080.M
QLast Update : Wed May 04 16:27:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

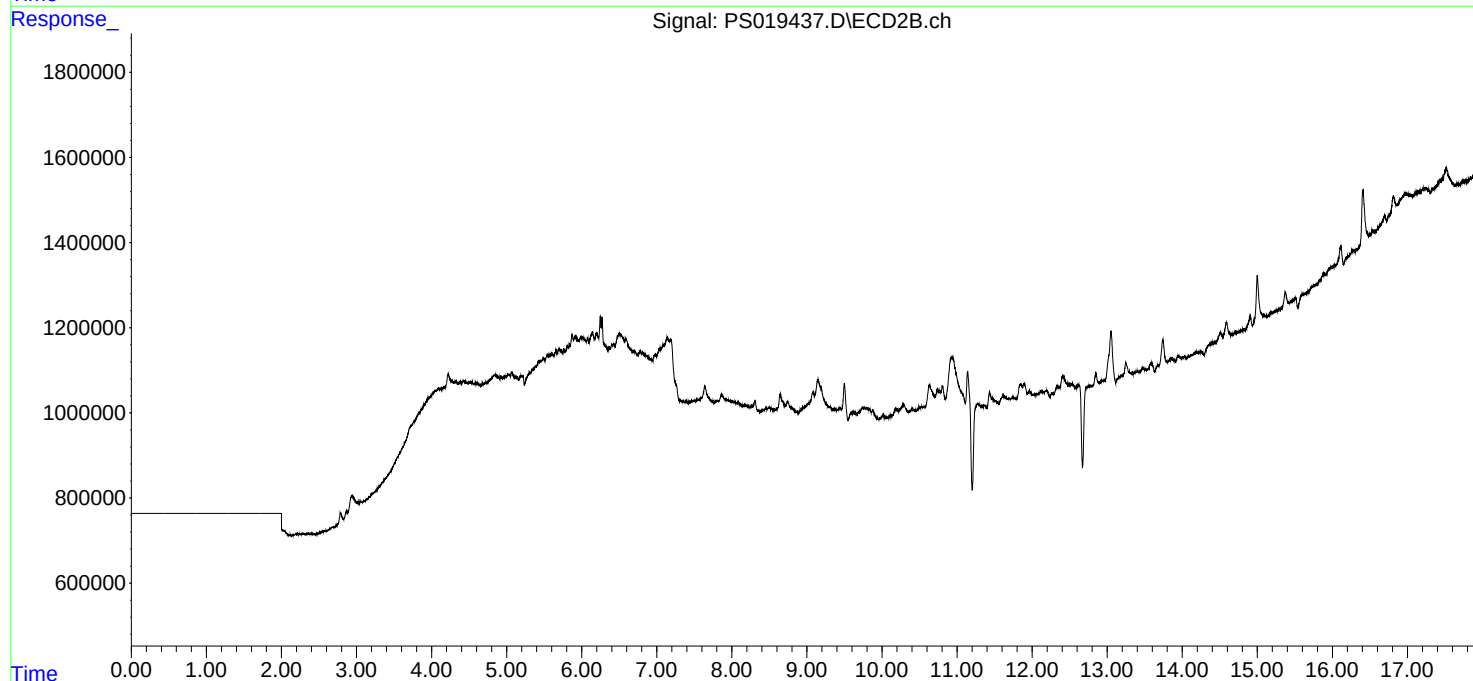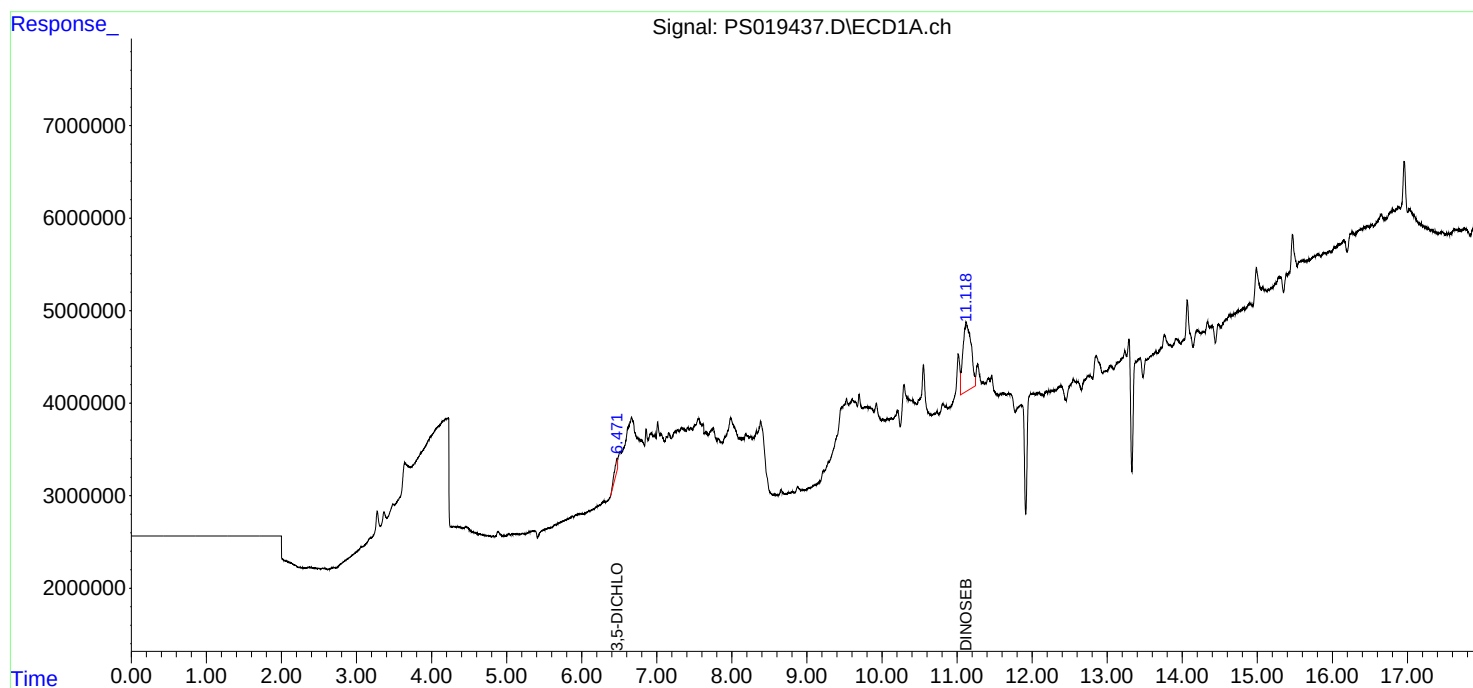


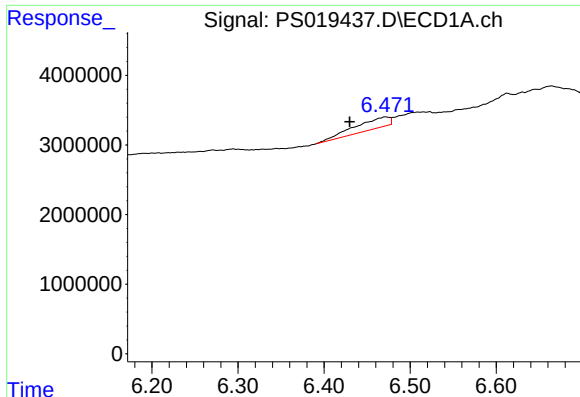

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.471 min
Delta R.T.: 0.042 min
Response: 4422911
Conc: 1.25 ng/ml

Instrument :
FID_B
ClientSampleId :

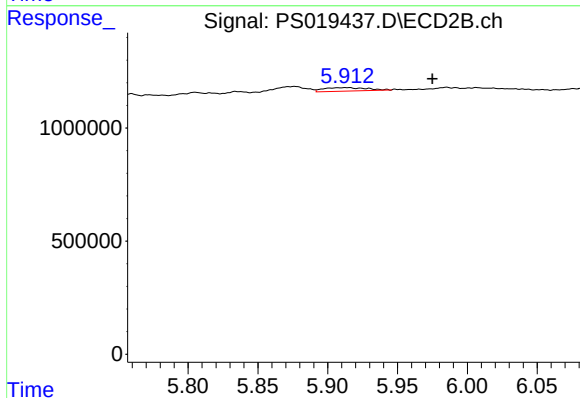


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.908 min
Delta R.T.: -0.067 min
Response: 358424
Conc: N.D.

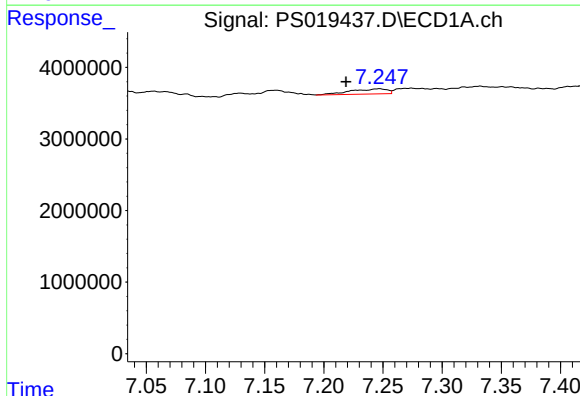


#4 2,4-DCAA

R.T.: 7.247 min
Delta R.T.: 0.028 min
Response: 1584428
Conc: N.D.

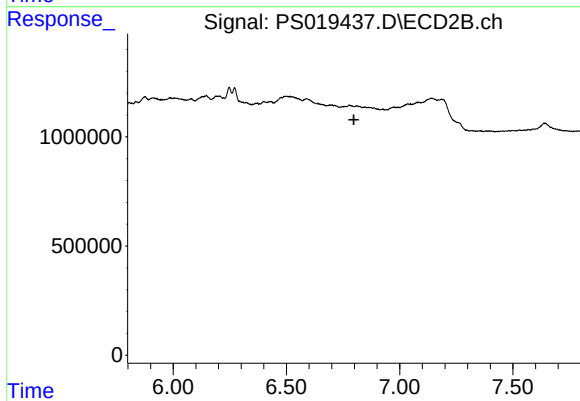

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 6.798 min
Response: 0
Conc: N.D.

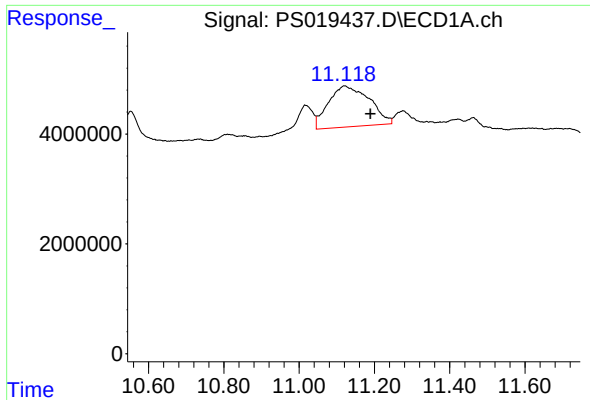

#14 DINOSEB

R.T.: 11.120 min
Delta R.T.: -0.069 min
Response: 56247679
Conc: 3.41 ng/ml

Instrument :
FID_B
ClientSampleId :

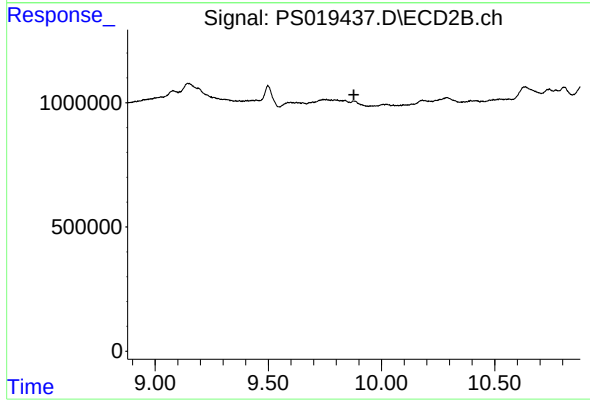

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.878 min
Response: 0
Conc: N.D.