

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051722\
 Data File : PS019439.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2022 00:25
 Operator : AJ\MA
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 00:53:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
 Quant Title : 8080.M
 QLast Update : Wed May 04 16:27:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.798	1987.8E6	549.8E6	727.884	709.851
Target Compounds							
1) T	Dalapon	3.025	2.533	3016.6E6	594.6E6	624.855	668.927
2) T	3,5-DICHL...	6.431	5.975	2244.3E6	809.1E6	634.937	693.791
3) T	4-Nitroph...	7.057	6.418	713.5E6	253.8E6	736.306	719.392
5) T	DICAMBA	7.409	6.963	7030.7E6	2381.7E6	636.591	710.790
6) T	MCPD	7.579	7.060	565.6E6	187.5E6	63.269	70.519
7) T	MCPA	7.728	7.274	726.4E6	258.3E6	58.286	69.355
8) T	DICHLORPROP	8.103	7.586	1713.8E6	599.3E6	612.613	699.287
9) T	2,4-D	8.336	7.880	1951.0E6	702.3E6	618.437	703.253
10) T	Pentachlo...	8.641	8.305	24565.6E6	7999.5E6	625.291	711.607
11) T	2,4,5-TP ...	9.194	8.667	11202.0E6	3465.6E6	619.746	720.121
12) T	2,4,5-T	9.480	9.046	13334.8E6	3111.9E6	630.454	718.663
13) T	2,4-DB	10.037	9.552	2578.8E6	388.9E6	601.370	684.015
14) T	DINOSEB	11.187	9.876	11687.7E6	2313.6E6	707.858	798.394
15) T	Picloram	11.032	10.871	18081.6E6	4033.7E6	618.596	674.436
16) T	DCPA	11.455	10.807	16959.1E6	4235.0E6	648.012	721.413



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051722\
Data File : PS019439.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2022 00:25
Operator : AJ\MA
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 00:53:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
Quant Title : 8080.M
QLast Update : Wed May 04 16:27:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

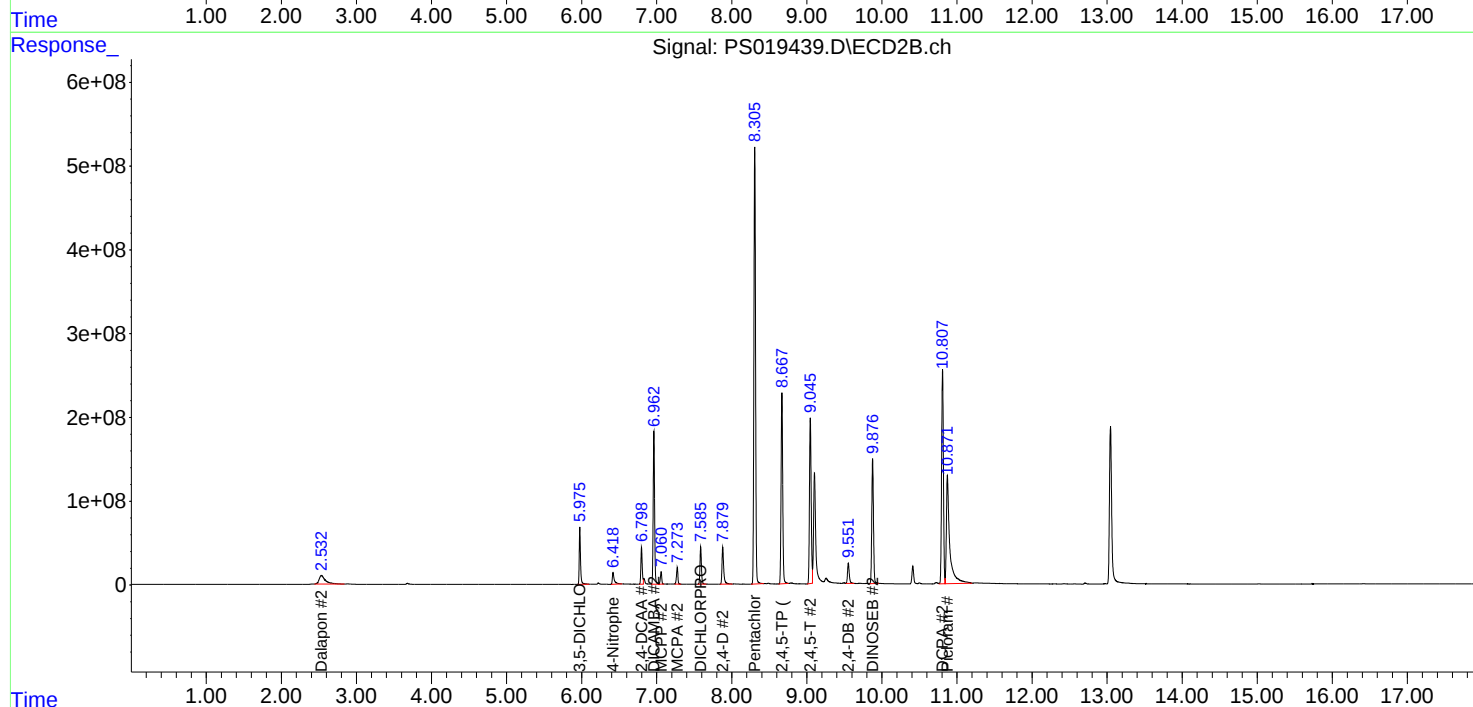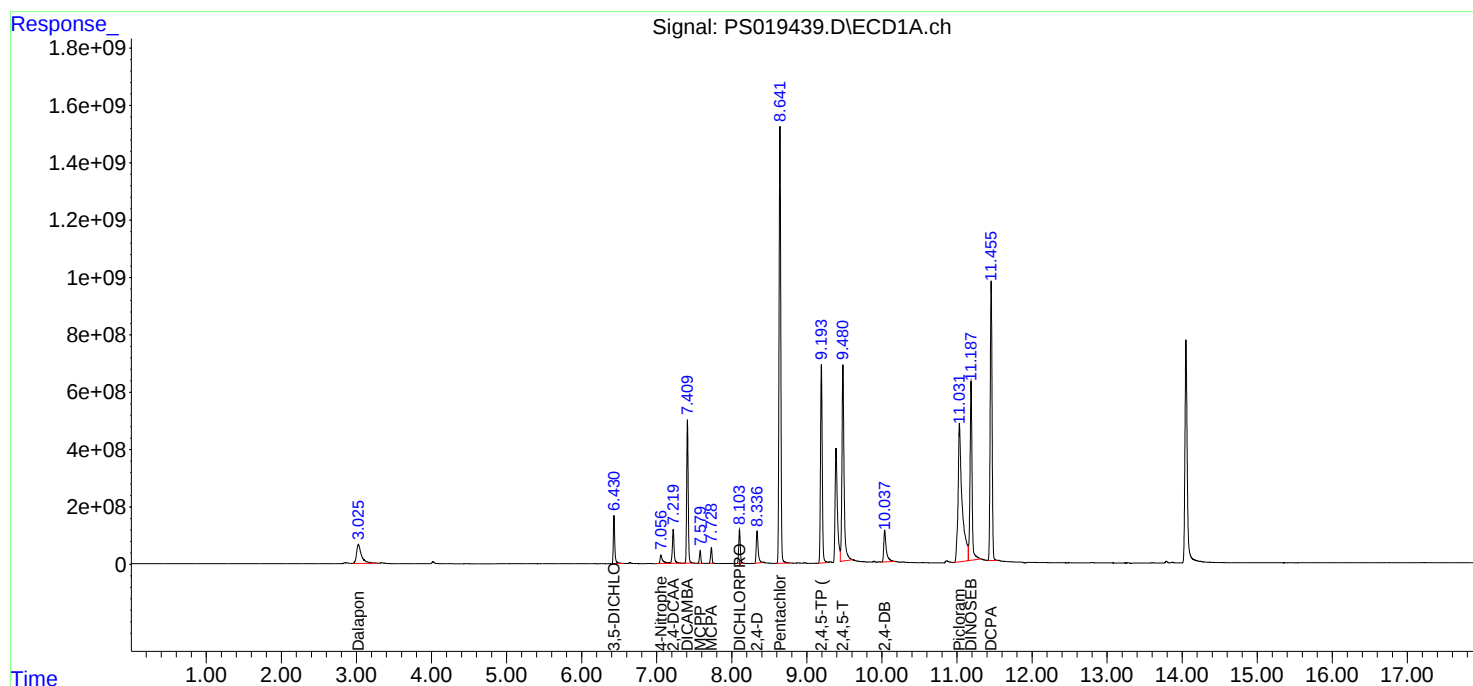


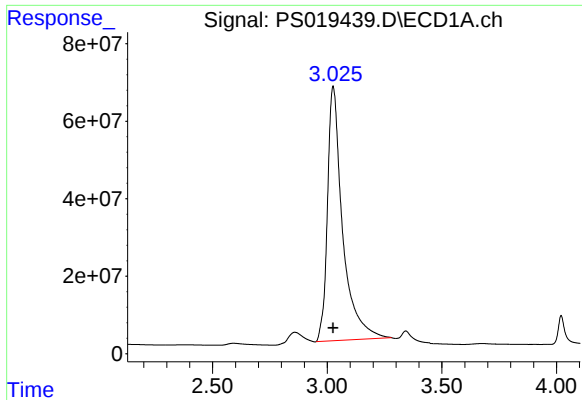

#1 Dalapon


R.T.: 3.025 min
Delta R.T.: 0.000 min
Response: 3016607498
Conc: 624.85 ng/ml

Instrument : FID_B
ClientSampleId :

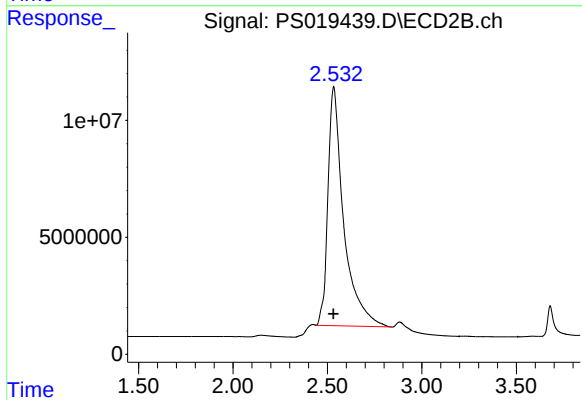


#1 Dalapon

R.T.: 2.533 min
Delta R.T.: 0.002 min
Response: 594623374
Conc: 668.93 ng/ml

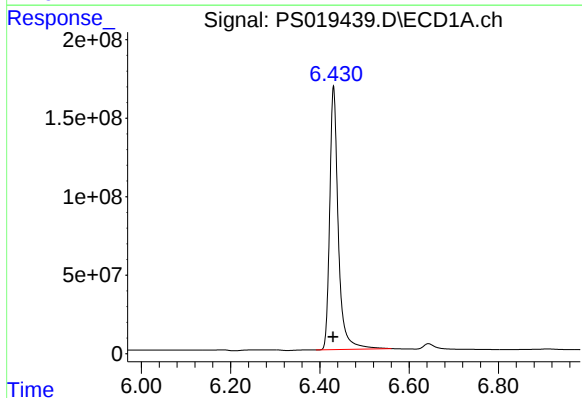


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.431 min
Delta R.T.: 0.001 min
Response: 2244298432
Conc: 634.94 ng/ml

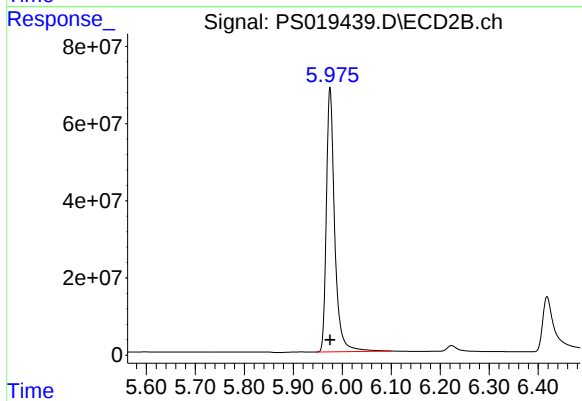

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 809129265
Conc: 693.79 ng/ml

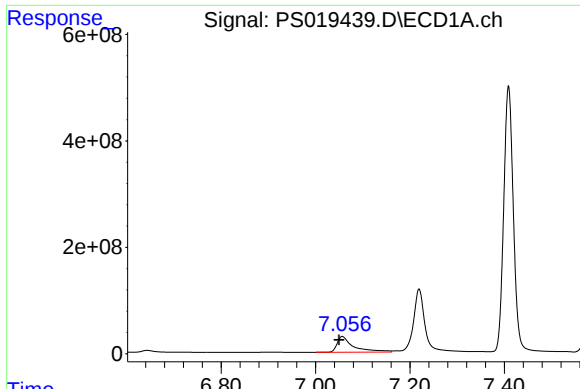

#3 4-Nitrophenol


R.T.: 7.057 min
Delta R.T.: 0.007 min
Response: 713546115
Conc: 736.31 ng/ml

Instrument :
FID_B
ClientSampleId :

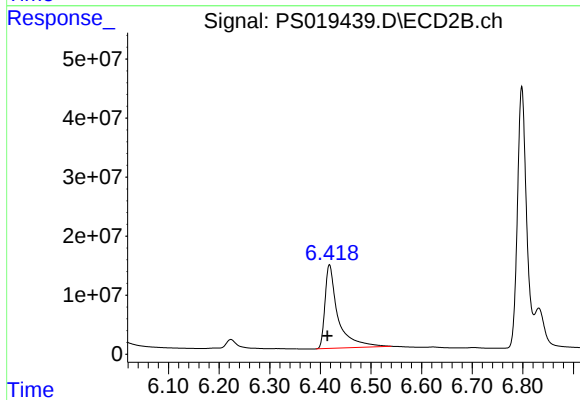


#3 4-Nitrophenol

R.T.: 6.418 min
Delta R.T.: 0.004 min
Response: 253825677
Conc: 719.39 ng/ml

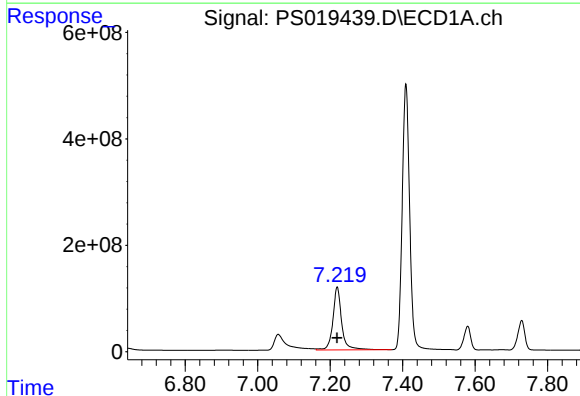


#4 2,4-DCAA

R.T.: 7.219 min
Delta R.T.: 0.000 min
Response: 1987760623
Conc: 727.88 ng/ml

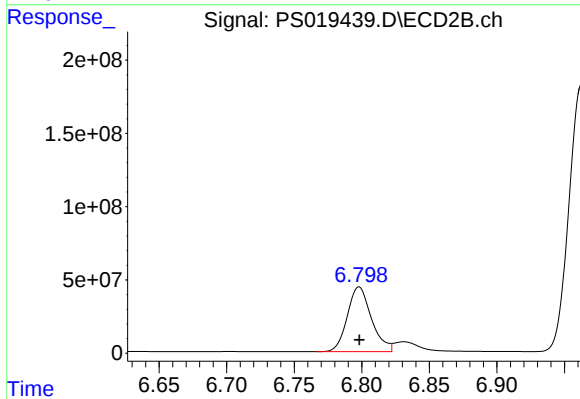

#4 2,4-DCAA


R.T.: 6.798 min
Delta R.T.: 0.000 min
Response: 549819499
Conc: 709.85 ng/ml

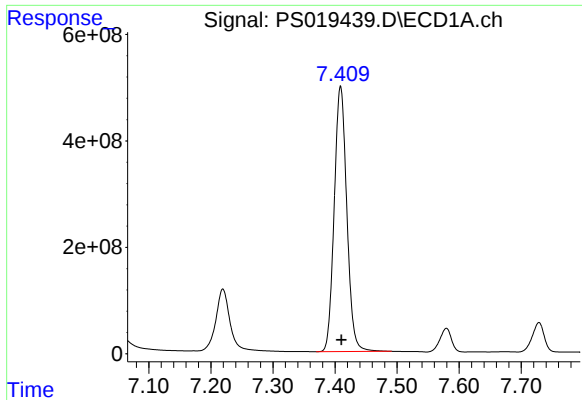

#5 DICAMBA


R.T.: 7.409 min
Delta R.T.: -0.001 min
Response: 7030703520
Conc: 636.59 ng/ml

Instrument :
FID_B
ClientSampleId :

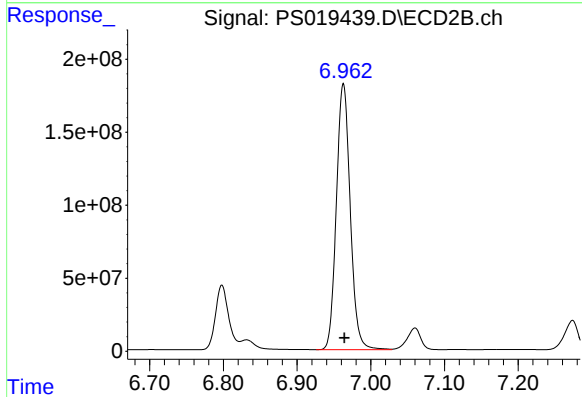


#5 DICAMBA

R.T.: 6.963 min
Delta R.T.: -0.001 min
Response: 2381725851
Conc: 710.79 ng/ml

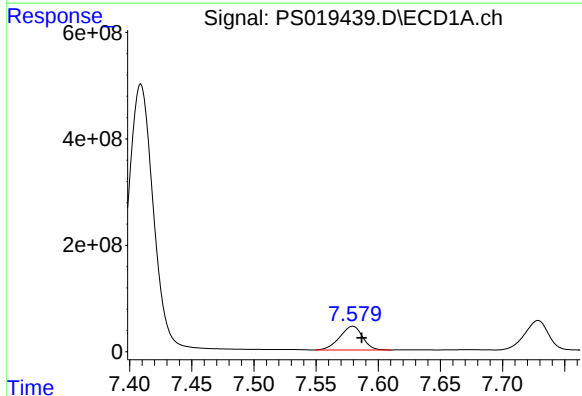


#6 MCP

R.T.: 7.579 min
Delta R.T.: -0.008 min
Response: 565578496
Conc: 63.27 ug/ml

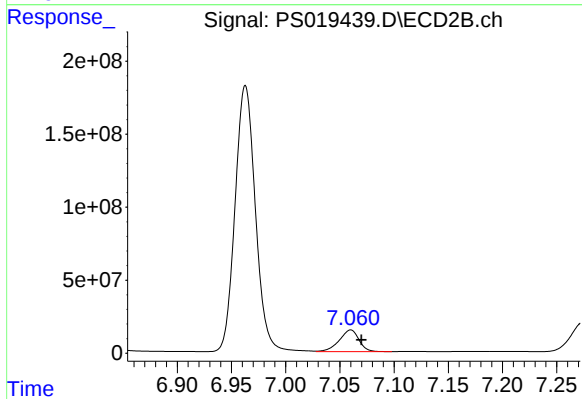

#6 MCP


R.T.: 7.060 min
Delta R.T.: -0.010 min
Response: 187533069
Conc: 70.52 ug/ml

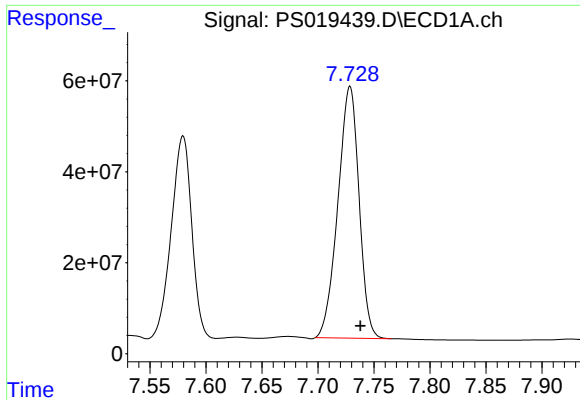

#7 MCPA


R.T.: 7.728 min
Delta R.T.: -0.009 min
Response: 726424959
Conc: 58.29 ug/ml

Instrument :
FID_B
ClientSampleId :

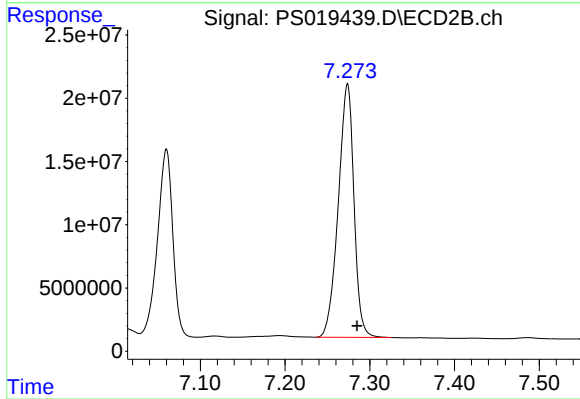


#7 MCPA

R.T.: 7.274 min
Delta R.T.: -0.011 min
Response: 258322559
Conc: 69.36 ug/ml

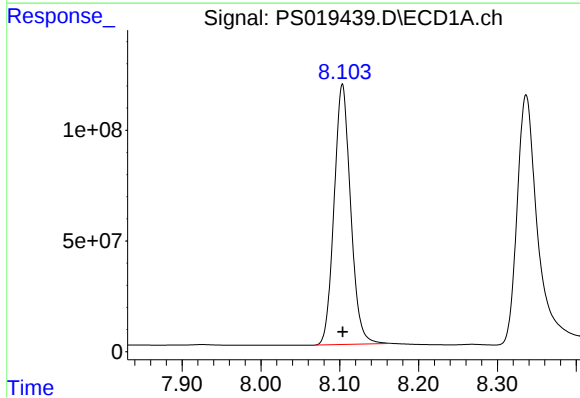


#8 DICHLORPROP

R.T.: 8.103 min
Delta R.T.: 0.000 min
Response: 1713833546
Conc: 612.61 ng/ml

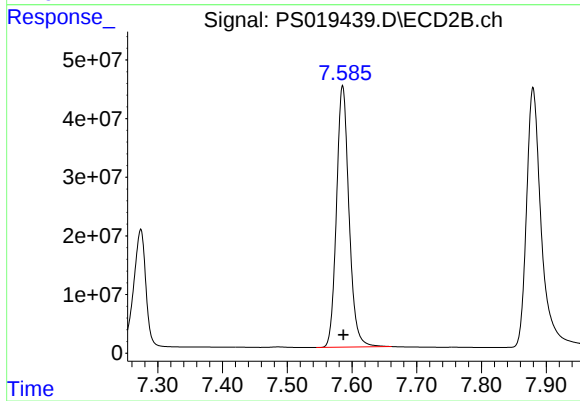

#8 DICHLORPROP


R.T.: 7.586 min
Delta R.T.: -0.001 min
Response: 599287892
Conc: 699.29 ng/ml

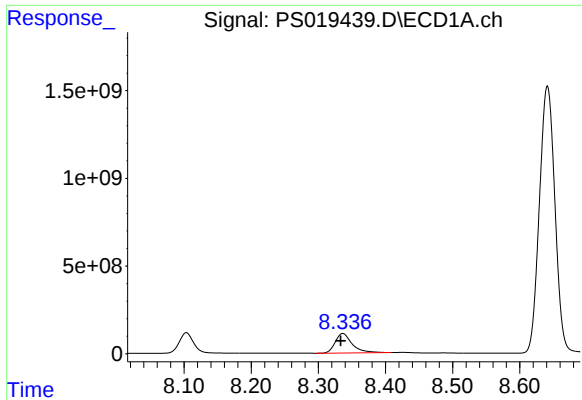

#9 2,4-D


R.T.: 8.336 min
Delta R.T.: 0.003 min
Response: 1951037640
Conc: 618.44 ng/ml

Instrument :
FID_B
ClientSampleId :

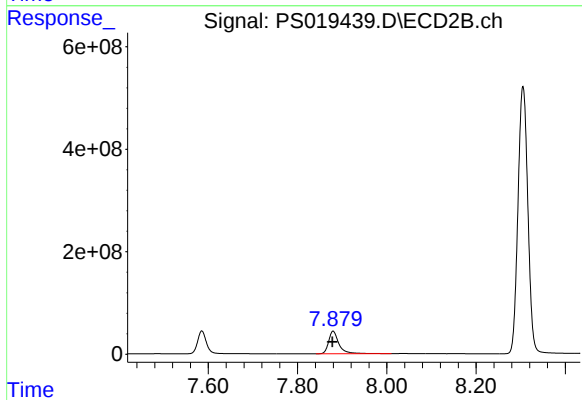


#9 2,4-D

R.T.: 7.880 min
Delta R.T.: 0.001 min
Response: 702291773
Conc: 703.25 ng/ml

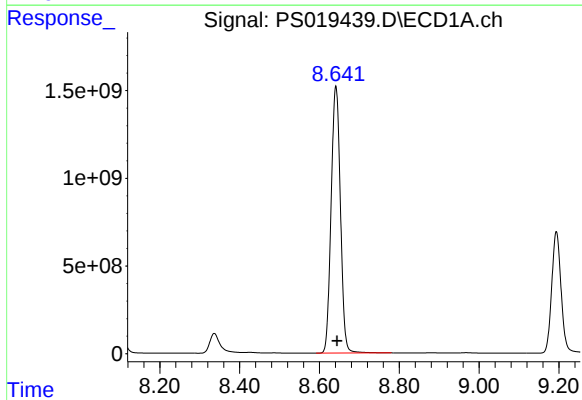


#10 Pentachlorophenol

R.T.: 8.641 min
Delta R.T.: -0.003 min
Response: 24565580868
Conc: 625.29 ng/ml

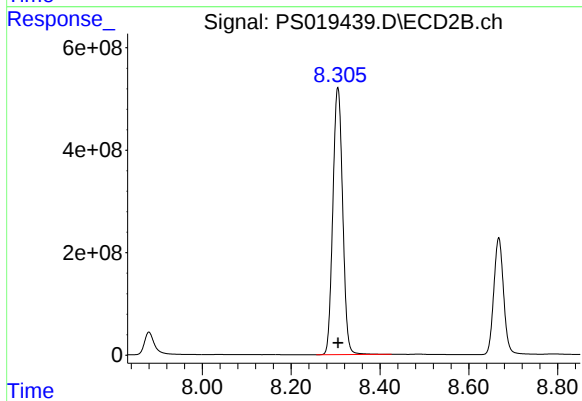

#10 Pentachlorophenol


R.T.: 8.305 min
Delta R.T.: 0.000 min
Response: 7999488979
Conc: 711.61 ng/ml

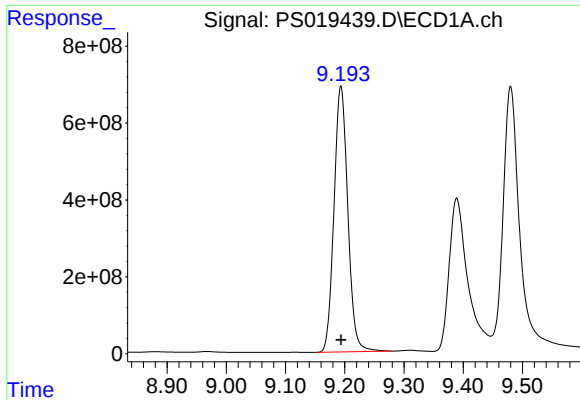

#11 2,4,5-TP (SILVEX)


R.T.: 9.194 min
Delta R.T.: 0.000 min
Response: 11201988042
Conc: 619.75 ng/ml

Instrument :
FID_B
ClientSampleId :

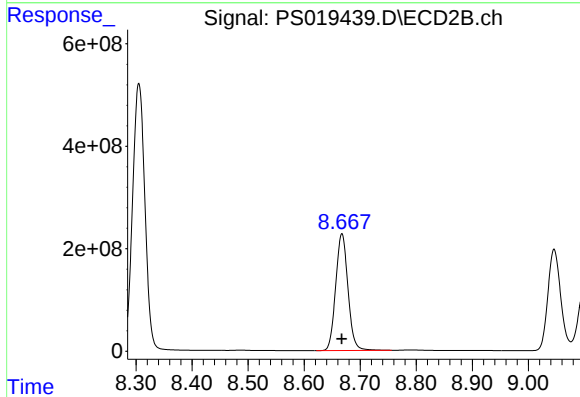


#11 2,4,5-TP (SILVEX)

R.T.: 8.667 min
Delta R.T.: 0.000 min
Response: 3465615471
Conc: 720.12 ng/ml

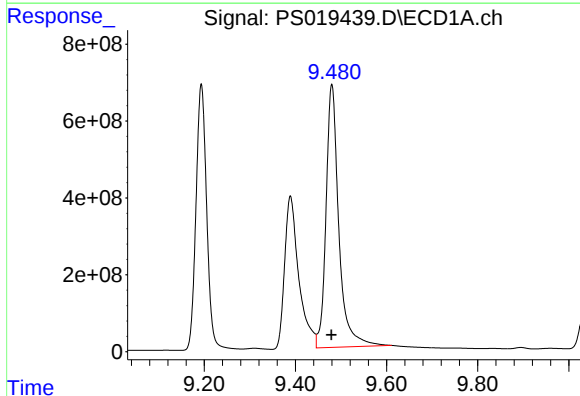


#12 2,4,5-T

R.T.: 9.480 min
Delta R.T.: 0.001 min
Response: 13334785283
Conc: 630.45 ng/ml

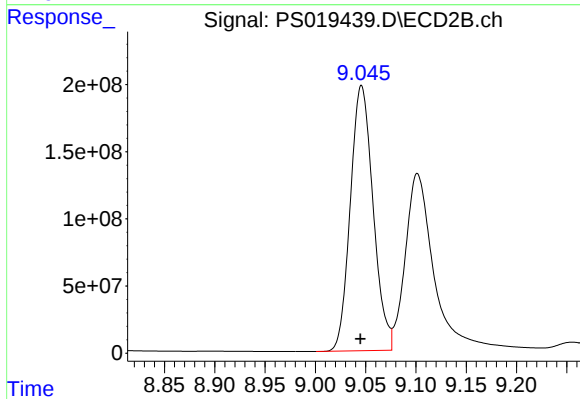

#12 2,4,5-T


R.T.: 9.046 min
Delta R.T.: 0.001 min
Response: 3111855418
Conc: 718.66 ng/ml

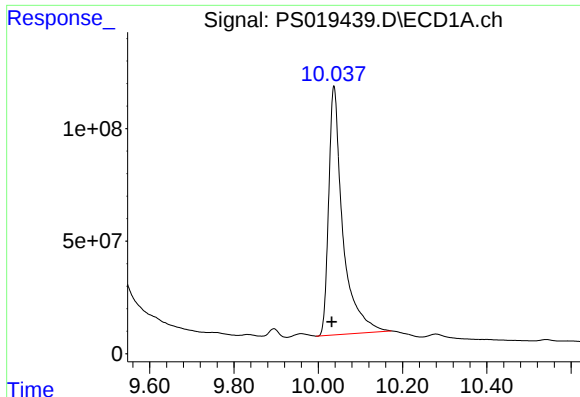

#13 2,4-DB


R.T.: 10.037 min
Delta R.T.: 0.005 min
Response: 2578831011
Conc: 601.37 ng/ml

Instrument :
FID_B
ClientSampleId :

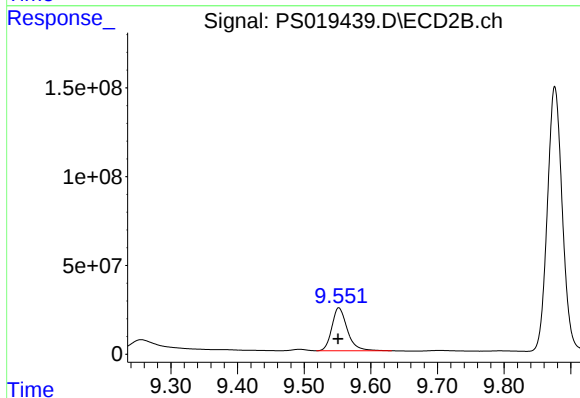


#13 2,4-DB

R.T.: 9.552 min
Delta R.T.: 0.000 min
Response: 388904855
Conc: 684.01 ng/ml

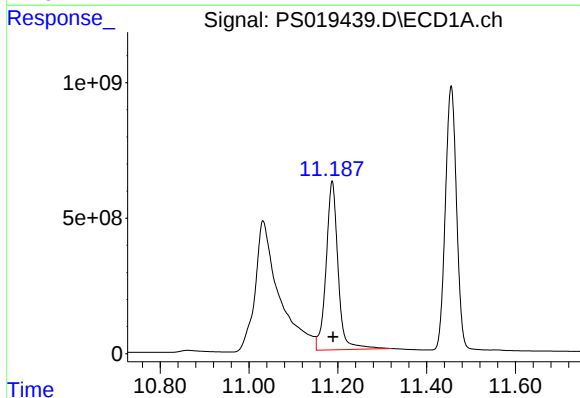


#14 DINOSEB

R.T.: 11.187 min
Delta R.T.: -0.002 min
Response: 11687684197
Conc: 707.86 ng/ml

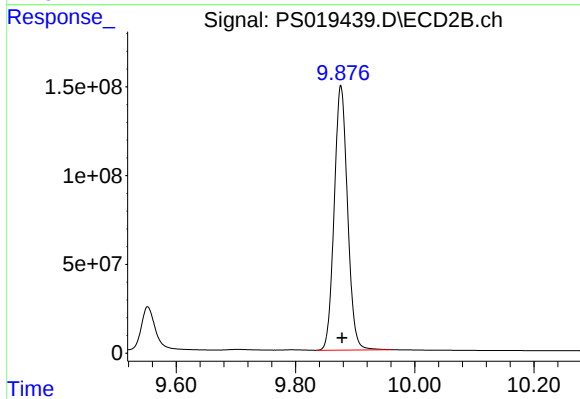

#14 DINOSEB


R.T.: 9.876 min
Delta R.T.: -0.002 min
Response: 2313648963
Conc: 798.39 ng/ml

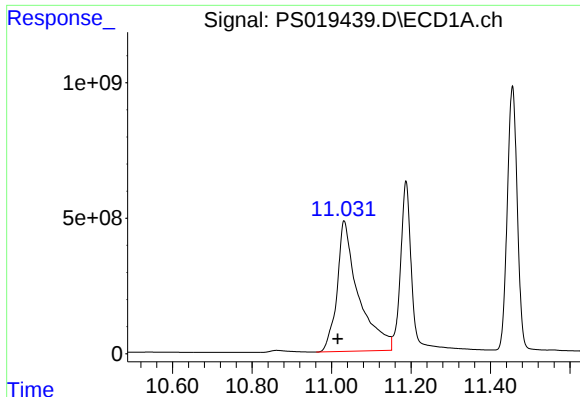

#15 Picloram


R.T.: 11.032 min
Delta R.T.: 0.016 min
Response: 18081625917
Conc: 618.60 ng/ml

Instrument :
FID_B
ClientSampleId :

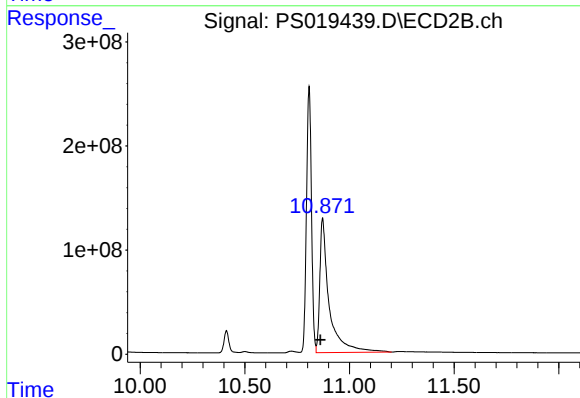


#15 Picloram

R.T.: 10.871 min
Delta R.T.: 0.010 min
Response: 4033663865
Conc: 674.44 ng/ml

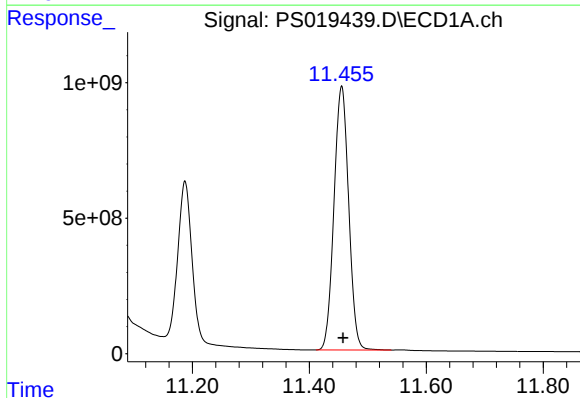

#16 DCPA

R.T.: 11.455 min
Delta R.T.: -0.003 min
Response: 16959105334
Conc: 648.01 ng/ml

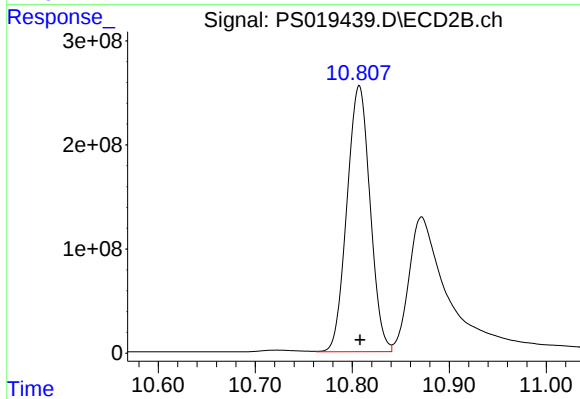

#16 DCPA

R.T.: 10.807 min
Delta R.T.: 0.000 min
Response: 4235031501
Conc: 721.41 ng/ml