

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051820\
 Data File : FB024360.D
 Signal(s) : FID2B.CH
 Acq On : 18 May 2020 9:14
 Operator : DD/AJ
 Sample : BSF0518S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 18 14:41:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
 Quant Title :
 QLast Update : Mon May 11 11:14:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.796	439200	19.890 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.688	897617	30.417 ng/ml
2) t	2,2,4-Trimethylpentane	7.415	982527	32.162 ng/ml
3) t	n-Heptane	7.755	322487	10.645 ng/ml
4) t	Benzene	7.890	385243	10.190 ng/ml
6) t	Toluene	10.627	1103207	30.445 ng/ml
7) t	Ethylbenzene	13.067	349486	10.309 ng/ml
8) t	m-Xylene	13.199	682279	20.675 ng/ml
9) t	O-Xylene	13.927	658869	20.417 ng/ml
10) t	1,2,4-Trimethylbenzene	16.204	547349	20.295 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051820\
Data File : FB024360.D
Signal(s) : FID2B.CH
Acq On : 18 May 2020 9:14
Operator : DD/AJ
Sample : BSF0518S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 18 14:41:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

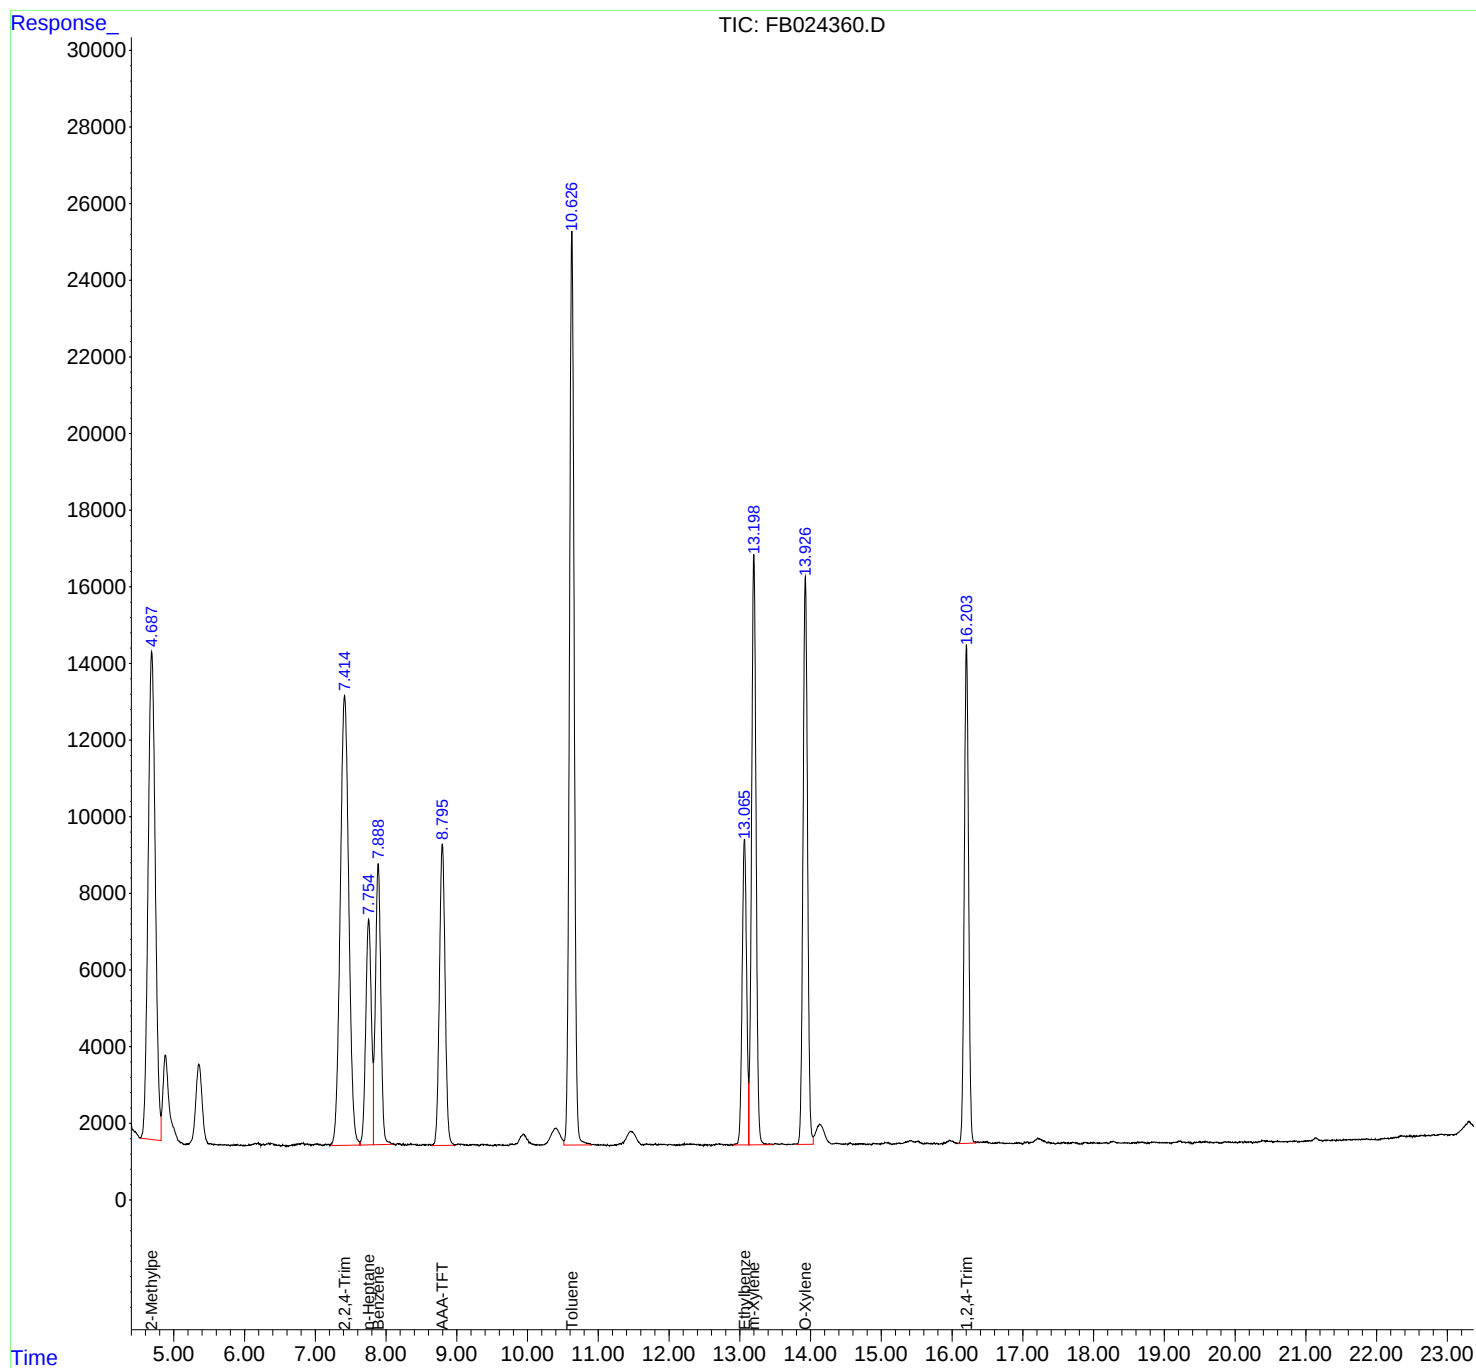

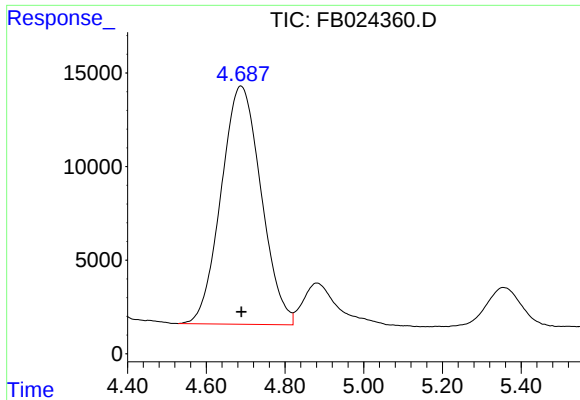


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 897617
Conc: 30.42 ng/ml

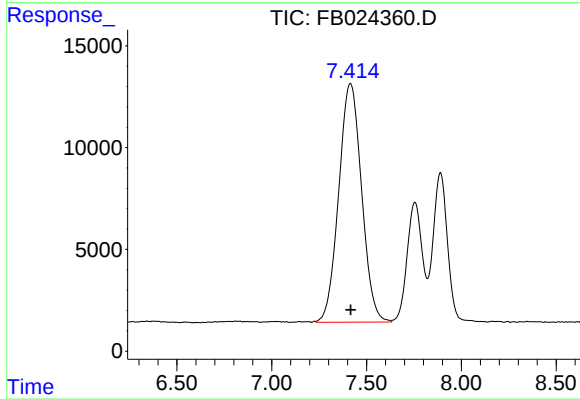


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.002 min
Response: 982527
Conc: 32.16 ng/ml

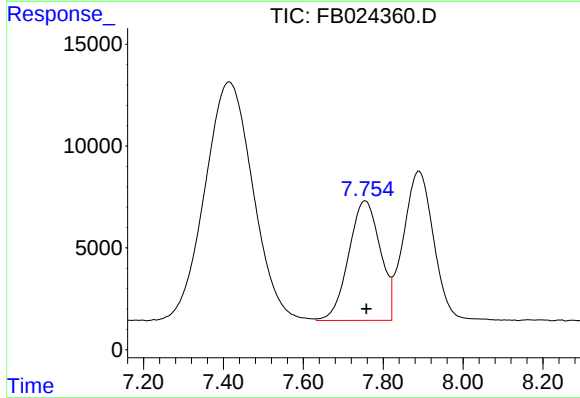


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.002 min
Response: 322487
Conc: 10.64 ng/ml

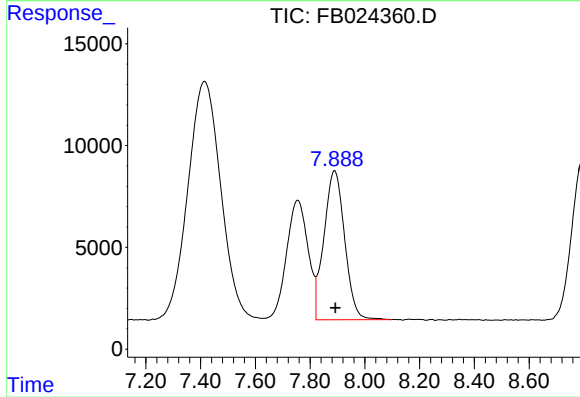


#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.003 min
Response: 385243
Conc: 10.19 ng/ml

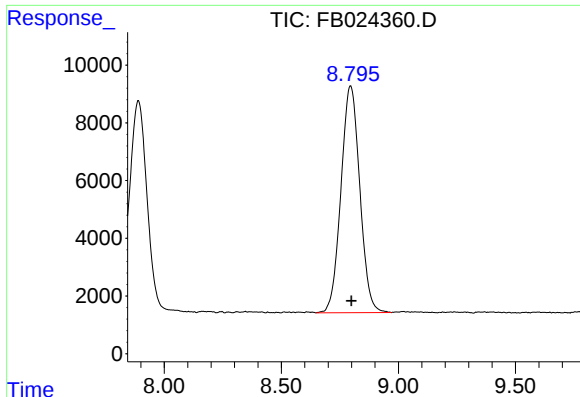


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: -0.003 min
Response: 439200
Conc: 19.89 ng/ml

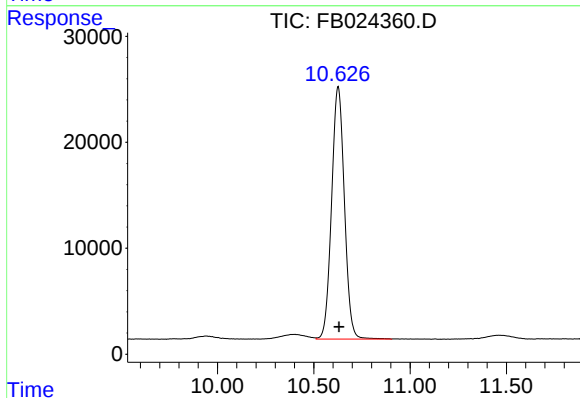


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.004 min
Response: 1103207
Conc: 30.44 ng/ml

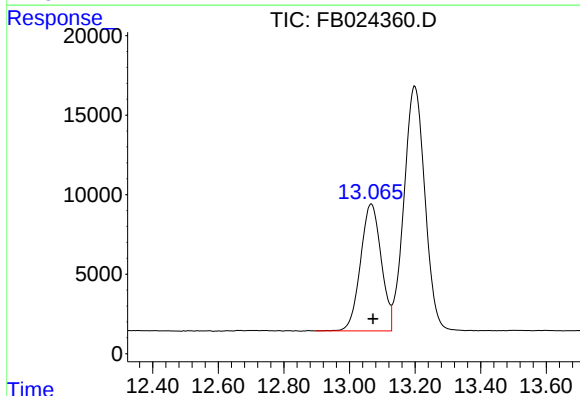


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.005 min
Response: 349486
Conc: 10.31 ng/ml

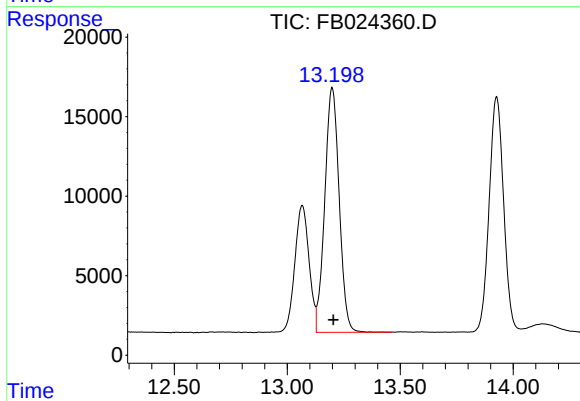


#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: -0.005 min
Response: 682279
Conc: 20.68 ng/ml

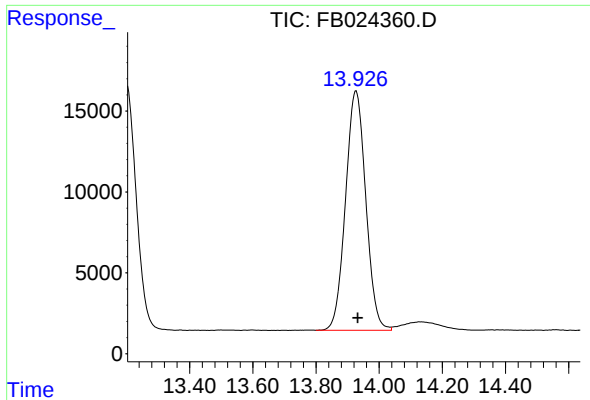

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: -0.005 min
Response: 658869
Conc: 20.42 ng/ml

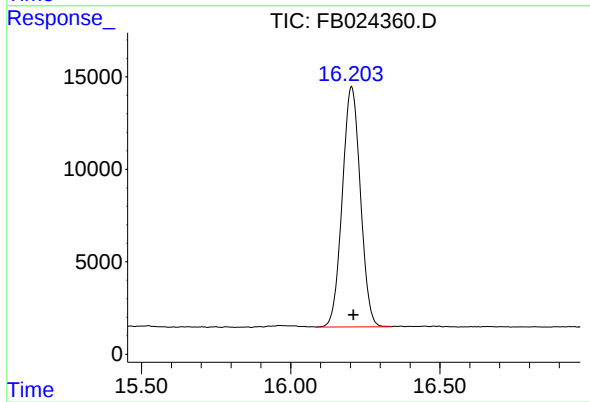

#10 1,2,4-Trimethylbenzene

R.T.: 16.204 min
Delta R.T.: -0.005 min
Response: 547349
Conc: 20.29 ng/ml