

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051820\
 Data File : FB024366.D
 Signal(s) : FID2B.CH
 Acq On : 18 May 2020 12:17
 Operator : DD/AJ
 Sample : L2674-01MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 18 14:42:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
 Quant Title :
 QLast Update : Mon May 11 11:14:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	347989	15.759 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	702579	23.808 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	745708	24.410 ng/ml
3) t n-Heptane	7.755	243035	8.022 ng/ml
4) t Benzene	7.891	325466	8.609 ng/ml
6) t Toluene	10.628	925266	25.534 ng/ml
7) t Ethylbenzene	13.068	291143	8.588 ng/ml
8) t m-Xylene	13.201	576024	17.455 ng/ml
9) t O-Xylene	13.929	572931	17.754 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	481609	17.857 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051820\
Data File : FB024366.D
Signal(s) : FID2B.CH
Acq On : 18 May 2020 12:17
Operator : DD/AJ
Sample : L2674-01MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 18 14:42:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

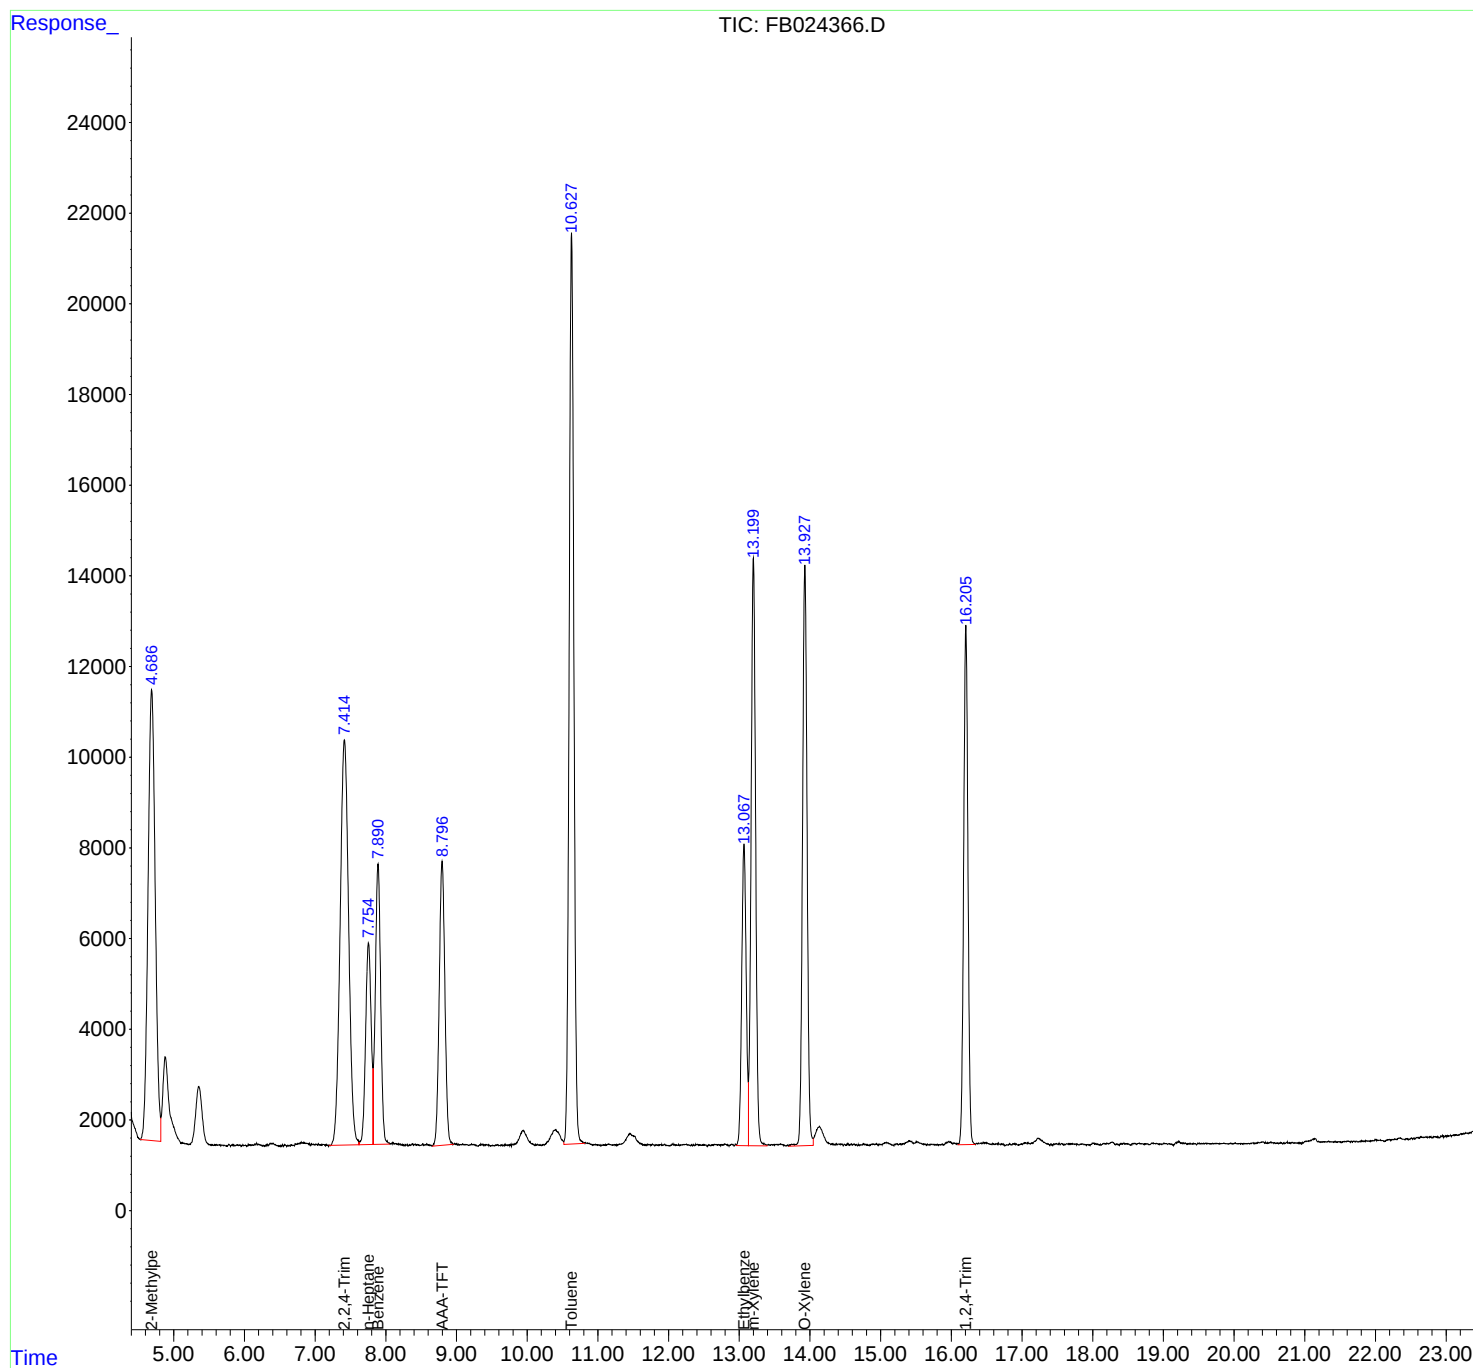

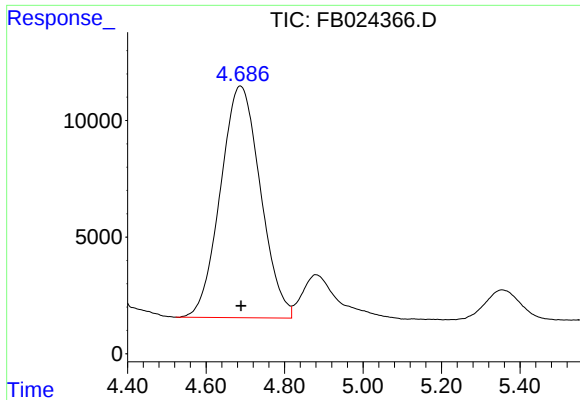


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: -0.001 min
Response: 702579
Conc: 23.81 ng/ml

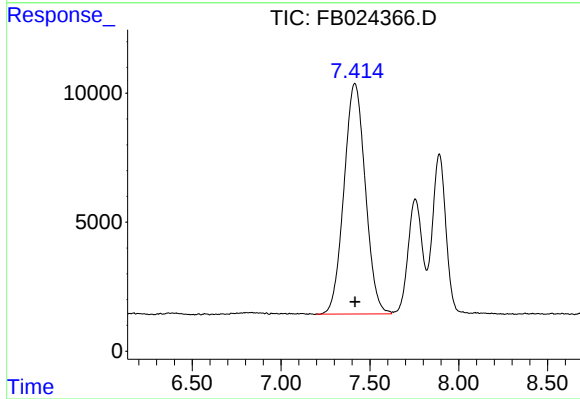


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.002 min
Response: 745708
Conc: 24.41 ng/ml

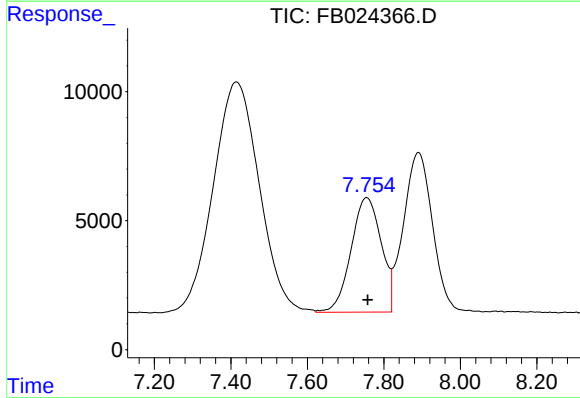


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 243035
Conc: 8.02 ng/ml

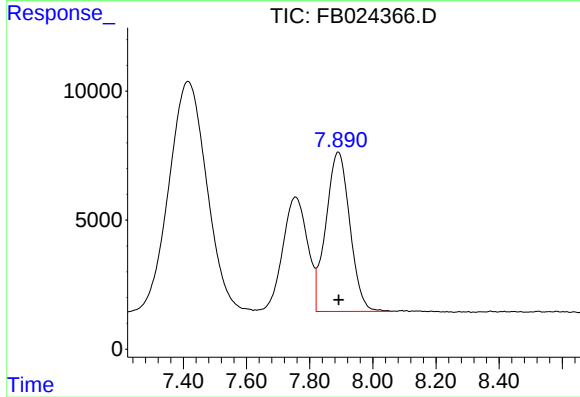


#4 Benzene

R.T.: 7.891 min
Delta R.T.: -0.001 min
Response: 325466
Conc: 8.61 ng/ml

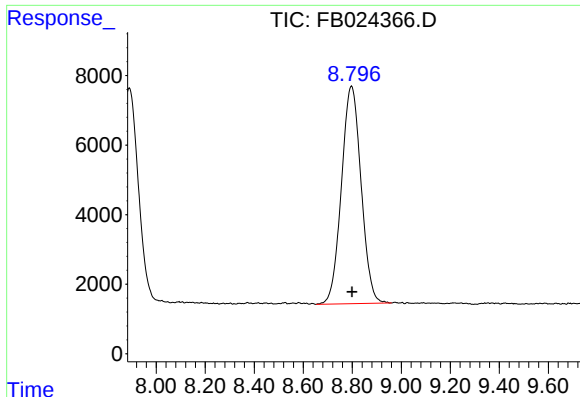


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 347989
Conc: 15.76 ng/ml

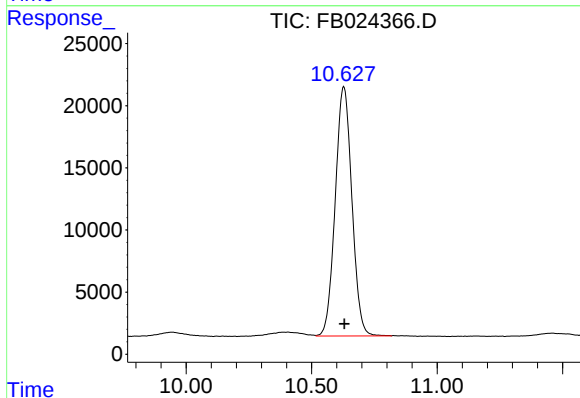


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.002 min
Response: 925266
Conc: 25.53 ng/ml

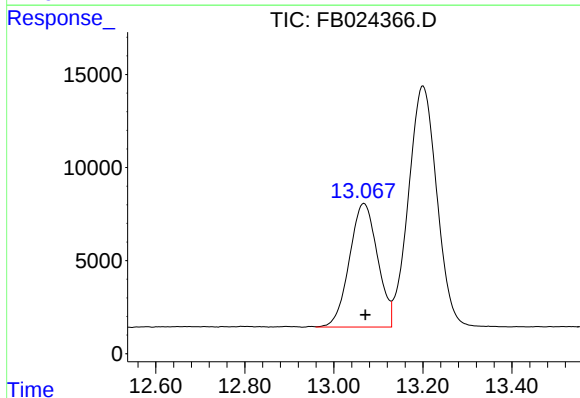


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.003 min
Response: 291143
Conc: 8.59 ng/ml

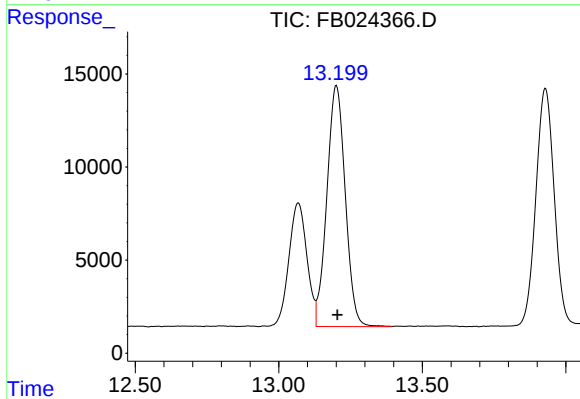


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.004 min
Response: 576024
Conc: 17.46 ng/ml

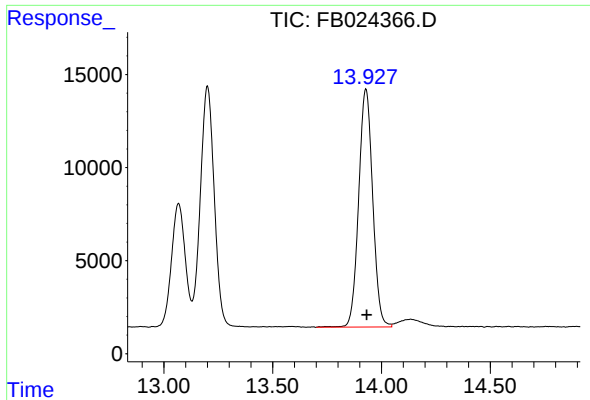

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.003 min
Response: 572931
Conc: 17.75 ng/ml

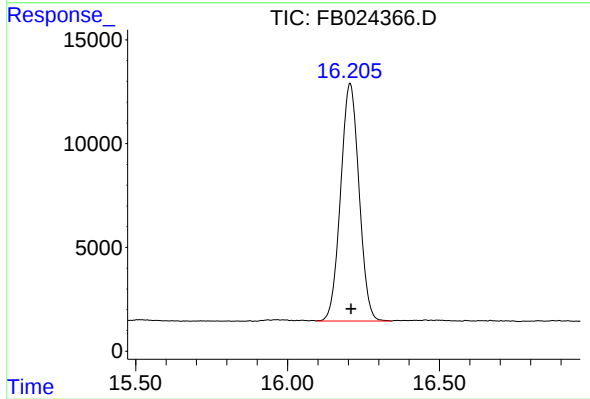

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.003 min
Response: 481609
Conc: 17.86 ng/ml