

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051820\
 Data File : FB024370.D
 Signal(s) : FID2B.CH
 Acq On : 18 May 2020 16:12
 Operator : DD/AJ
 Sample : L2182-03
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 19 01:04:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
 Quant Title :
 QLast Update : Mon May 11 11:14:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.797	424259	19.213 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.692	48401	1.640 ng/ml
2) t	2,2,4-Trimethylpentane	7.410	47199	1.545 ng/ml
3) t	n-Heptane	7.758	15007	0.495 ng/ml
4) t	Benzene	7.890	17731	0.469 ng/ml
6) t	Toluene	10.628	62413	1.722 ng/ml
7) t	Ethylbenzene	13.066	20650	0.609 ng/ml
8) t	m-Xylene	13.200	39502	1.197 ng/ml
9) t	O-Xylene	13.930	37433	1.160 ng/ml
10) t	1,2,4-Trimethylbenzene	16.208	32014	1.187 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051820\
Data File : FB024370.D
Signal(s) : FID2B.CH
Acq On : 18 May 2020 16:12
Operator : DD/AJ
Sample : L2182-03
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 19 01:04:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

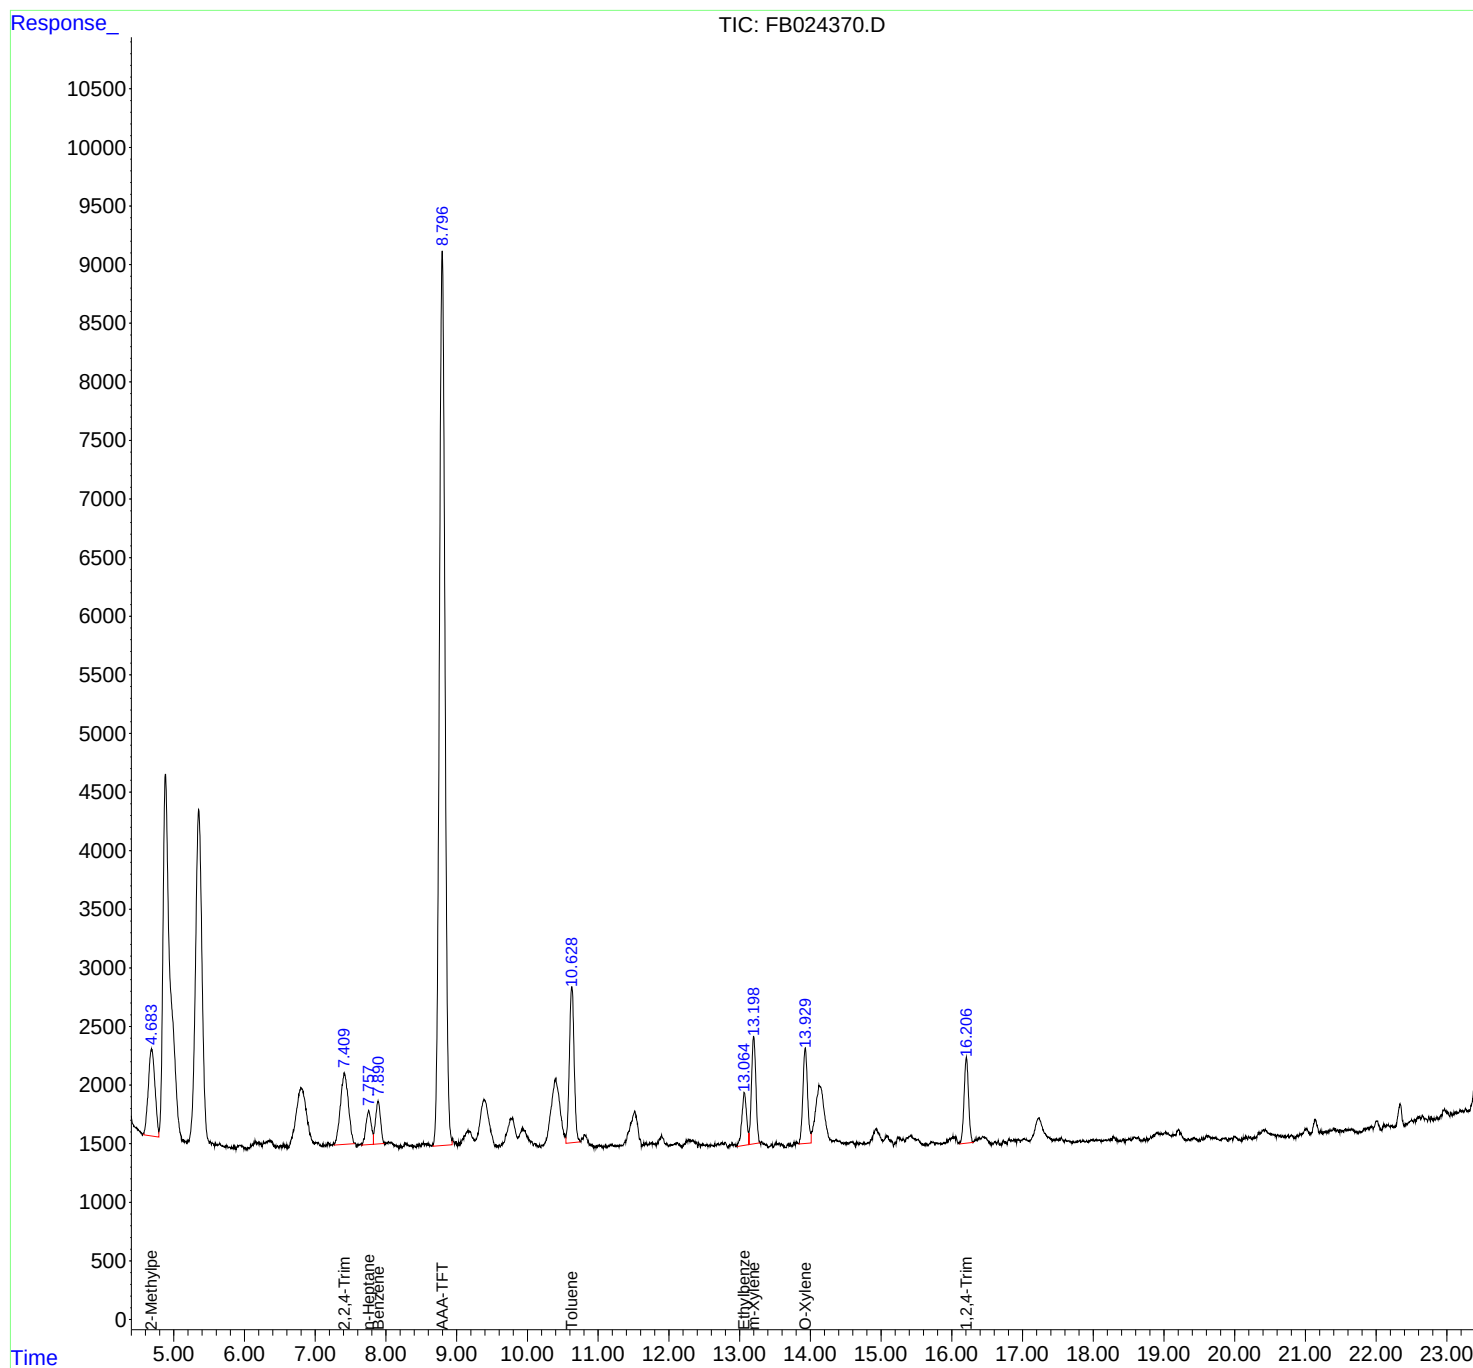

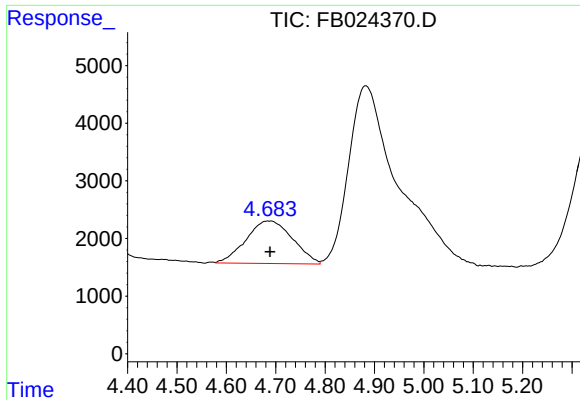


#1 2-Methylpentane

R.T.: 4.692 min
Delta R.T.: 0.003 min
Response: 48401
Conc: 1.64 ng/ml

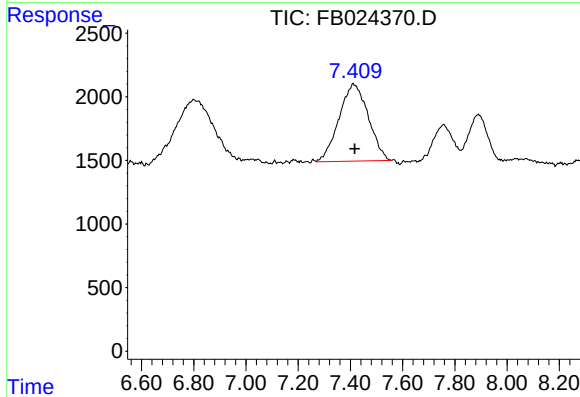


#2 2,2,4-Trimethylpentane

R.T.: 7.410 min
Delta R.T.: -0.007 min
Response: 47199
Conc: 1.55 ng/ml

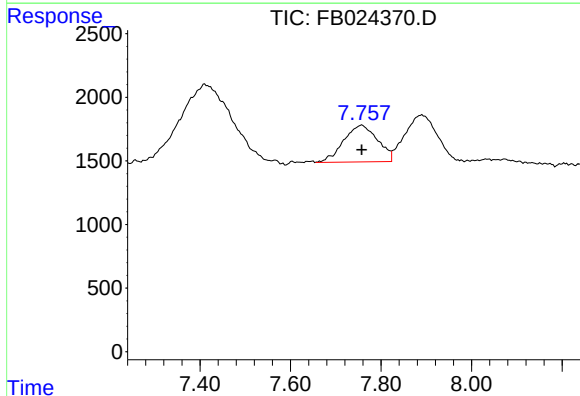


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 15007
Conc: 0.50 ng/ml

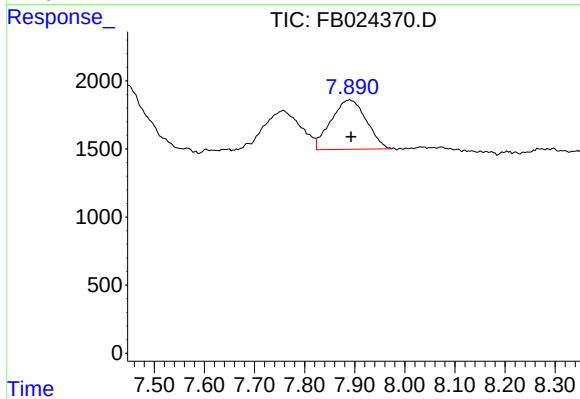


#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.002 min
Response: 17731
Conc: 0.47 ng/ml

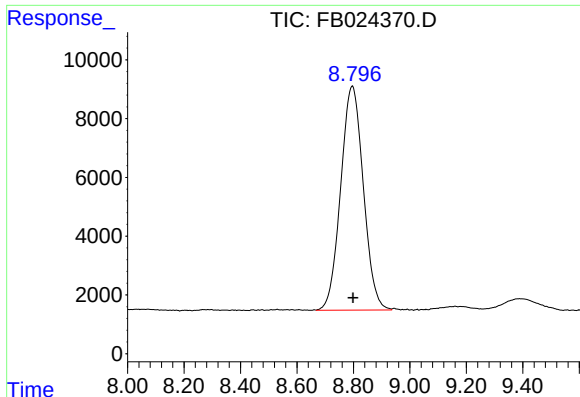


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 424259
Conc: 19.21 ng/ml

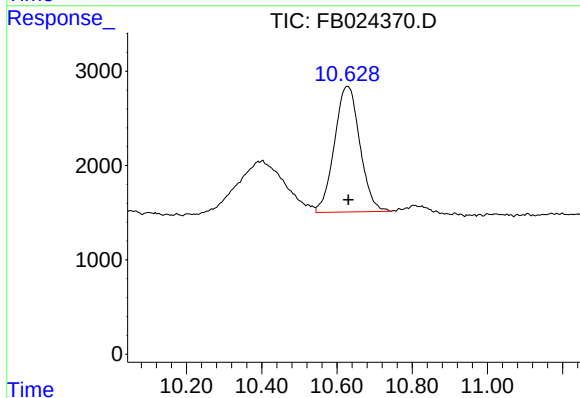


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.002 min
Response: 62413
Conc: 1.72 ng/ml

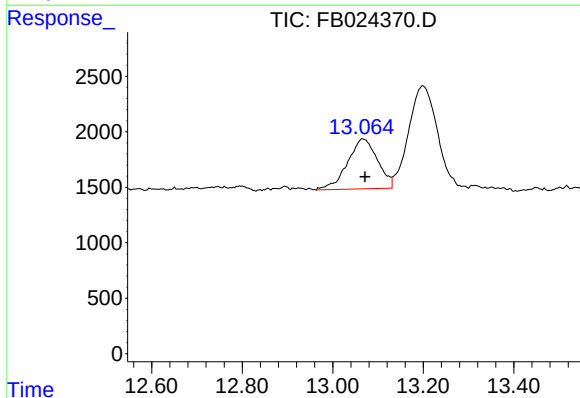


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: -0.005 min
Response: 20650
Conc: 0.61 ng/ml

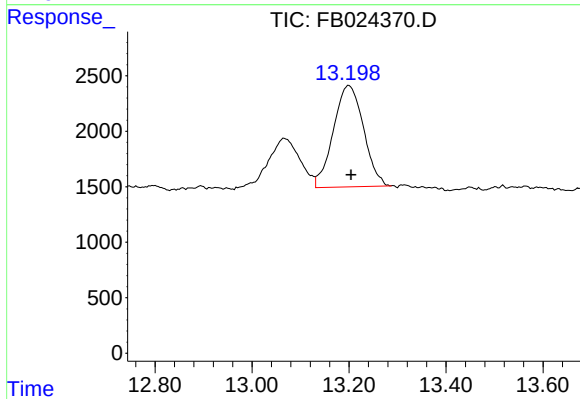


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.005 min
Response: 39502
Conc: 1.20 ng/ml

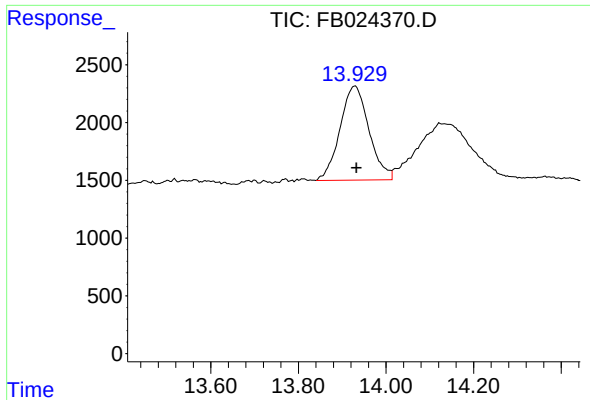

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.002 min
Response: 37433
Conc: 1.16 ng/ml

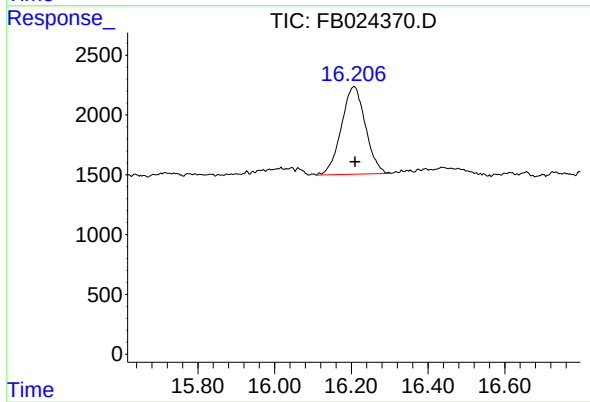

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.002 min
Response: 32014
Conc: 1.19 ng/ml