

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051822\
 Data File : FB027270.D
 Signal(s) : FID2B.CH
 Acq On : 18 May 2022 11:35
 Operator : AJ/MA
 Sample : BSF0518S1
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: May 18 23:44:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
 Quant Title :
 QLast Update : Tue May 10 13:42:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	227919	21.712 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	405220	25.464 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	425811	26.392 ng/ml
3) t n-Heptane	7.747	144000	8.812 ng/ml
4) t Benzene	7.884	171463	9.246 ng/ml
6) t Toluene	10.617	491640	27.691 ng/ml
7) t Ethylbenzene	13.053	151823	9.194 ng/ml
8) t m-Xylene	13.186	300163	18.242 ng/ml
9) t O-Xylene	13.913	294358	17.946 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	298237	17.864 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051822\
Data File : FB027270.D
Signal(s) : FID2B.CH
Acq On : 18 May 2022 11:35
Operator : AJ/MA
Sample : BSF0518S1
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 18 23:44:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
Quant Title :
QLast Update : Tue May 10 13:42:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

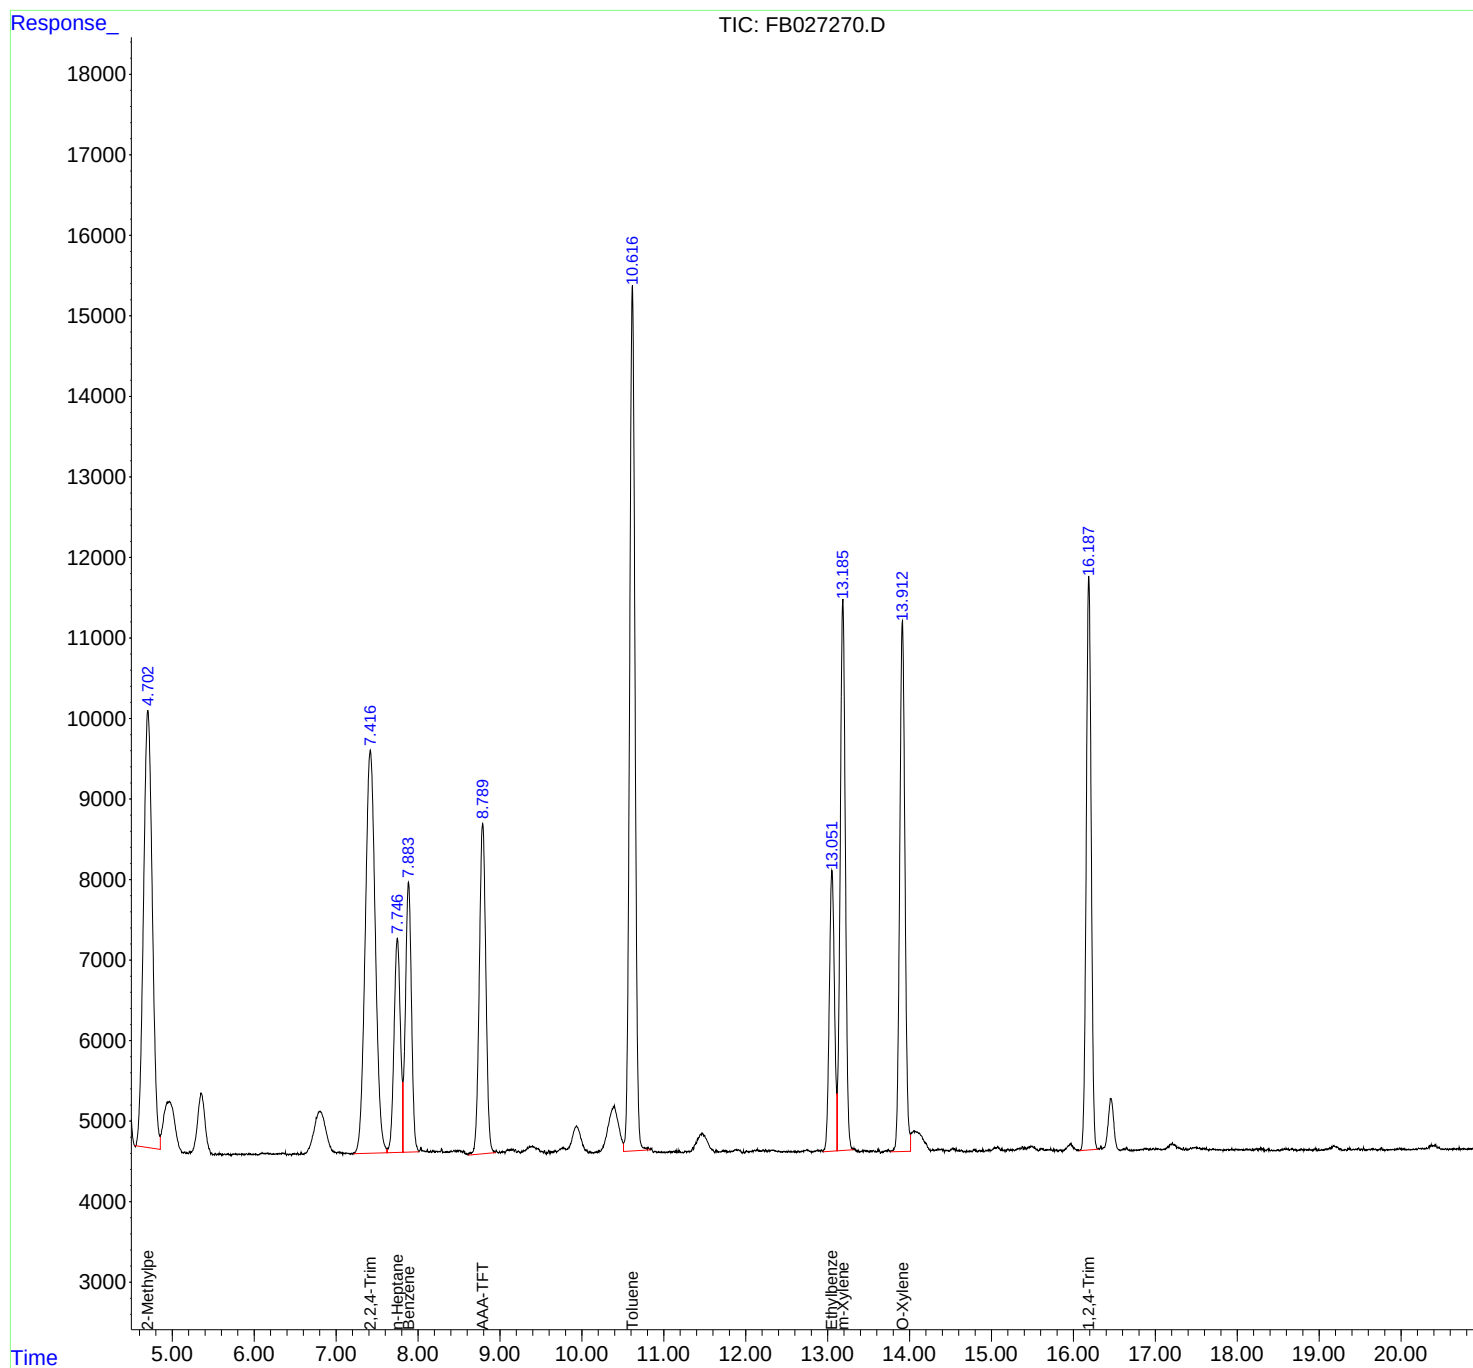


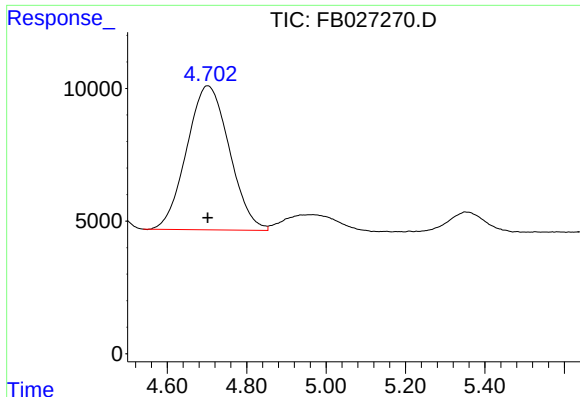

#1 2-Methylpentane


R.T.: 4.702 min
Delta R.T.: 0.000 min
Response: 405220
Conc: 25.46 ng/ml

Instrument :
FID_B
ClientSampleId :

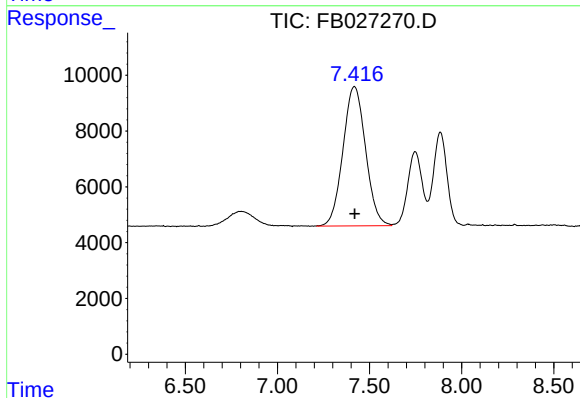


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: -0.002 min
Response: 425811
Conc: 26.39 ng/ml

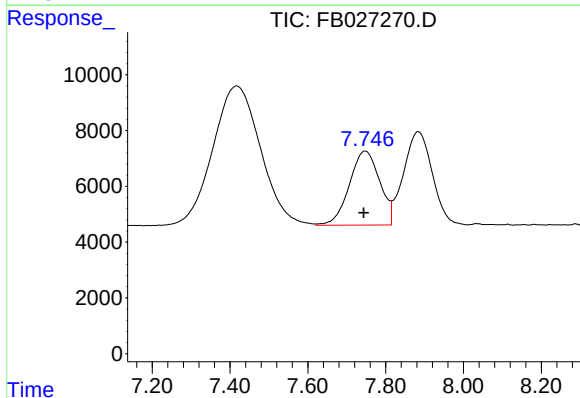


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: 0.004 min
Response: 144000
Conc: 8.81 ng/ml

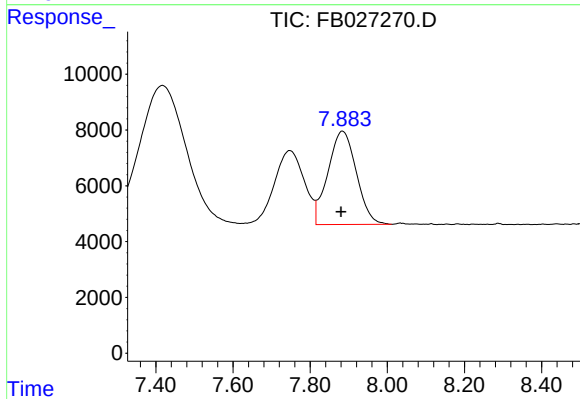

#4 Benzene


R.T.: 7.884 min
Delta R.T.: 0.004 min
Response: 171463
Conc: 9.25 ng/ml

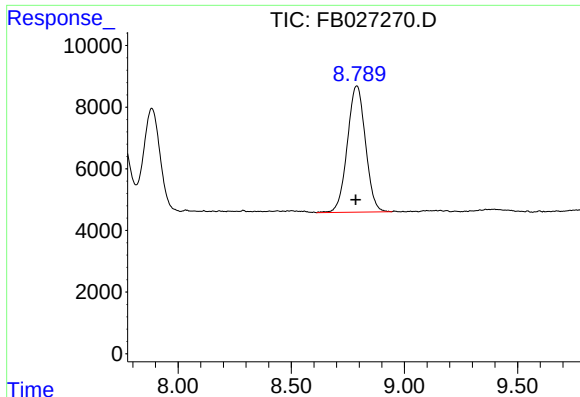

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: 0.005 min
Response: 227919
Conc: 21.71 ng/ml

Instrument :
FID_B
ClientSampleId :

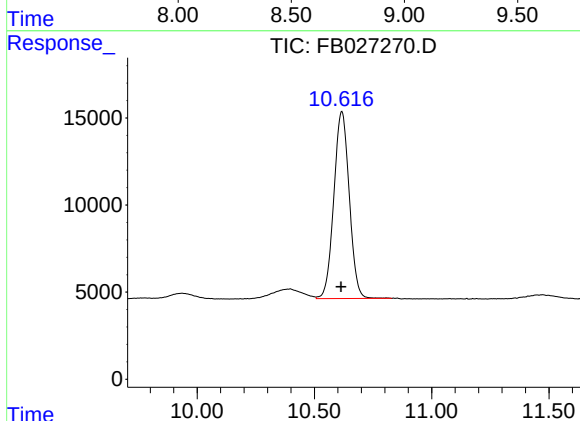


#6 Toluene

R.T.: 10.617 min
Delta R.T.: 0.004 min
Response: 491640
Conc: 27.69 ng/ml

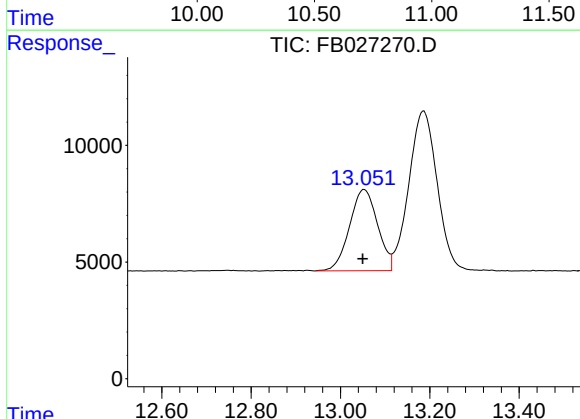


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: 0.003 min
Response: 151823
Conc: 9.19 ng/ml

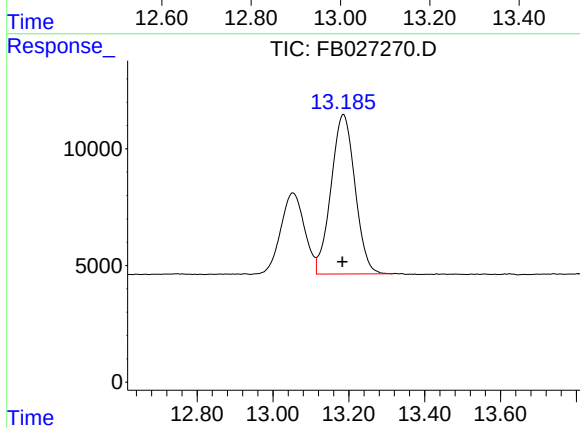

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: 0.003 min
Response: 300163
Conc: 18.24 ng/ml

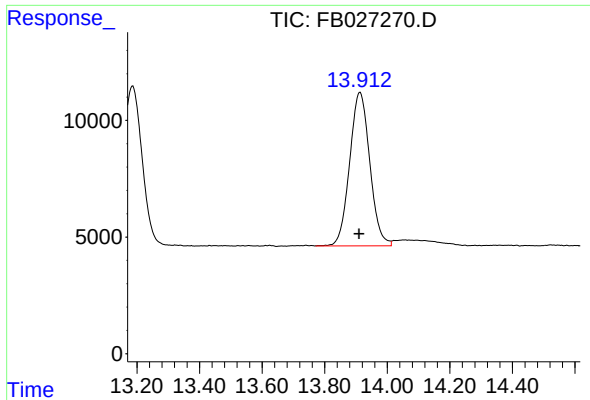

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: 0.003 min
Response: 294358
Conc: 17.95 ng/ml

Instrument :
FID_B
ClientSampleId :

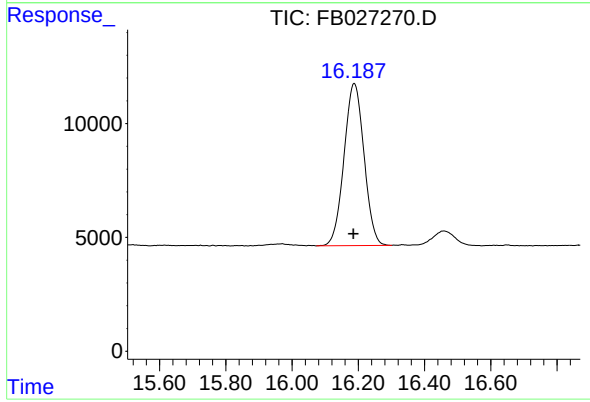

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: 0.003 min
Response: 298237
Conc: 17.86 ng/ml