

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB051822\  
 Data File : FB027276.D  
 Signal(s) : FID2B.CH  
 Acq On : 18 May 2022 15:14  
 Operator : AJ/MA  
 Sample : N2824-02  
 Misc : 5.05G/5.00 ML DI WATER  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :

Integration File: Calibration.e  
 Quant Time: May 18 23:44:42 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB051022.M  
 Quant Title :  
 QLast Update : Tue May 10 13:42:12 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.792  | 182956   | 17.429 ng/ml |
| Target Compounds             |        |          |              |
| 6) t Toluene                 | 10.631 | 5539     | 0.312 ng/ml  |
| 9) t O-Xylene                | 13.921 | 25996    | 1.585 ng/ml  |
| 10) t 1,2,4-Trimethylbenzene | 16.150 | 14430    | 0.864 ng/ml  |
| -----                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB051822\  
Data File : FB027276.D  
Signal(s) : FID2B.CH  
Acq On : 18 May 2022 15:14  
Operator : AJ/MA  
Sample : N2824-02  
Misc : 5.05G/5.00 ML DI WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: May 18 23:44:42 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB051022.M  
Quant Title :  
QLast Update : Tue May 10 13:42:12 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

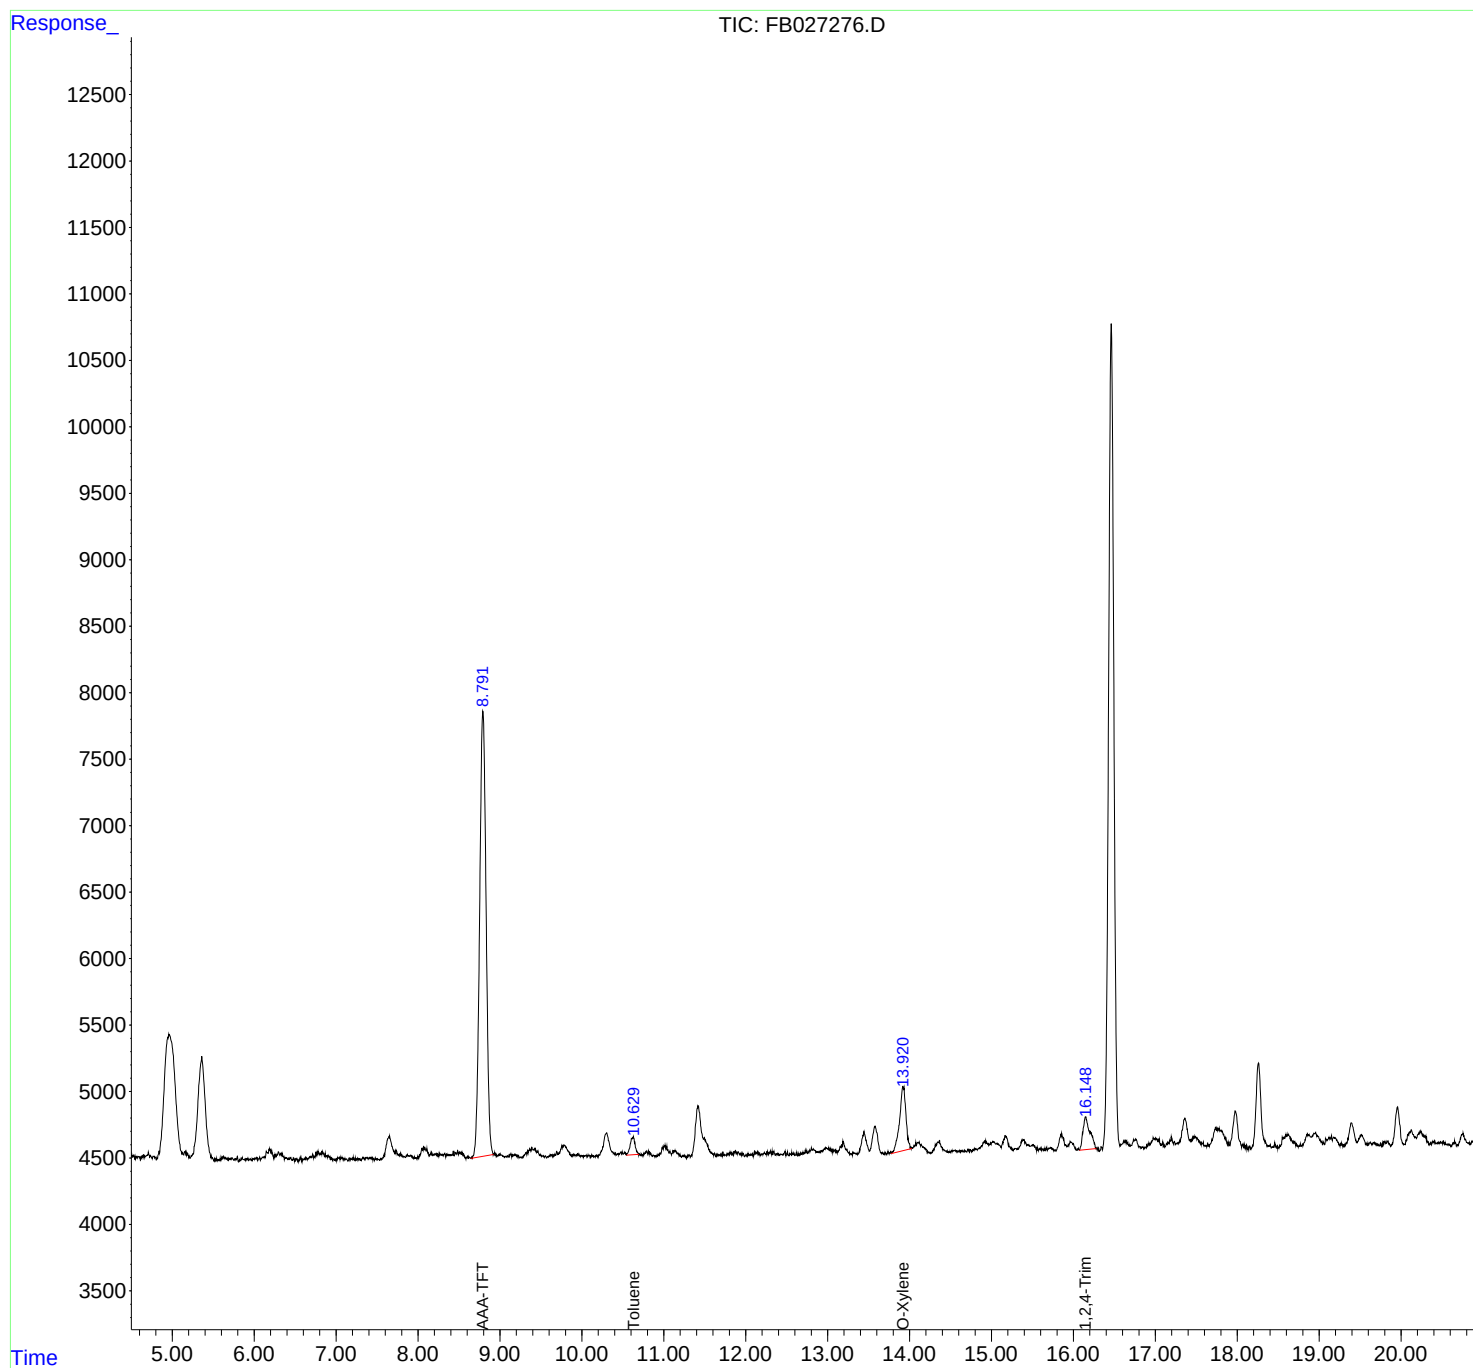


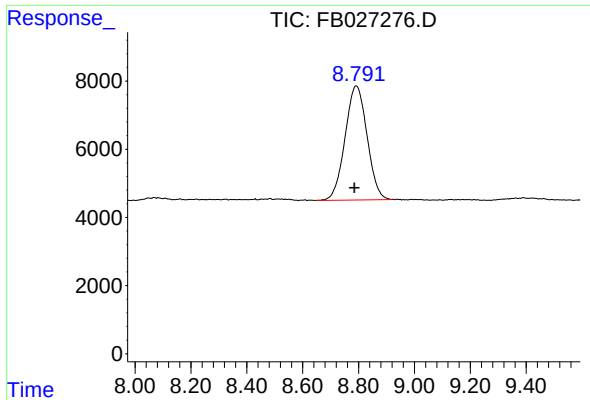

#5 AAA-TFT


R.T.: 8.792 min  
Delta R.T.: 0.007 min  
Response: 182956  
Conc: 17.43 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

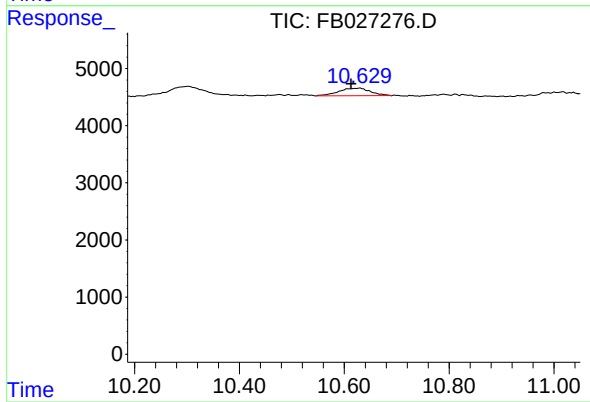


#6 Toluene

R.T.: 10.631 min  
Delta R.T.: 0.018 min  
Response: 5539  
Conc: 0.31 ng/ml

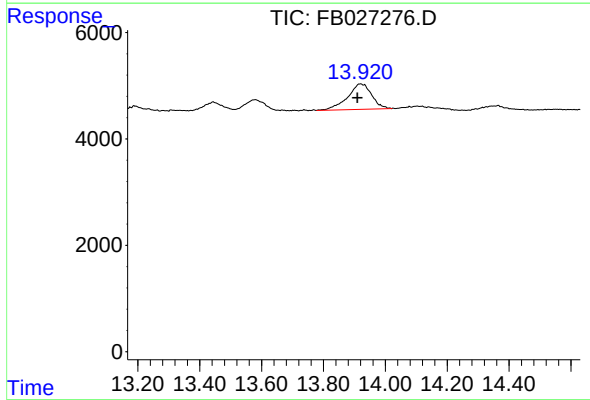

#9 O-Xylene

R.T.: 13.921 min  
Delta R.T.: 0.011 min  
Response: 25996  
Conc: 1.58 ng/ml

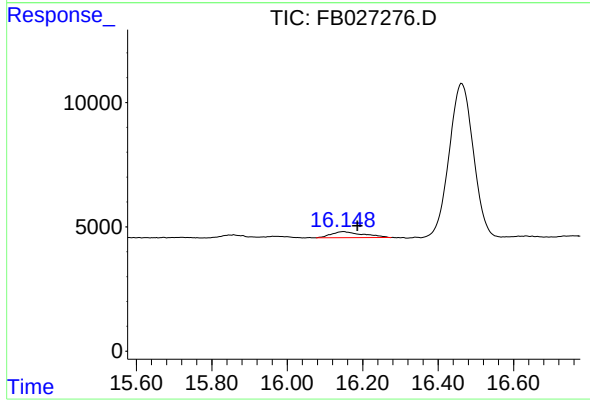

#10 1,2,4-Trimethylbenzene

R.T.: 16.150 min  
Delta R.T.: -0.035 min  
Response: 14430  
Conc: 0.86 ng/ml