

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051822\
Data File : FB027282.D
Signal(s) : FID2B.CH
Acq On : 18 May 2022 19:29
Operator : AJ/MA
Sample : N2685-06
Misc : 5.08G/5.00 ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 18 23:45:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
Quant Title :
QLast Update : Tue May 10 13:42:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.843	15633	1.489 ng/ml
Target Compounds			
7) t Ethylbenzene	13.018	298465	18.074 ng/ml
9) t O-Xylene	13.937	50115	3.055 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051822\
Data File : FB027282.D
Signal(s) : FID2B.CH
Acq On : 18 May 2022 19:29
Operator : AJ/MA
Sample : N2685-06
Misc : 5.08G/5.00 ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 18 23:45:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
Quant Title :
QLast Update : Tue May 10 13:42:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

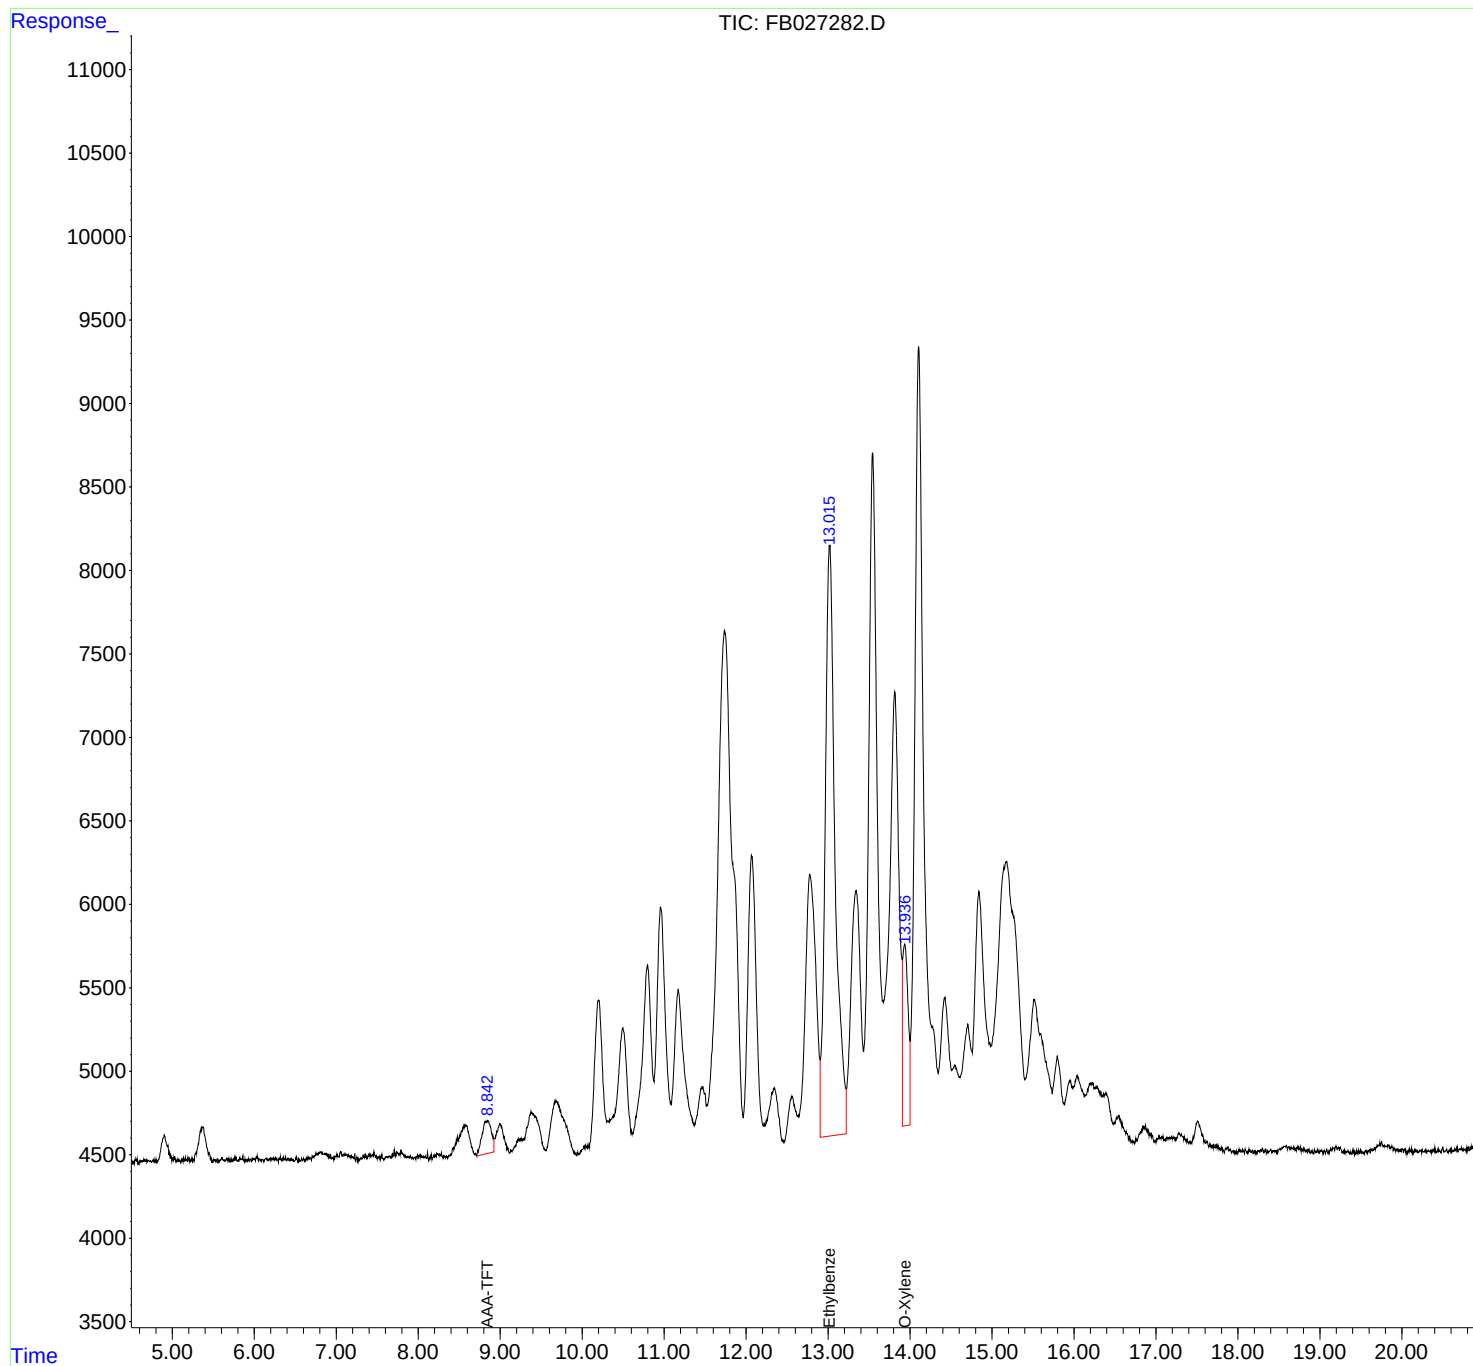


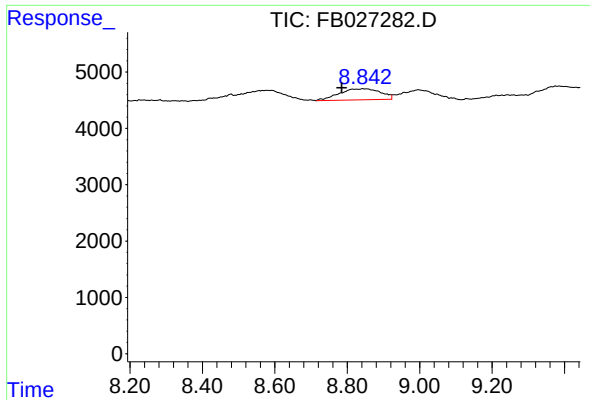

#5 AAA-TFT


R.T.: 8.843 min
Delta R.T.: 0.058 min
Response: 15633
Conc: 1.49 ng/ml

Instrument :
FID_B
ClientSampleId :

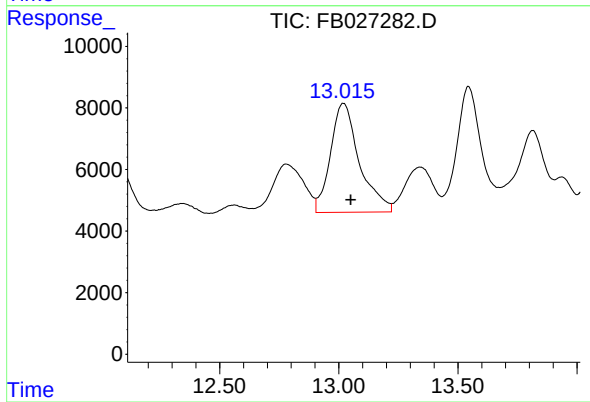

#7 Ethylbenzene

R.T.: 13.018 min
Delta R.T.: -0.033 min
Response: 298465
Conc: 18.07 ng/ml

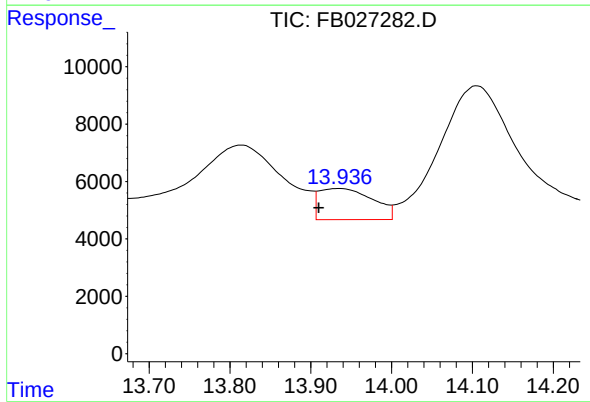

#9 O-Xylene

R.T.: 13.937 min
Delta R.T.: 0.027 min
Response: 50115
Conc: 3.06 ng/ml