

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051822\
 Data File : FB027284.D
 Signal(s) : FID2B.CH
 Acq On : 18 May 2022 20:42
 Operator : AJ/MA
 Sample : BSF0518S3
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0518S3

Integration File: Calibration.e
 Quant Time: May 18 23:45:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
 Quant Title :
 QLast Update : Tue May 10 13:42:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	236400	22.520 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	476586	29.948 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	523381	32.440 ng/ml
3) t n-Heptane	7.751	159132	9.738 ng/ml
4) t Benzene	7.888	205267	11.069 ng/ml
6) t Toluene	10.621	574034	32.332 ng/ml
7) t Ethylbenzene	13.057	167087	10.118 ng/ml
8) t m-Xylene	13.190	346604	21.065 ng/ml
9) t O-Xylene	13.918	388498	23.685 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	387087	23.186 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051822\
Data File : FB027284.D
Signal(s) : FID2B.CH
Acq On : 18 May 2022 20:42
Operator : AJ/MA
Sample : BSF0518S3
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0518S3

Integration File: Calibration.e
Quant Time: May 18 23:45:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
Quant Title :
QLast Update : Tue May 10 13:42:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

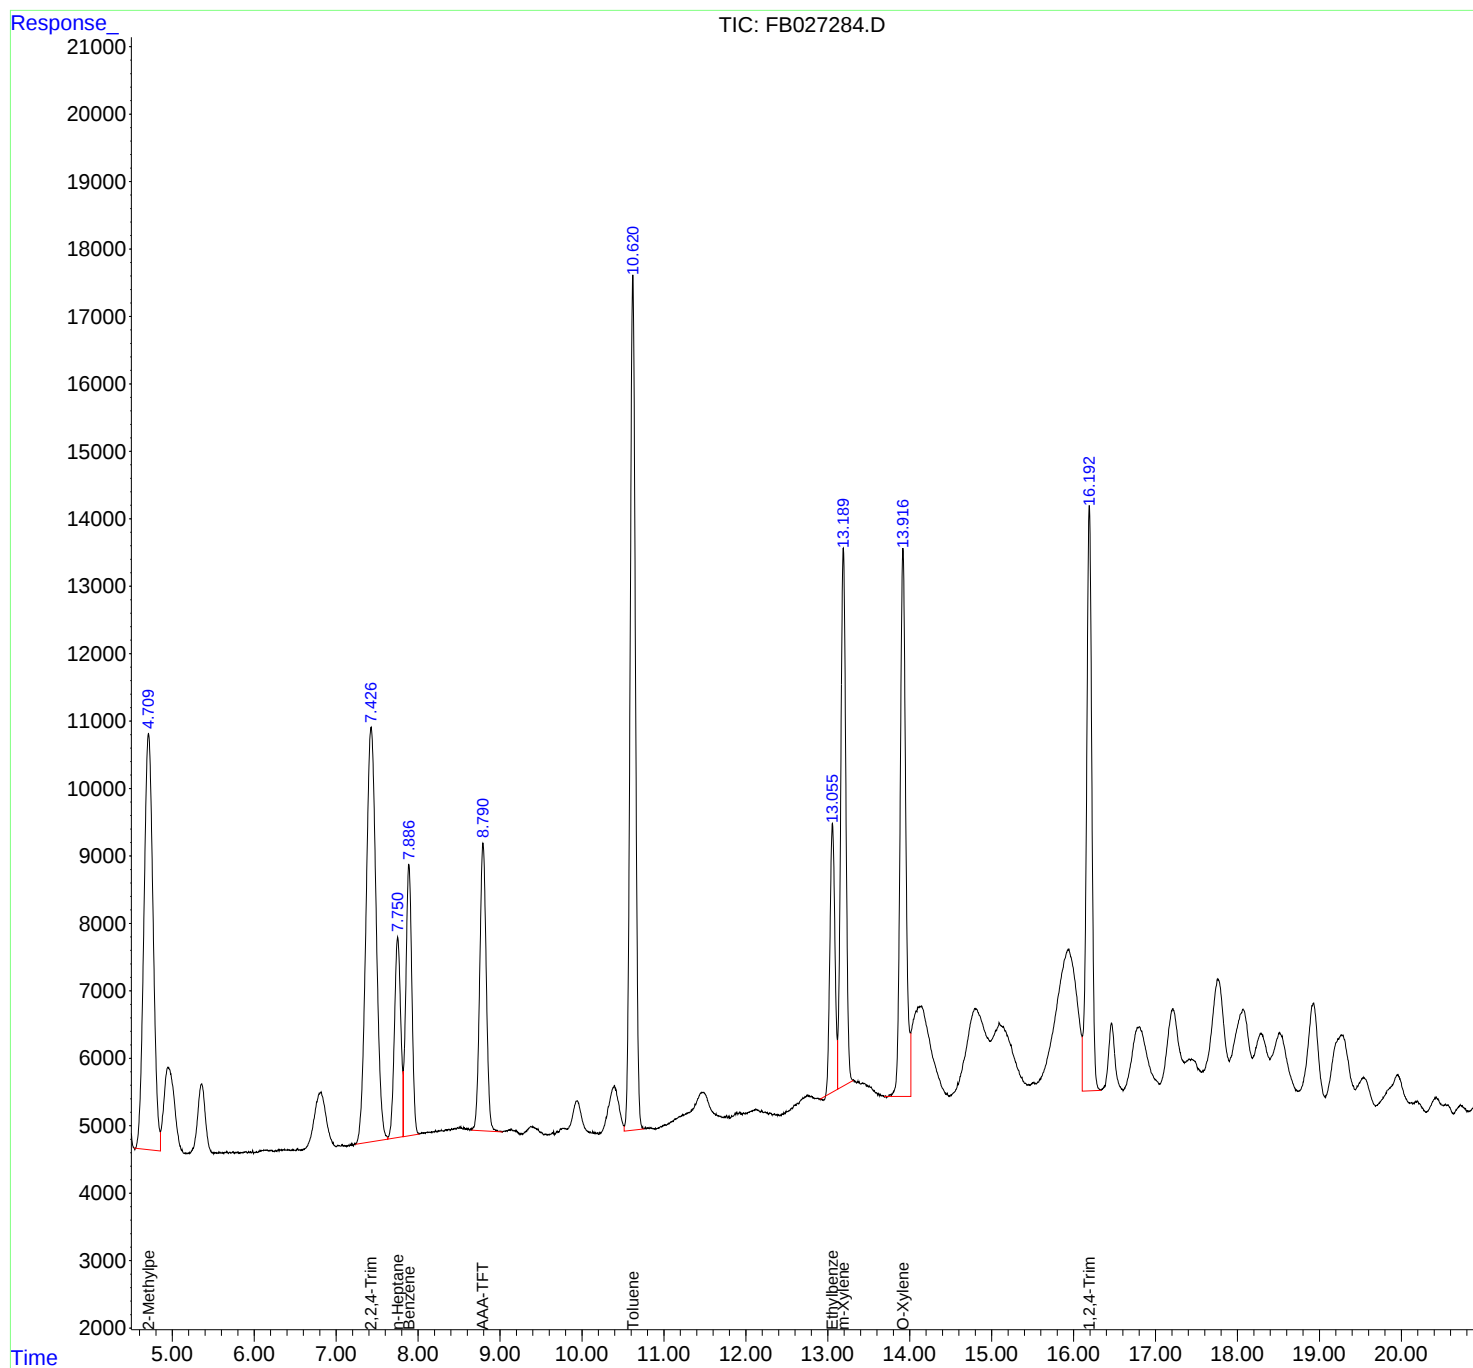


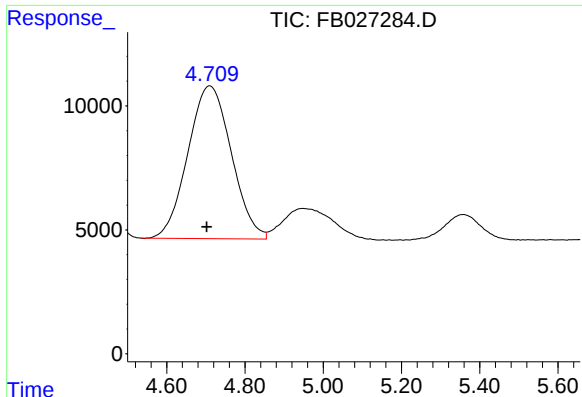

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: 0.008 min
Response: 476586
Conc: 29.95 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0518S3

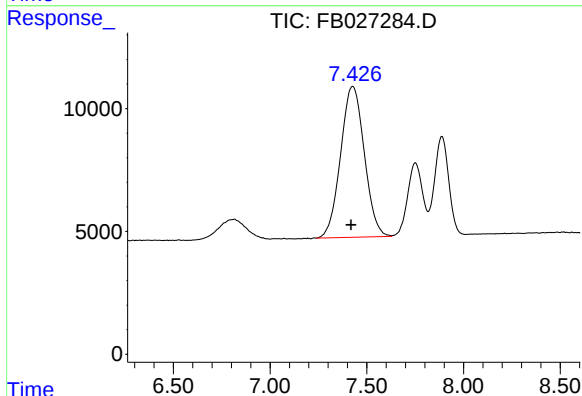


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: 0.008 min
Response: 523381
Conc: 32.44 ng/ml

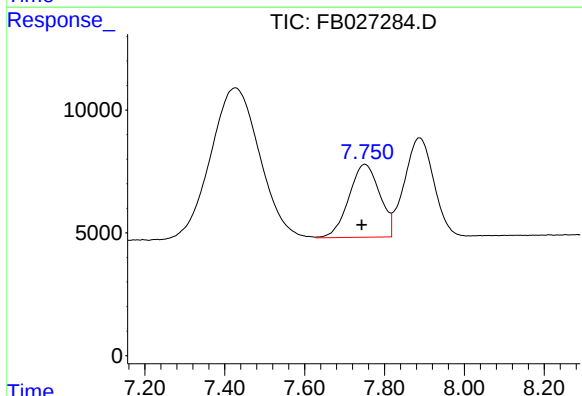


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.008 min
Response: 159132
Conc: 9.74 ng/ml

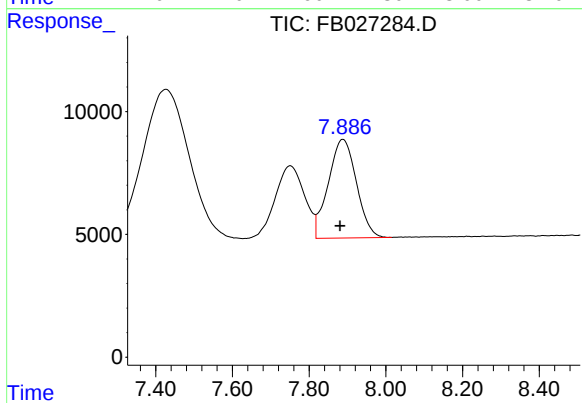

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.008 min
Response: 205267
Conc: 11.07 ng/ml

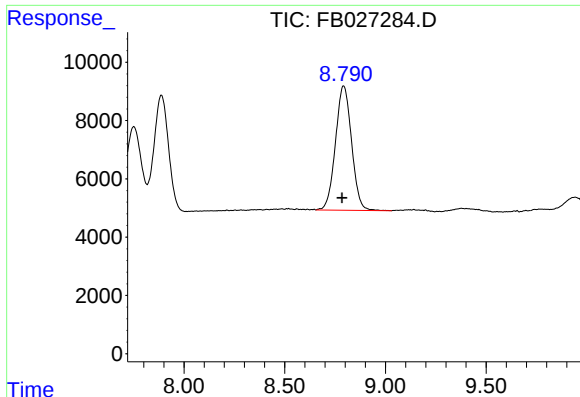

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.007 min
Response: 236400
Conc: 22.52 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0518S3

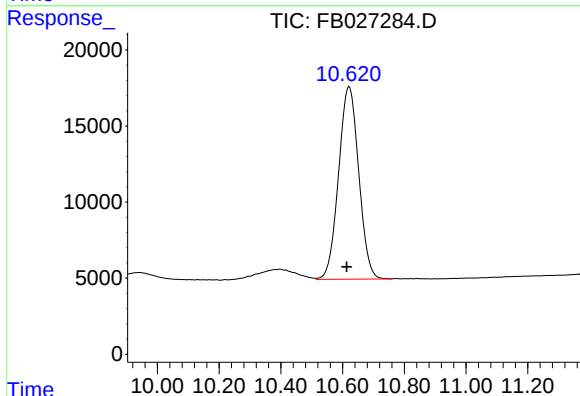


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.008 min
Response: 574034
Conc: 32.33 ng/ml

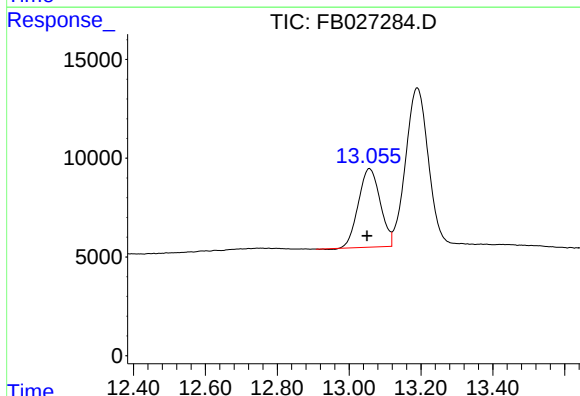


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.007 min
Response: 167087
Conc: 10.12 ng/ml

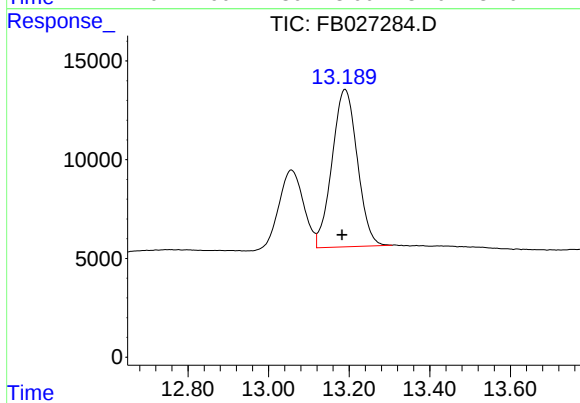

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.007 min
Response: 346604
Conc: 21.06 ng/ml

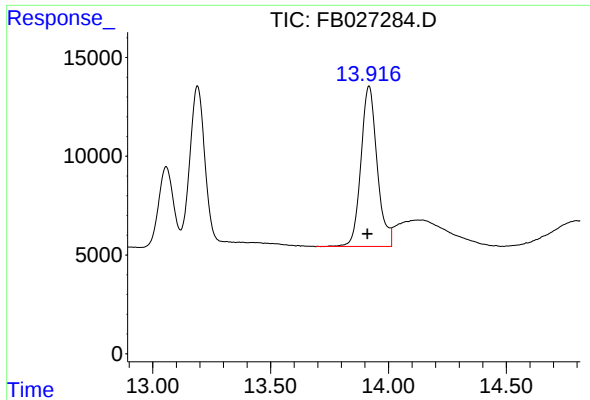

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.008 min
Response: 388498
Conc: 23.68 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0518S3

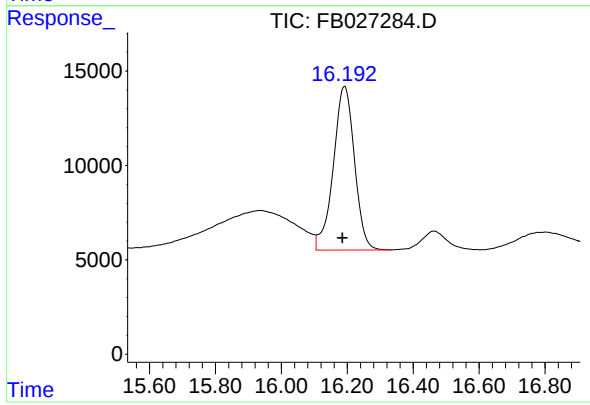

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.006 min
Response: 387087
Conc: 23.19 ng/ml