

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052019\
Data File : FB021119.D
Signal(s) : FID2B.CH
Acq On : 20 May 2019 20:25
Operator : MJ/SJ
Sample : K2951-08
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 21 08:55:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
Quant Title :
QLast Update : Mon Apr 29 15:53:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.997	301415	16.802 ng/ml
Target Compounds			
9) t O-Xylene	14.188	300	0.010 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052019\
Data File : FB021119.D
Signal(s) : FID2B.CH
Acq On : 20 May 2019 20:25
Operator : MJ/SJ
Sample : K2951-08
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 21 08:55:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
Quant Title :
QLast Update : Mon Apr 29 15:53:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

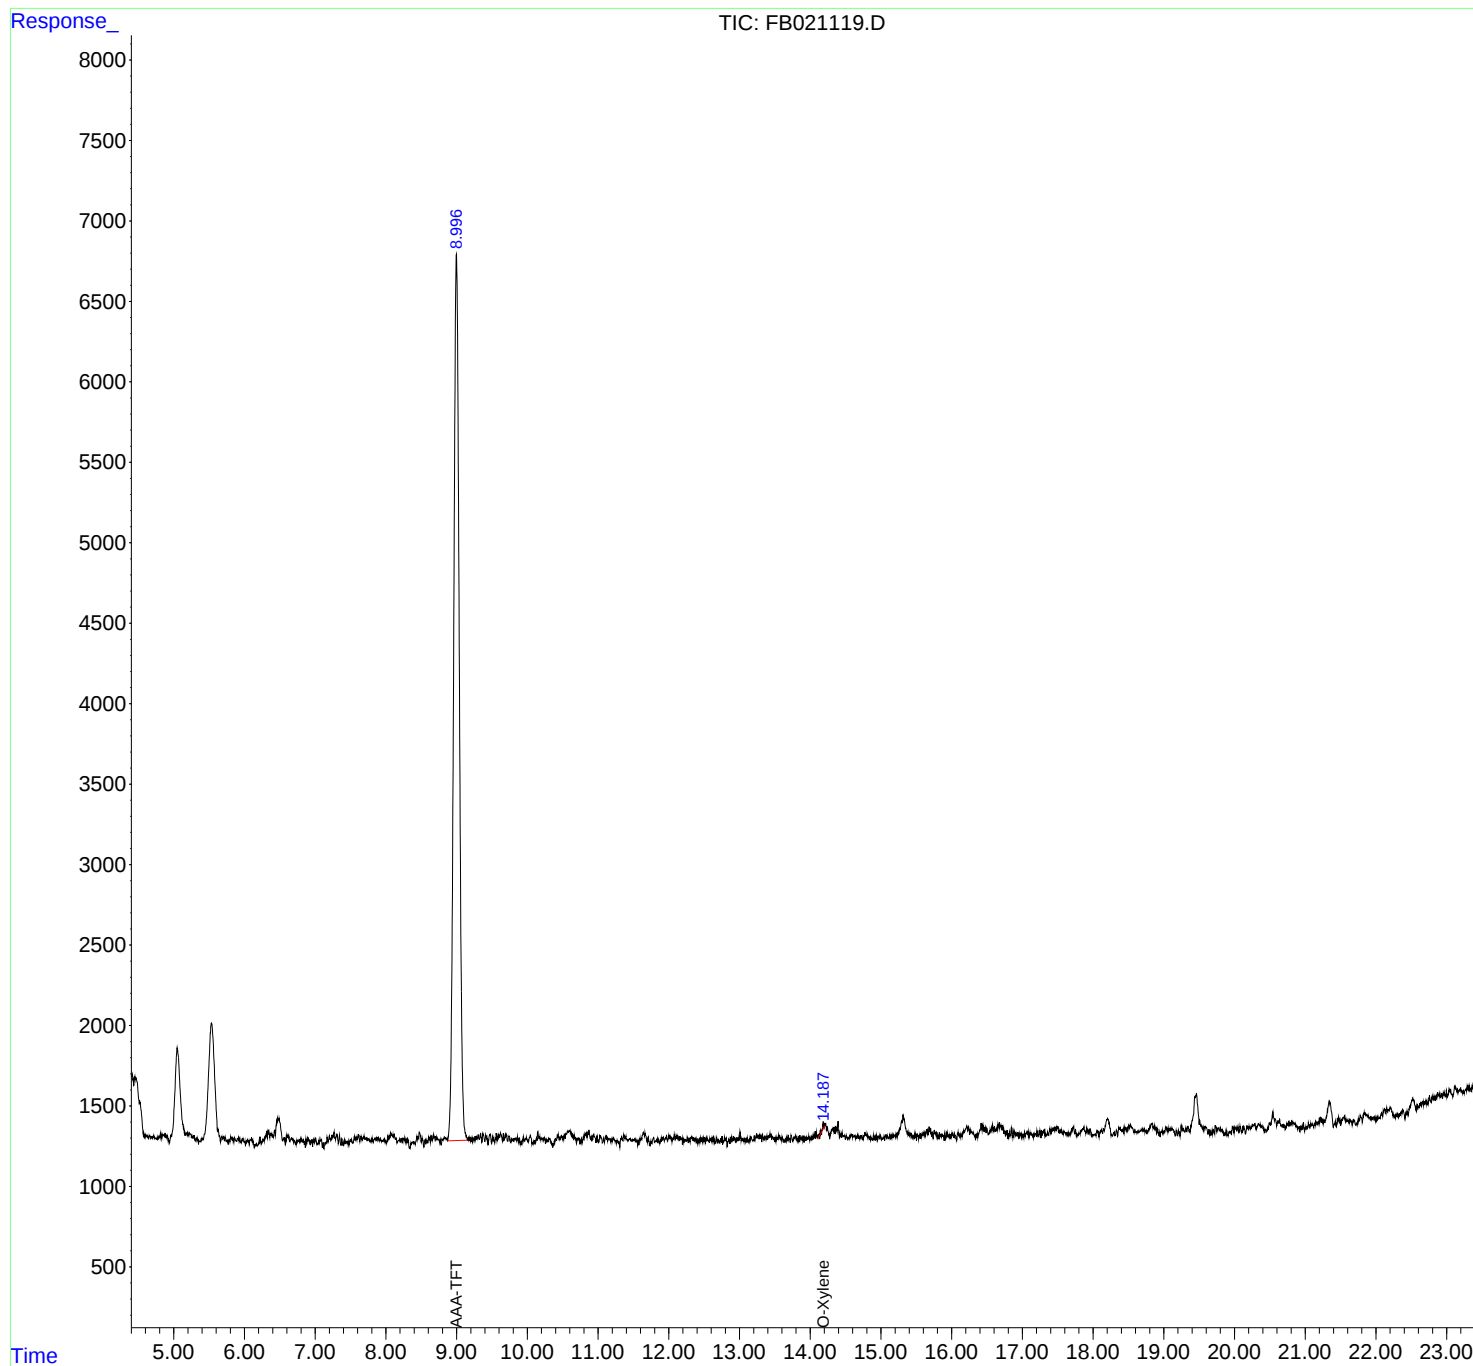


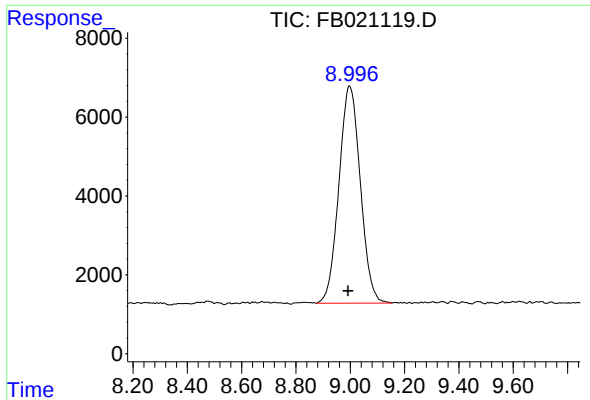

#5 AAA-TFT

R.T.: 8.997 min
Delta R.T.: 0.006 min
Response: 301415
Conc: 16.80 ng/ml

Instrument :
FID_B
ClientSampleId :

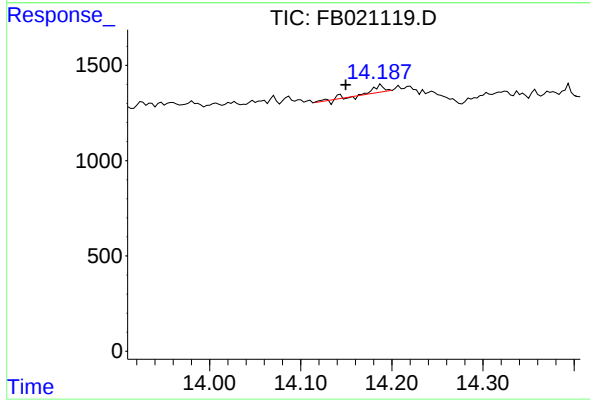

#9 O-Xylene

R.T.: 14.188 min
Delta R.T.: 0.039 min
Response: 300
Conc: 0.01 ng/ml