

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052021\
 Data File : FB025793.D
 Signal(s) : FID2B.CH
 Acq On : 20 May 2021 11:21
 Operator : DD/AJ
 Sample : M2392-08
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: May 20 12:18:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051821.M
 Quant Title :
 QLast Update : Tue May 18 16:50:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.225	193310	10.351 ng/ml
Target Compounds				
1) t	2-Methylpentane	5.198	625	0.029 ng/ml
2) t	2,2,4-Trimethylpentane	7.885	1245	0.067 ng/ml
3) t	n-Heptane	8.191	2412	0.085 ng/ml
4) t	Benzene	8.346	703	0.020 ng/ml
6) t	Toluene	11.052	1929	0.057 ng/ml
7) t	Ethylbenzene	13.404	49278	1.506 ng/ml
8) t	m-Xylene	13.592	1790	0.055 ng/ml
9) t	O-Xylene	14.303	8923	0.292 ng/ml
10) t	1,2,4-Trimethylbenzene	16.569	5668	0.224 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052021\
Data File : FB025793.D
Signal(s) : FID2B.CH
Acq On : 20 May 2021 11:21
Operator : DD/AJ
Sample : M2392-08
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 20 12:18:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051821.M
Quant Title :
QLast Update : Tue May 18 16:50:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

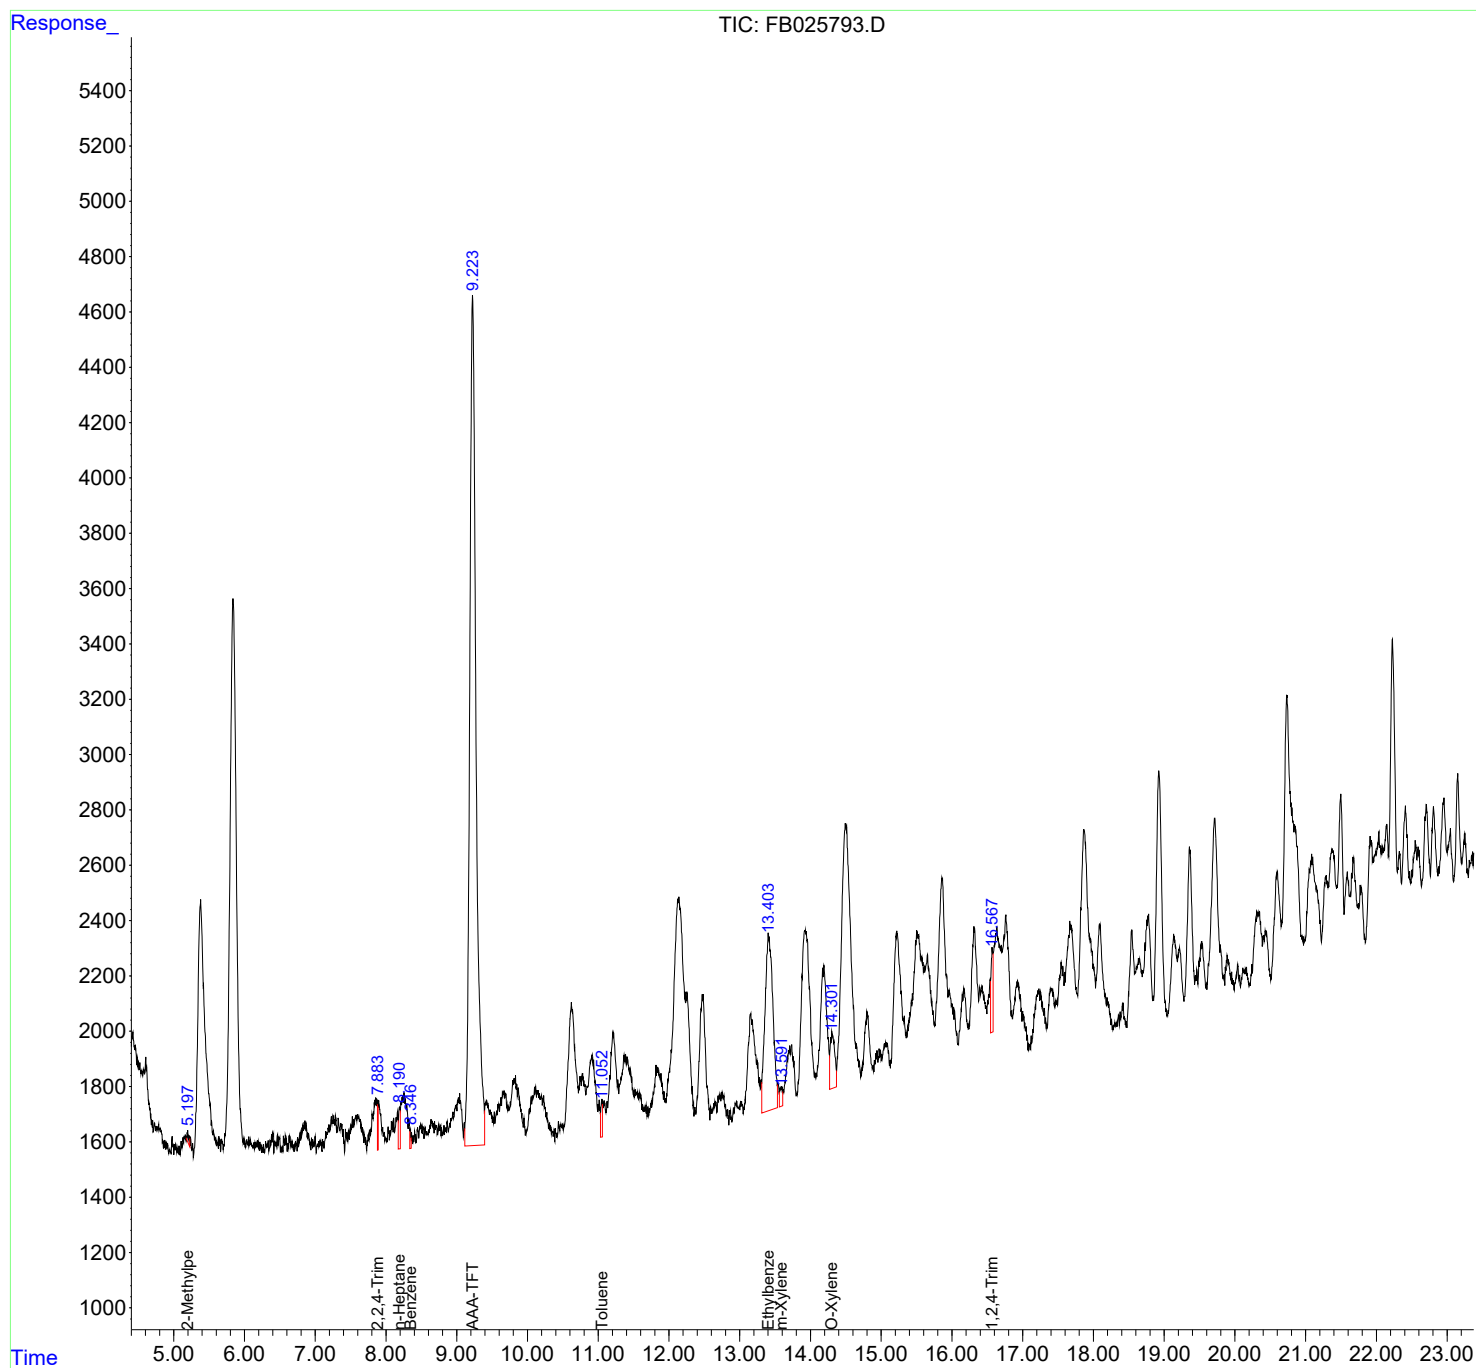


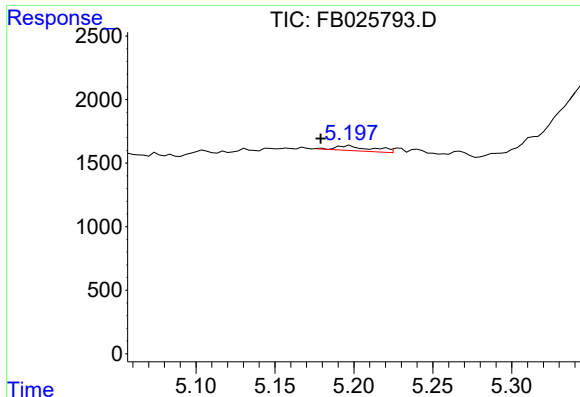

#1 2-Methylpentane


R.T.: 5.198 min
Delta R.T.: 0.019 min
Response: 625
Conc: 0.03 ng/ml

Instrument :
FID_B
ClientSampleId :

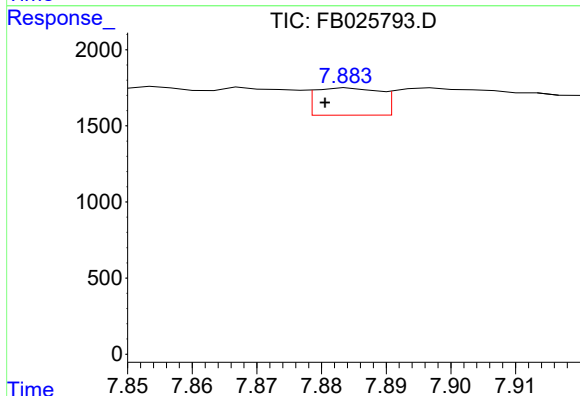


#2 2,2,4-Trimethylpentane

R.T.: 7.885 min
Delta R.T.: 0.004 min
Response: 1245
Conc: 0.07 ng/ml

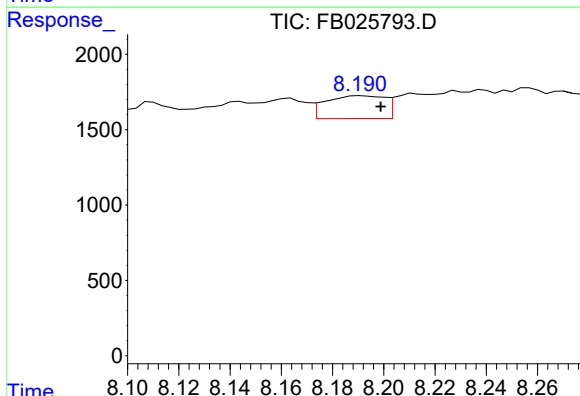


#3 n-Heptane

R.T.: 8.191 min
Delta R.T.: -0.007 min
Response: 2412
Conc: 0.09 ng/ml

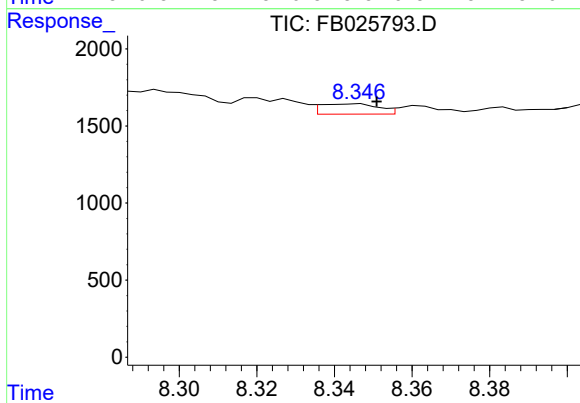

#4 Benzene


R.T.: 8.346 min
Delta R.T.: -0.005 min
Response: 703
Conc: 0.02 ng/ml

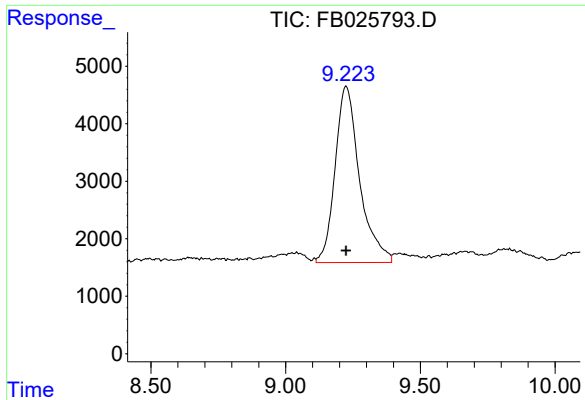

#5 AAA-TFT


R.T.: 9.225 min
Delta R.T.: 0.000 min
Response: 193310
Conc: 10.35 ng/ml

Instrument :
FID_B
ClientSampleId :

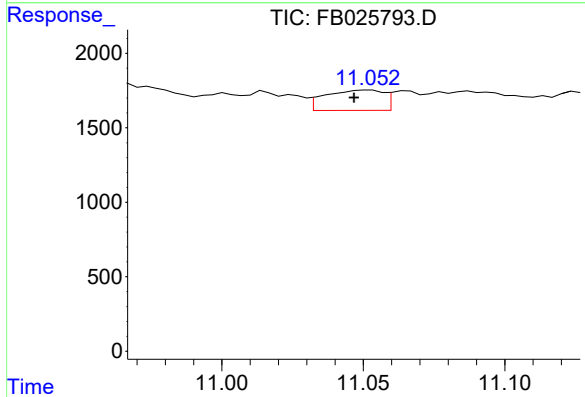


#6 Toluene

R.T.: 11.052 min
Delta R.T.: 0.005 min
Response: 1929
Conc: 0.06 ng/ml

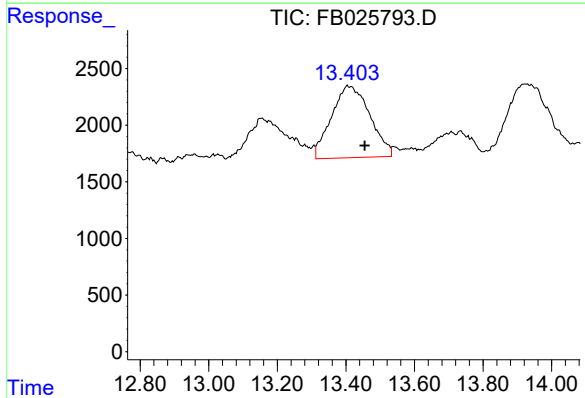


#7 Ethylbenzene

R.T.: 13.404 min
Delta R.T.: -0.051 min
Response: 49278
Conc: 1.51 ng/ml

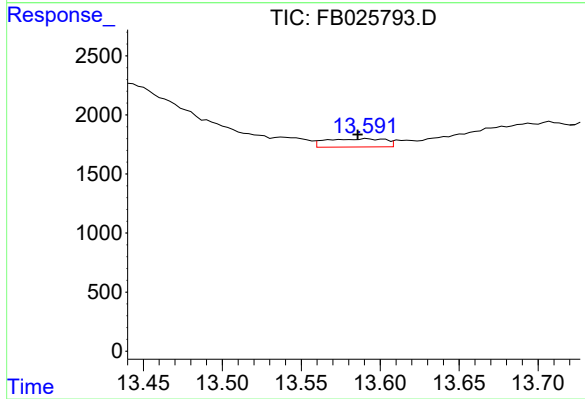

#8 m-Xylene


R.T.: 13.592 min
Delta R.T.: 0.006 min
Response: 1790
Conc: 0.05 ng/ml

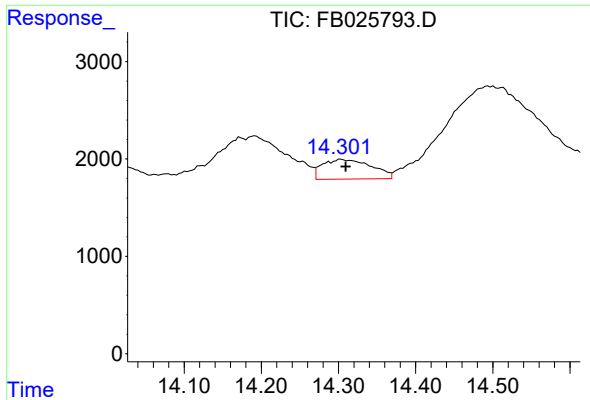

#9 O-Xylene

R.T.: 14.303 min
Delta R.T.: -0.006 min
Response: 8923
Conc: 0.29 ng/ml

Instrument :
FID_B
ClientSampleId :

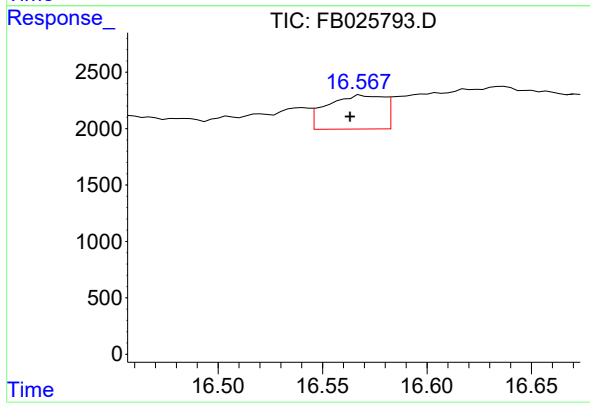

#10 1,2,4-Trimethylbenzene

R.T.: 16.569 min
Delta R.T.: 0.006 min
Response: 5668
Conc: 0.22 ng/ml