

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052021\
 Data File : FB025789.D
 Signal(s) : FID2B.CH
 Acq On : 20 May 2021 9:07
 Operator : DD/AJ
 Sample : BSF0520S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0520S1

Integration File: Calibration.e
 Quant Time: May 20 09:31:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051821.M
 Quant Title :
 QLast Update : Tue May 18 16:50:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.222	394668	21.133 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.181	768660	35.792 ng/ml
2) t 2,2,4-Trimethylpentane	7.875	710537	38.435 ng/ml
3) t n-Heptane	8.197	313208	11.055 ng/ml
4) t Benzene	8.348	382782	10.783 ng/ml
6) t Toluene	11.043	1118875	32.983 ng/ml
7) t Ethylbenzene	13.451	354302	10.829 ng/ml
8) t m-Xylene	13.581	711404	21.740 ng/ml
9) t O-Xylene	14.305	654471	21.397 ng/ml
10) t 1,2,4-Trimethylbenzene	16.558	546128	21.554 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052021\
Data File : FB025789.D
Signal(s) : FID2B.CH
Acq On : 20 May 2021 9:07
Operator : DD/AJ
Sample : BSF0520S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0520S1

Integration File: Calibration.e
Quant Time: May 20 09:31:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051821.M
Quant Title :
QLast Update : Tue May 18 16:50:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

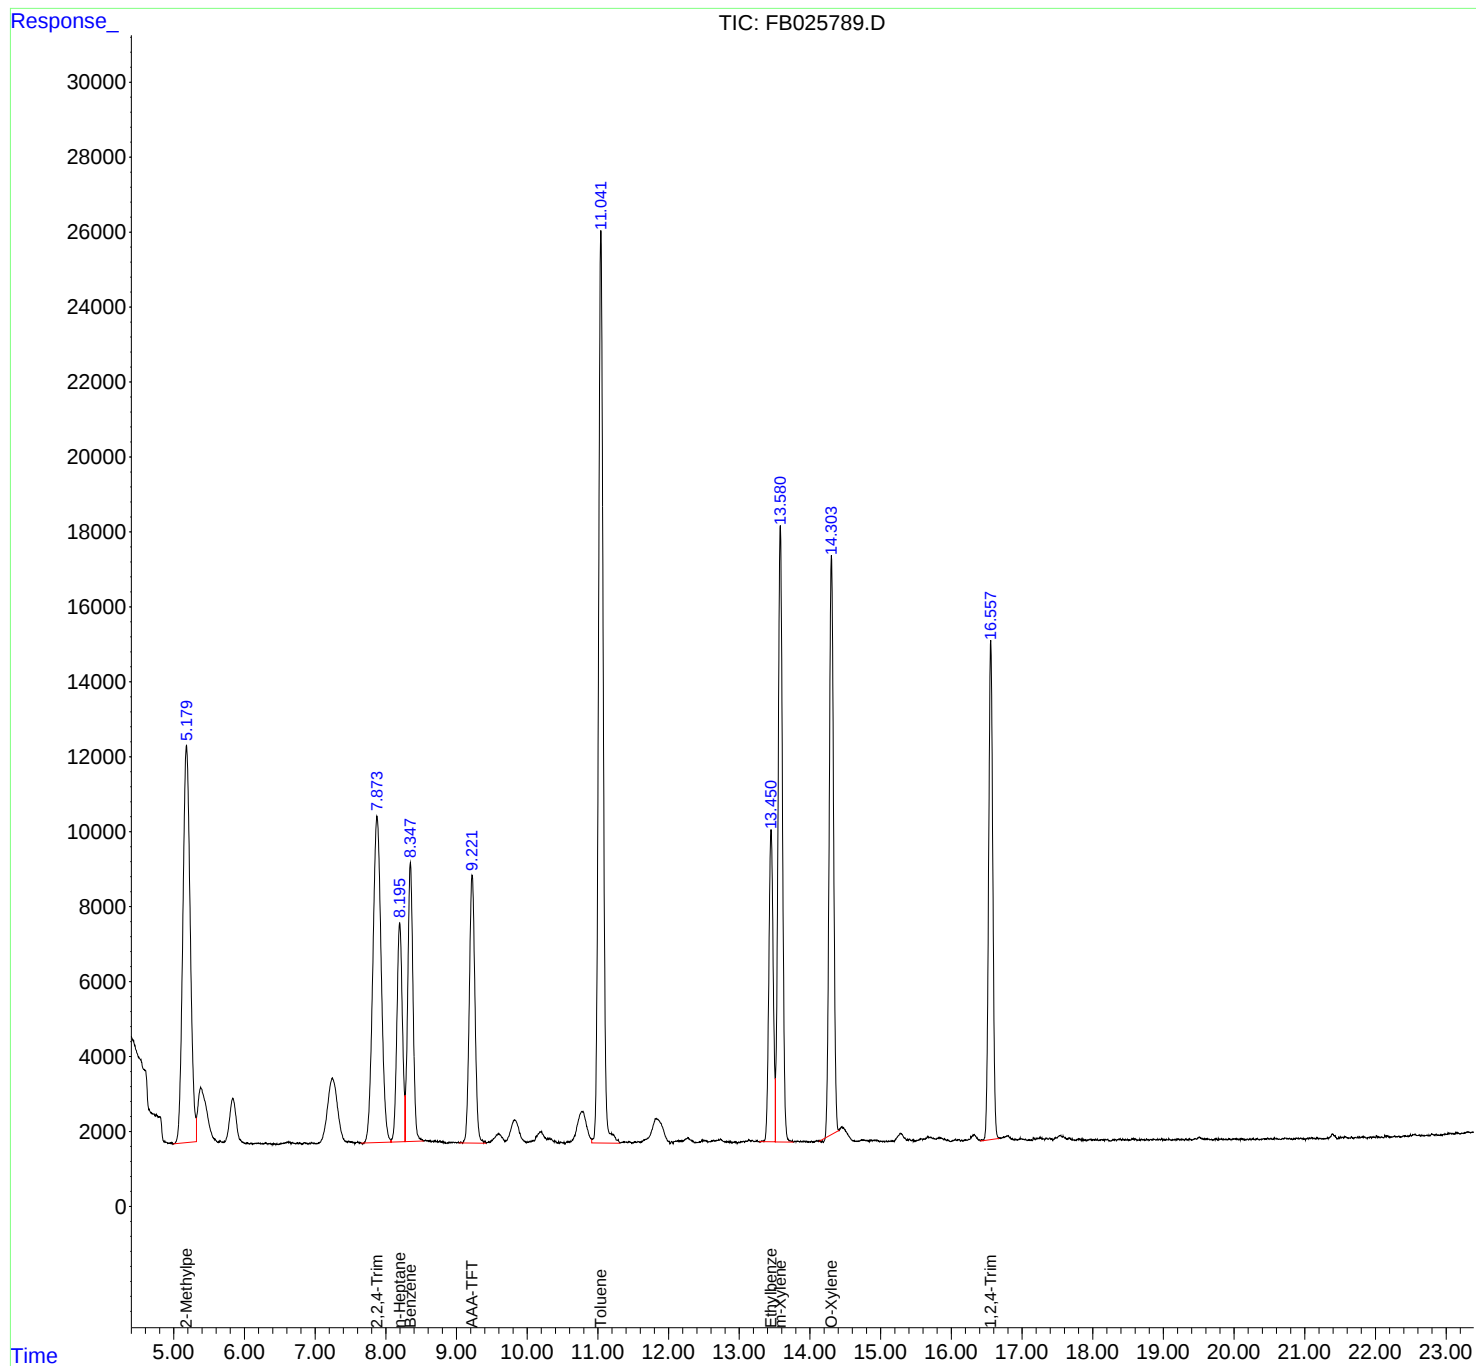


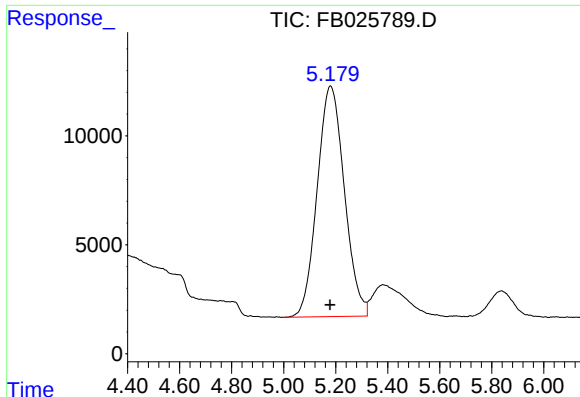

#1 2-Methylpentane


R.T.: 5.181 min
Delta R.T.: 0.002 min
Response: 768660
Conc: 35.79 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0520S1

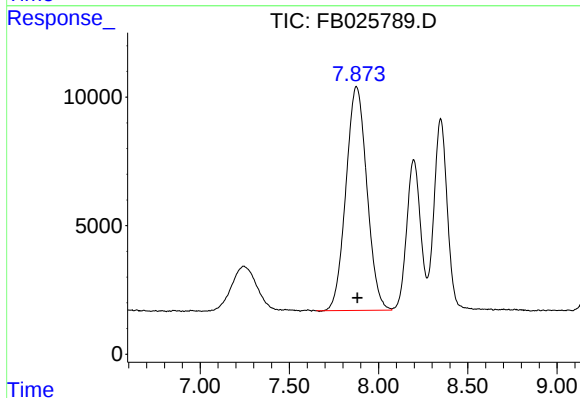


#2 2,2,4-Trimethylpentane

R.T.: 7.875 min
Delta R.T.: -0.006 min
Response: 710537
Conc: 38.44 ng/ml

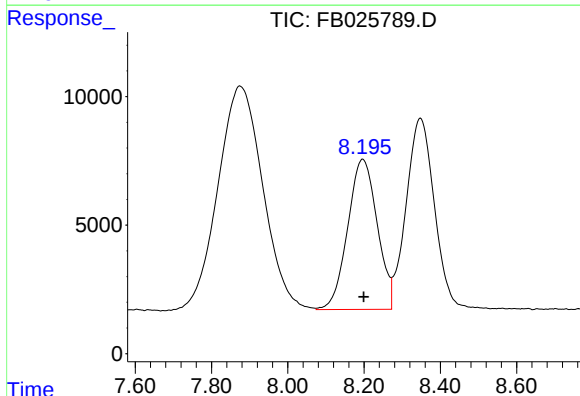


#3 n-Heptane

R.T.: 8.197 min
Delta R.T.: -0.002 min
Response: 313208
Conc: 11.06 ng/ml

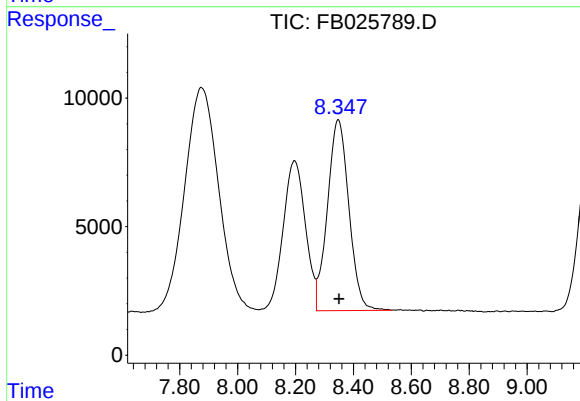

#4 Benzene


R.T.: 8.348 min
Delta R.T.: -0.003 min
Response: 382782
Conc: 10.78 ng/ml

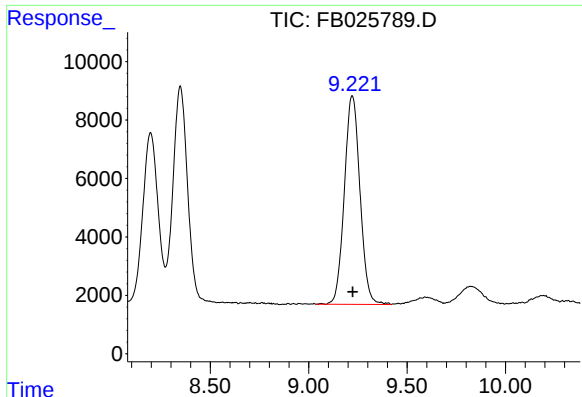

#5 AAA-TFT


R.T.: 9.222 min
Delta R.T.: -0.003 min
Response: 394668
Conc: 21.13 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0520S1

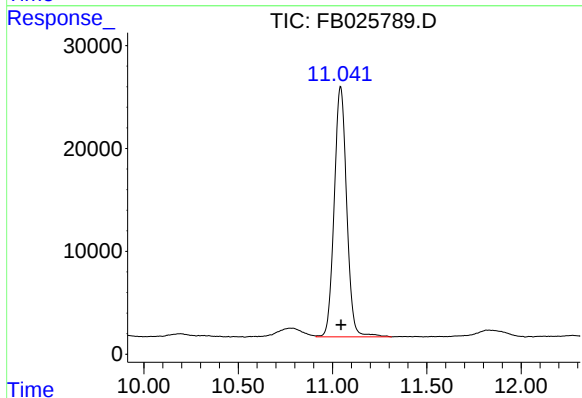


#6 Toluene

R.T.: 11.043 min
Delta R.T.: -0.004 min
Response: 1118875
Conc: 32.98 ng/ml

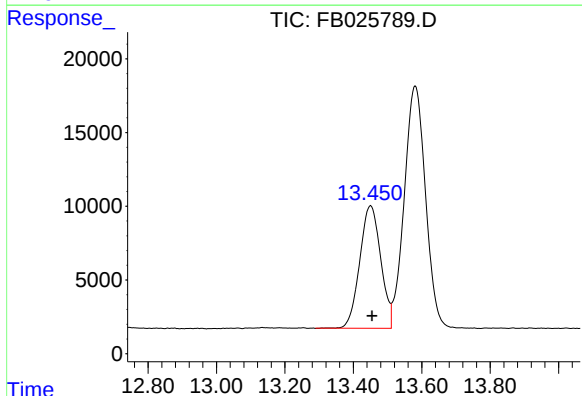


#7 Ethylbenzene

R.T.: 13.451 min
Delta R.T.: -0.004 min
Response: 354302
Conc: 10.83 ng/ml

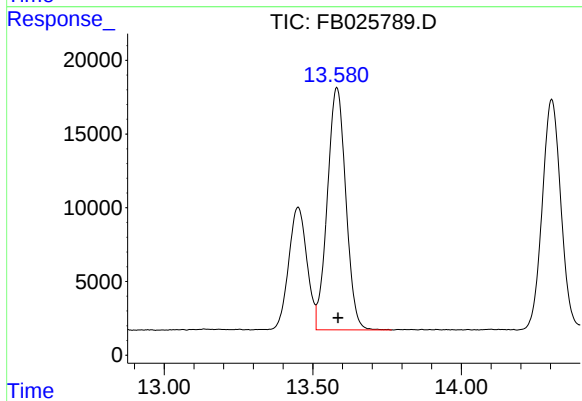

#8 m-Xylene


R.T.: 13.581 min
Delta R.T.: -0.004 min
Response: 711404
Conc: 21.74 ng/ml

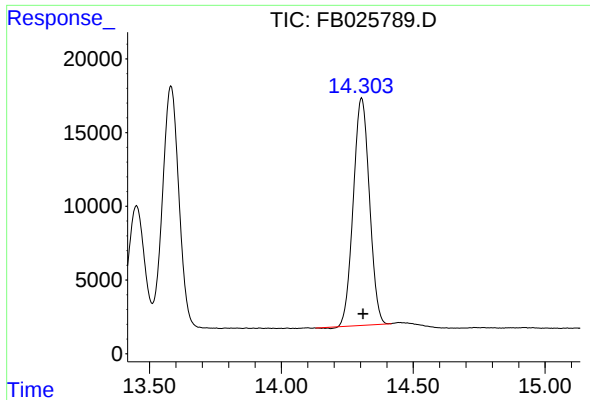

#9 O-Xylene

R.T.: 14.305 min
Delta R.T.: -0.005 min
Response: 654471
Conc: 21.40 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0520S1

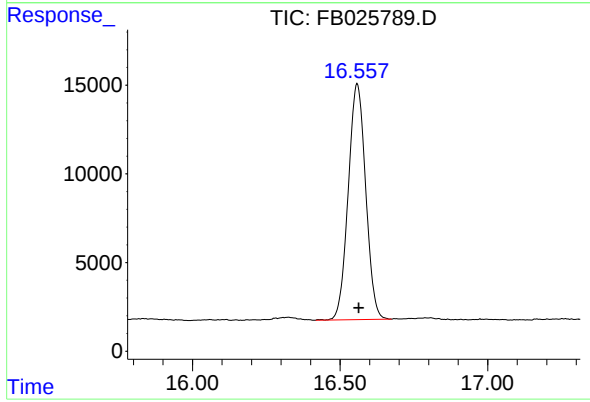

#10 1,2,4-Trimethylbenzene

R.T.: 16.558 min
Delta R.T.: -0.005 min
Response: 546128
Conc: 21.55 ng/ml