

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052021\
 Data File : FB025800.D
 Signal(s) : FID2B.CH
 Acq On : 20 May 2021 15:25
 Operator : DD/AJ
 Sample : M2413-03MS
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 124027MS

Integration File: Calibration.e
 Quant Time: May 20 16:21:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051821.M
 Quant Title :
 QLast Update : Tue May 18 16:50:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.233	386781	20.711 ng/ml
Target Compounds				
1) t	2-Methylpentane	5.203	632143	29.435 ng/ml
2) t	2,2,4-Trimethylpentane	7.893	534239	28.899 ng/ml
3) t	n-Heptane	8.209	275232	9.715 ng/ml
4) t	Benzene	8.361	368203	10.372 ng/ml
6) t	Toluene	11.051	1071763	31.594 ng/ml
7) t	Ethylbenzene	13.457	335799	10.263 ng/ml
8) t	m-Xylene	13.588	673601	20.585 ng/ml
9) t	O-Xylene	14.310	624187	20.407 ng/ml
10) t	1,2,4-Trimethylbenzene	16.563	504864	19.925 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052021\
Data File : FB025800.D
Signal(s) : FID2B.CH
Acq On : 20 May 2021 15:25
Operator : DD/AJ
Sample : M2413-03MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
124027MS

Integration File: Calibration.e
Quant Time: May 20 16:21:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051821.M
Quant Title :
QLast Update : Tue May 18 16:50:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

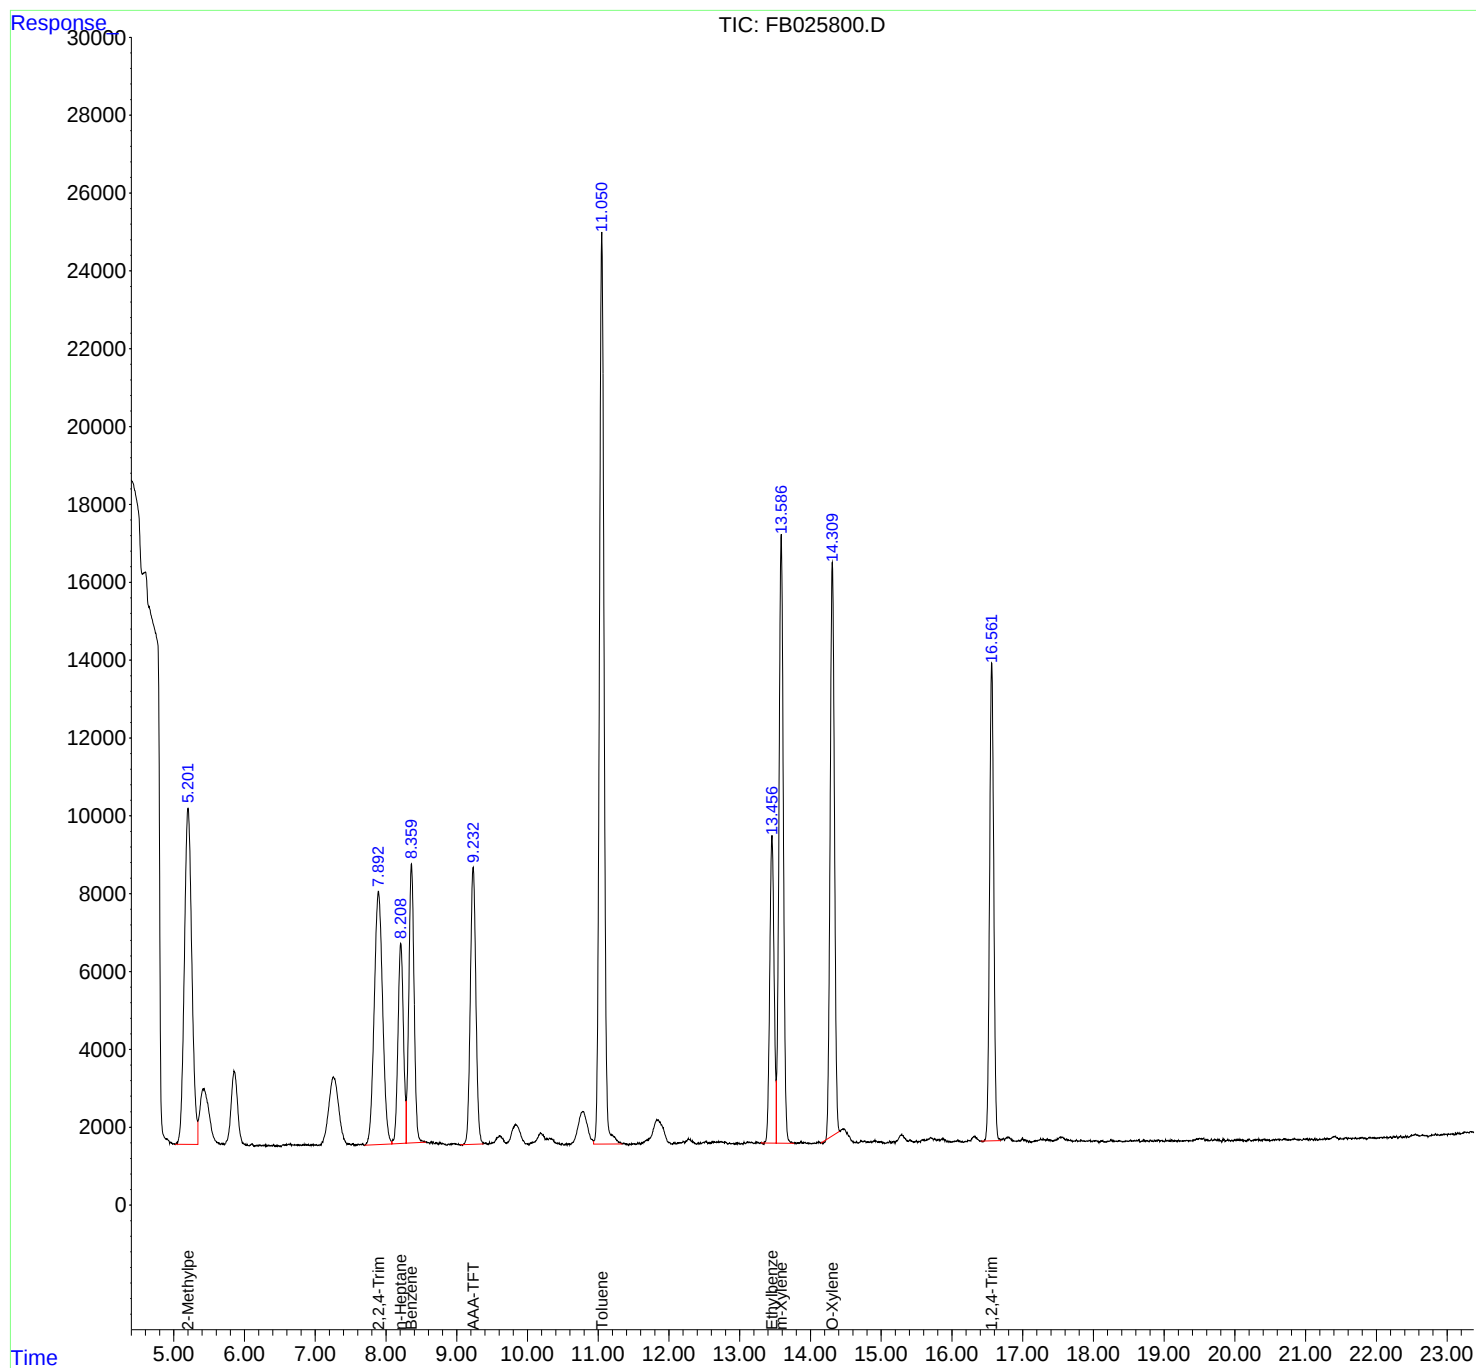


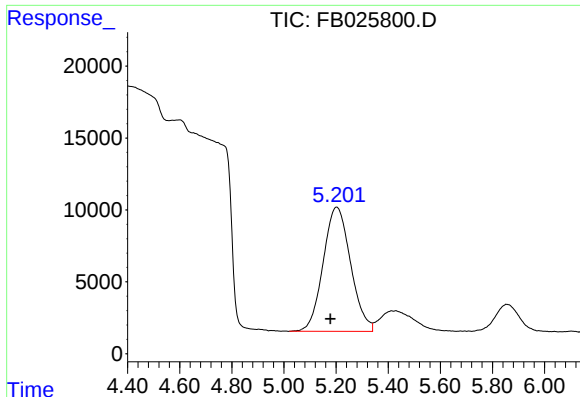

#1 2-Methylpentane


R.T.: 5.203 min
Delta R.T.: 0.024 min
Response: 632143
Conc: 29.44 ng/ml

Instrument :
FID_B
ClientSampleId :
124027MS

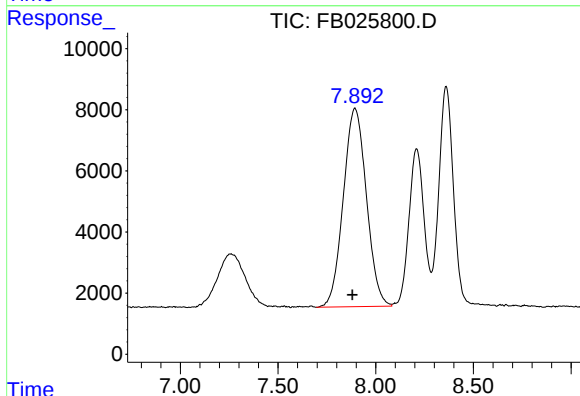


#2 2,2,4-Trimethylpentane

R.T.: 7.893 min
Delta R.T.: 0.013 min
Response: 534239
Conc: 28.90 ng/ml

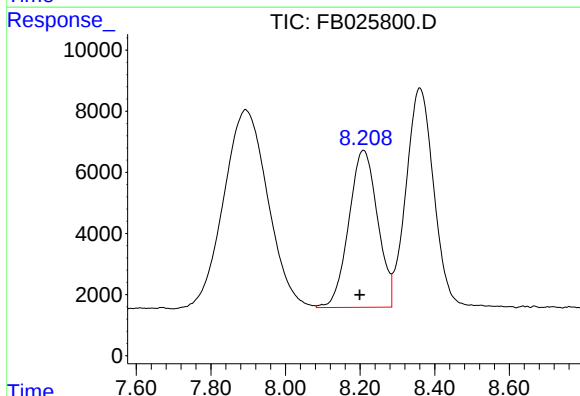


#3 n-Heptane

R.T.: 8.209 min
Delta R.T.: 0.011 min
Response: 275232
Conc: 9.71 ng/ml

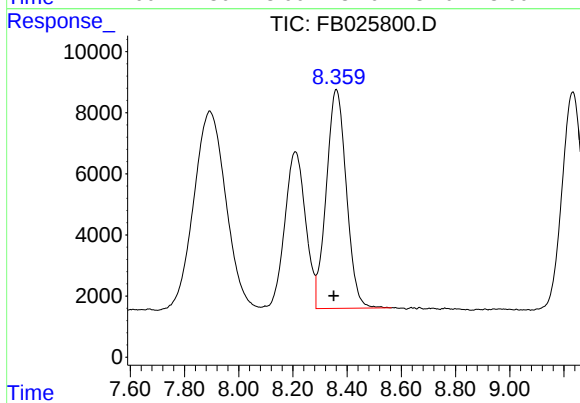

#4 Benzene


R.T.: 8.361 min
Delta R.T.: 0.010 min
Response: 368203
Conc: 10.37 ng/ml

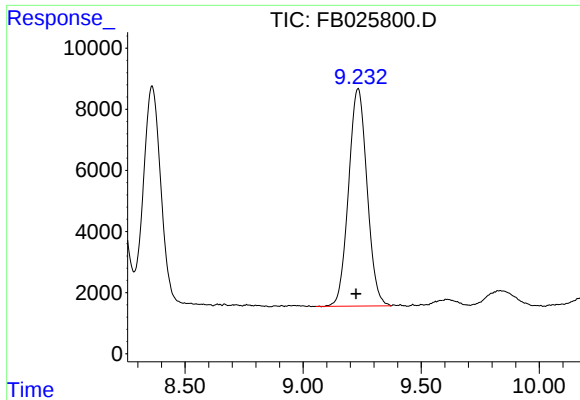

#5 AAA-TFT


R.T.: 9.233 min
Delta R.T.: 0.009 min
Response: 386781
Conc: 20.71 ng/ml

Instrument :
FID_B
ClientSampleId :
124027MS

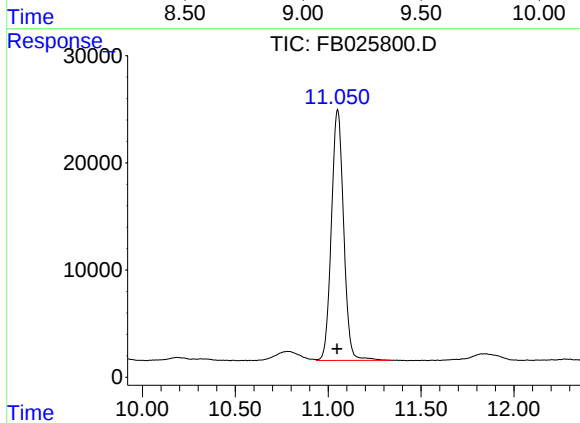


#6 Toluene

R.T.: 11.051 min
Delta R.T.: 0.004 min
Response: 1071763
Conc: 31.59 ng/ml

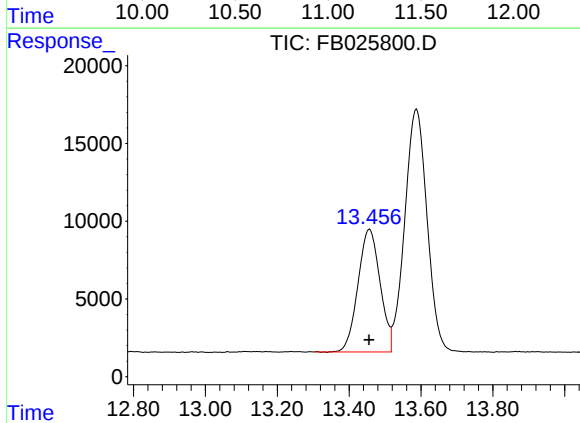


#7 Ethylbenzene

R.T.: 13.457 min
Delta R.T.: 0.002 min
Response: 335799
Conc: 10.26 ng/ml

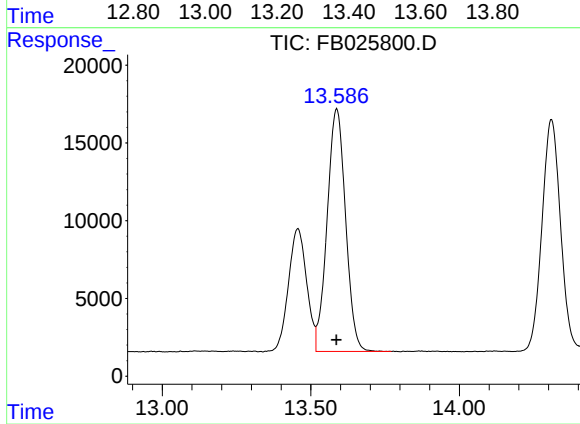

#8 m-Xylene


R.T.: 13.588 min
Delta R.T.: 0.002 min
Response: 673601
Conc: 20.58 ng/ml

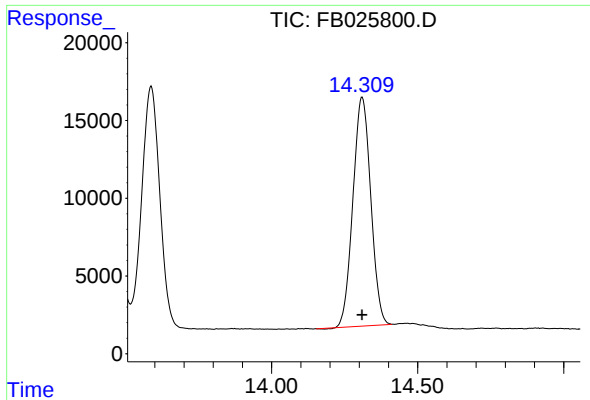

#9 O-Xylene

R.T.: 14.310 min
Delta R.T.: 0.000 min
Response: 624187
Conc: 20.41 ng/ml

Instrument :
FID_B
ClientSampleId :
124027MS

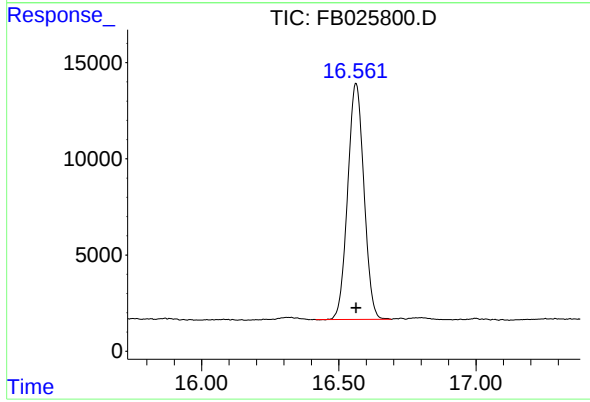

#10 1,2,4-Trimethylbenzene

R.T.: 16.563 min
Delta R.T.: 0.000 min
Response: 504864
Conc: 19.93 ng/ml