

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052025\
Data File : FB031791.D
Signal(s) : FID2B.CH
Acq On : 20 May 2025 15:56
Operator : YP/AJ
Sample : Q2074-07
Misc : 6.09G/5.00 ML DI WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-40

Integration File: Calibration.e
Quant Time: May 20 23:36:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051925.M
Quant Title :
QLast Update : Mon May 19 10:47:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	414605	19.174 ng/ml
Target Compounds			
6) t Toluene	10.623	6229	0.141 ng/ml
8) t m-Xylene	13.192	8725	0.202 ng/ml
9) t O-Xylene	13.924	10208	0.256 ng/ml
10) t 1,2,4-Trimethylbenzene	16.201	17552	0.615 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052025\
Data File : FB031791.D
Signal(s) : FID2B.CH
Acq On : 20 May 2025 15:56
Operator : YP/AJ
Sample : Q2074-07
Misc : 6.09G/5.00 ML DI WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-40

Integration File: Calibration.e
Quant Time: May 20 23:36:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051925.M
Quant Title :
QLast Update : Mon May 19 10:47:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

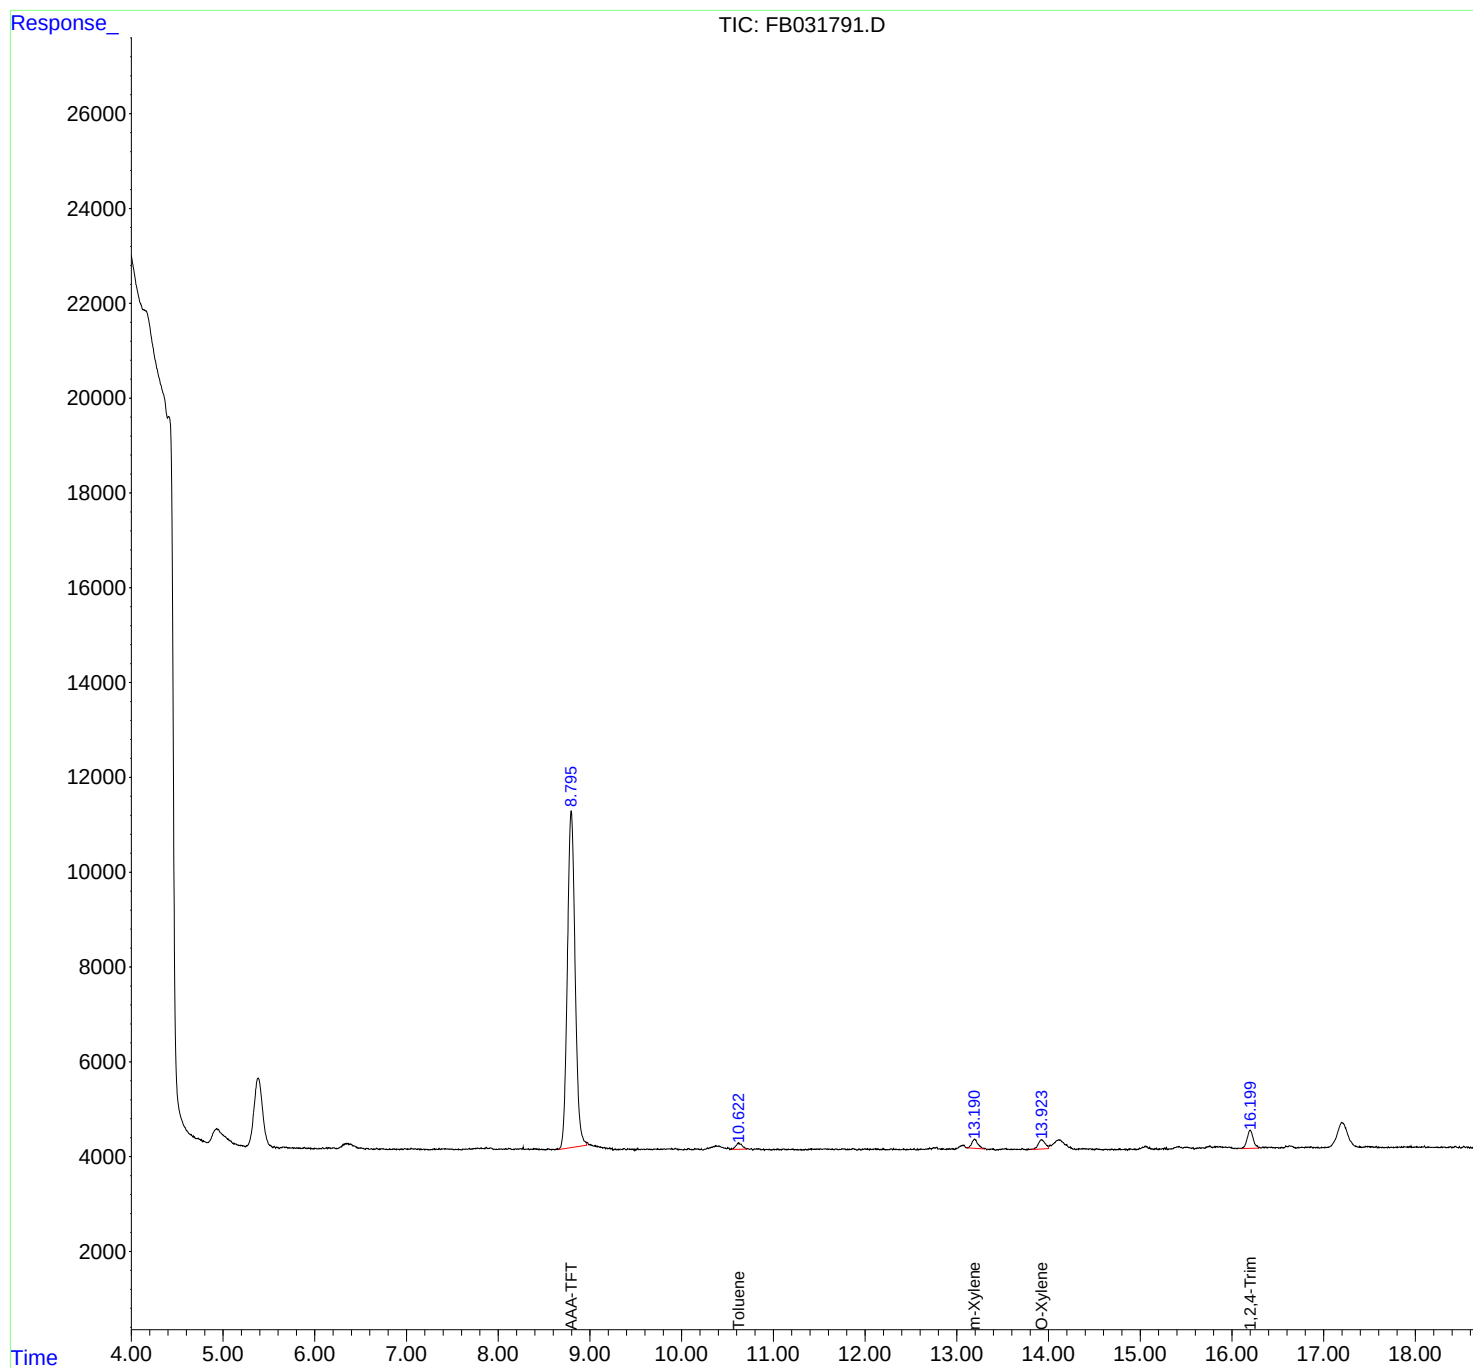


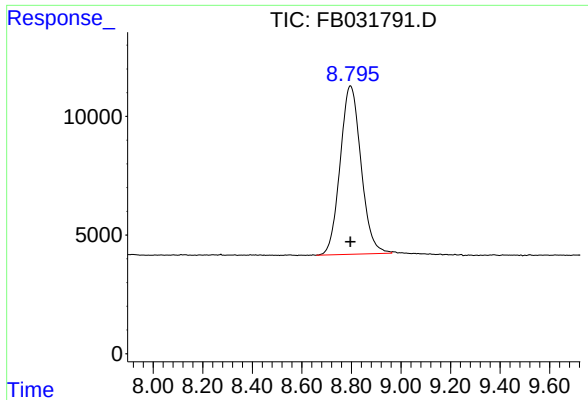

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 414605
Conc: 19.17 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-40

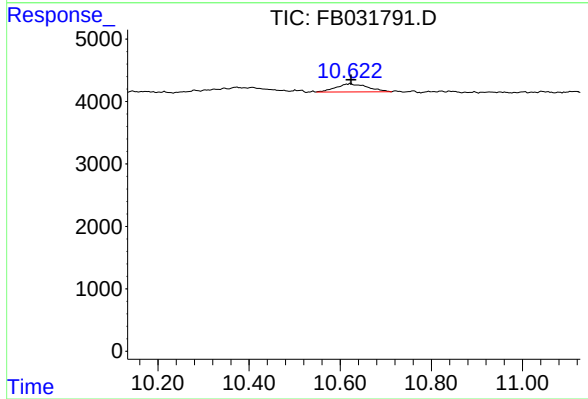


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.000 min
Response: 6229
Conc: 0.14 ng/ml

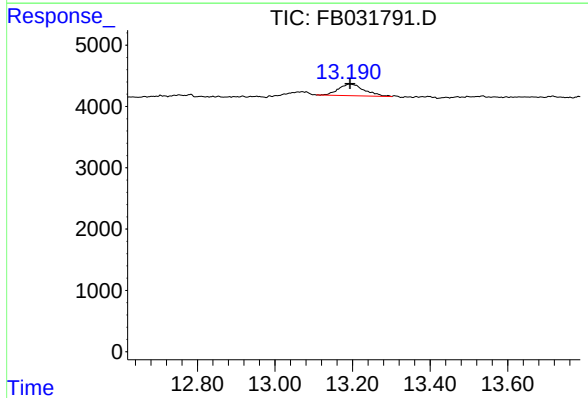


#8 m-Xylene

R.T.: 13.192 min
Delta R.T.: -0.002 min
Response: 8725
Conc: 0.20 ng/ml

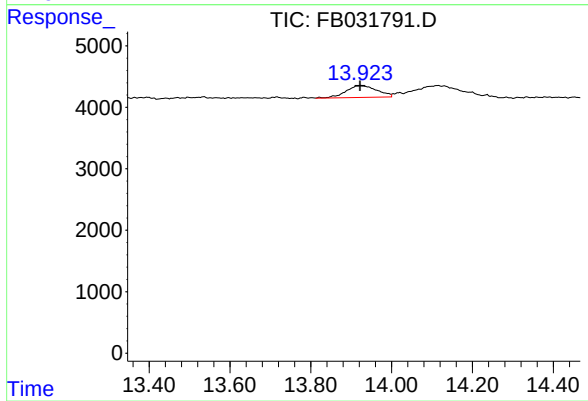

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.002 min
Response: 10208
Conc: 0.26 ng/ml

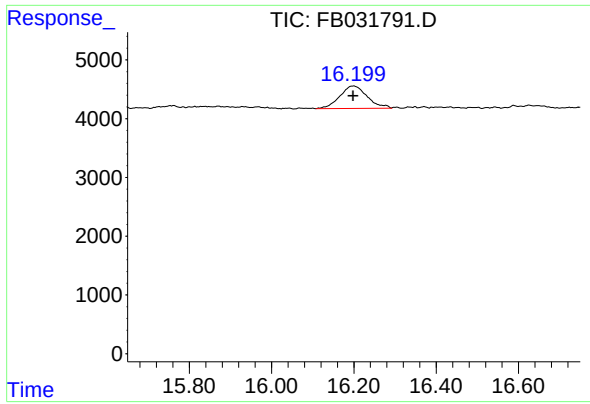

#10 1,2,4-Trimethylbenzene

R.T.: 16.201 min
Delta R.T.: 0.003 min
Response: 17552
Conc: 0.62 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-40