

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052025\
Data File : FB031796.D
Signal(s) : FID2B.CH
Acq On : 20 May 2025 18:22
Operator : YP/AJ
Sample : Q2074-05 50X
Misc : 6.90G/5.00 ML MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-38

Integration File: Calibration.e
Quant Time: May 20 23:37:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051925.M
Quant Title :
QLast Update : Mon May 19 10:47:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	422159	19.523 ng/ml
Target Compounds			
6) t Toluene	10.629	9108	0.206 ng/ml
8) t m-Xylene	13.195	6679	0.155 ng/ml
9) t O-Xylene	13.934	6170	0.155 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	6710	0.235 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052025\
Data File : FB031796.D
Signal(s) : FID2B.CH
Acq On : 20 May 2025 18:22
Operator : YP/AJ
Sample : Q2074-05 50X
Misc : 6.90G/5.00 ML MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-38

Integration File: Calibration.e
Quant Time: May 20 23:37:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051925.M
Quant Title :
QLast Update : Mon May 19 10:47:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

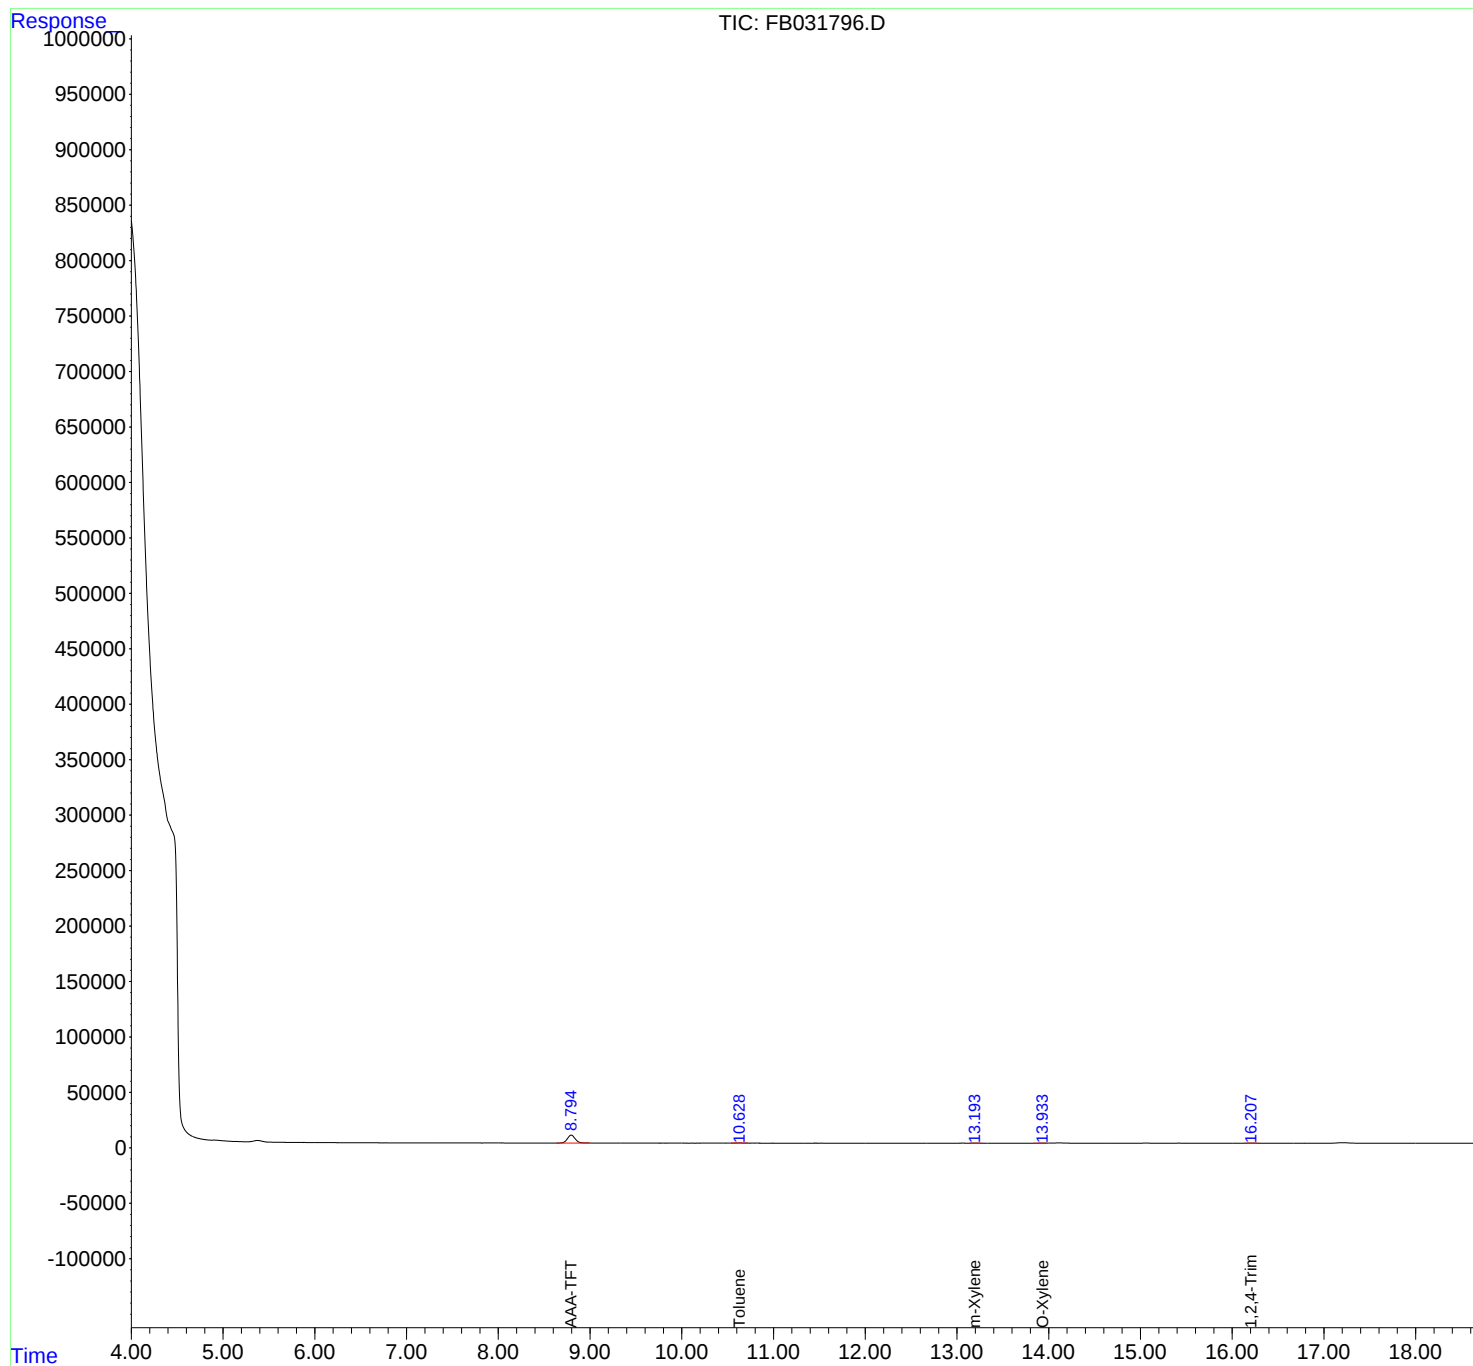


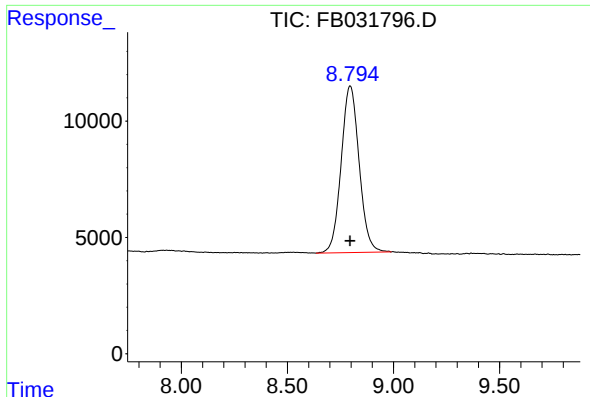

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: 0.000 min
Response: 422159
Conc: 19.52 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-38

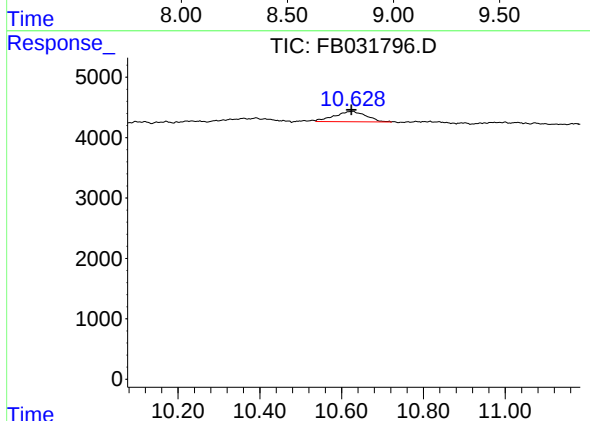


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.005 min
Response: 9108
Conc: 0.21 ng/ml

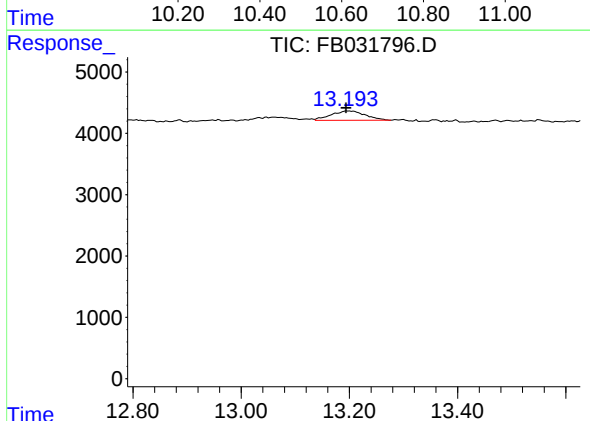


#8 m-Xylene

R.T.: 13.195 min
Delta R.T.: 0.001 min
Response: 6679
Conc: 0.15 ng/ml

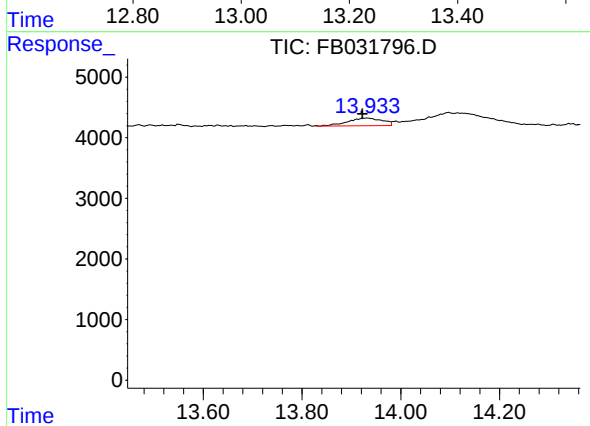

#9 O-Xylene

R.T.: 13.934 min
Delta R.T.: 0.012 min
Response: 6170
Conc: 0.15 ng/ml

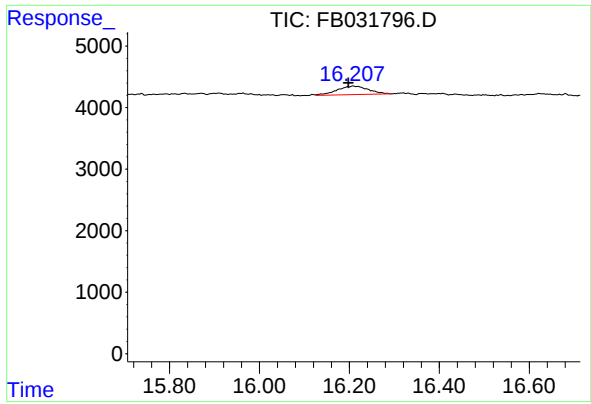

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.011 min
Response: 6710
Conc: 0.24 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-38