

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052120\
Data File : FB024377.D
Signal(s) : FID2B.CH
Acq On : 21 May 2020 16:47
Operator : DD/AJ
Sample : L2506-15
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 22 04:42:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	372747	16.880 ng/ml
Target Compounds			
6) t Toluene	10.632	648	0.018 ng/ml
8) t m-Xylene	13.195	524	0.016 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052120\
Data File : FB024377.D
Signal(s) : FID2B.CH
Acq On : 21 May 2020 16:47
Operator : DD/AJ
Sample : L2506-15
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 22 04:42:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

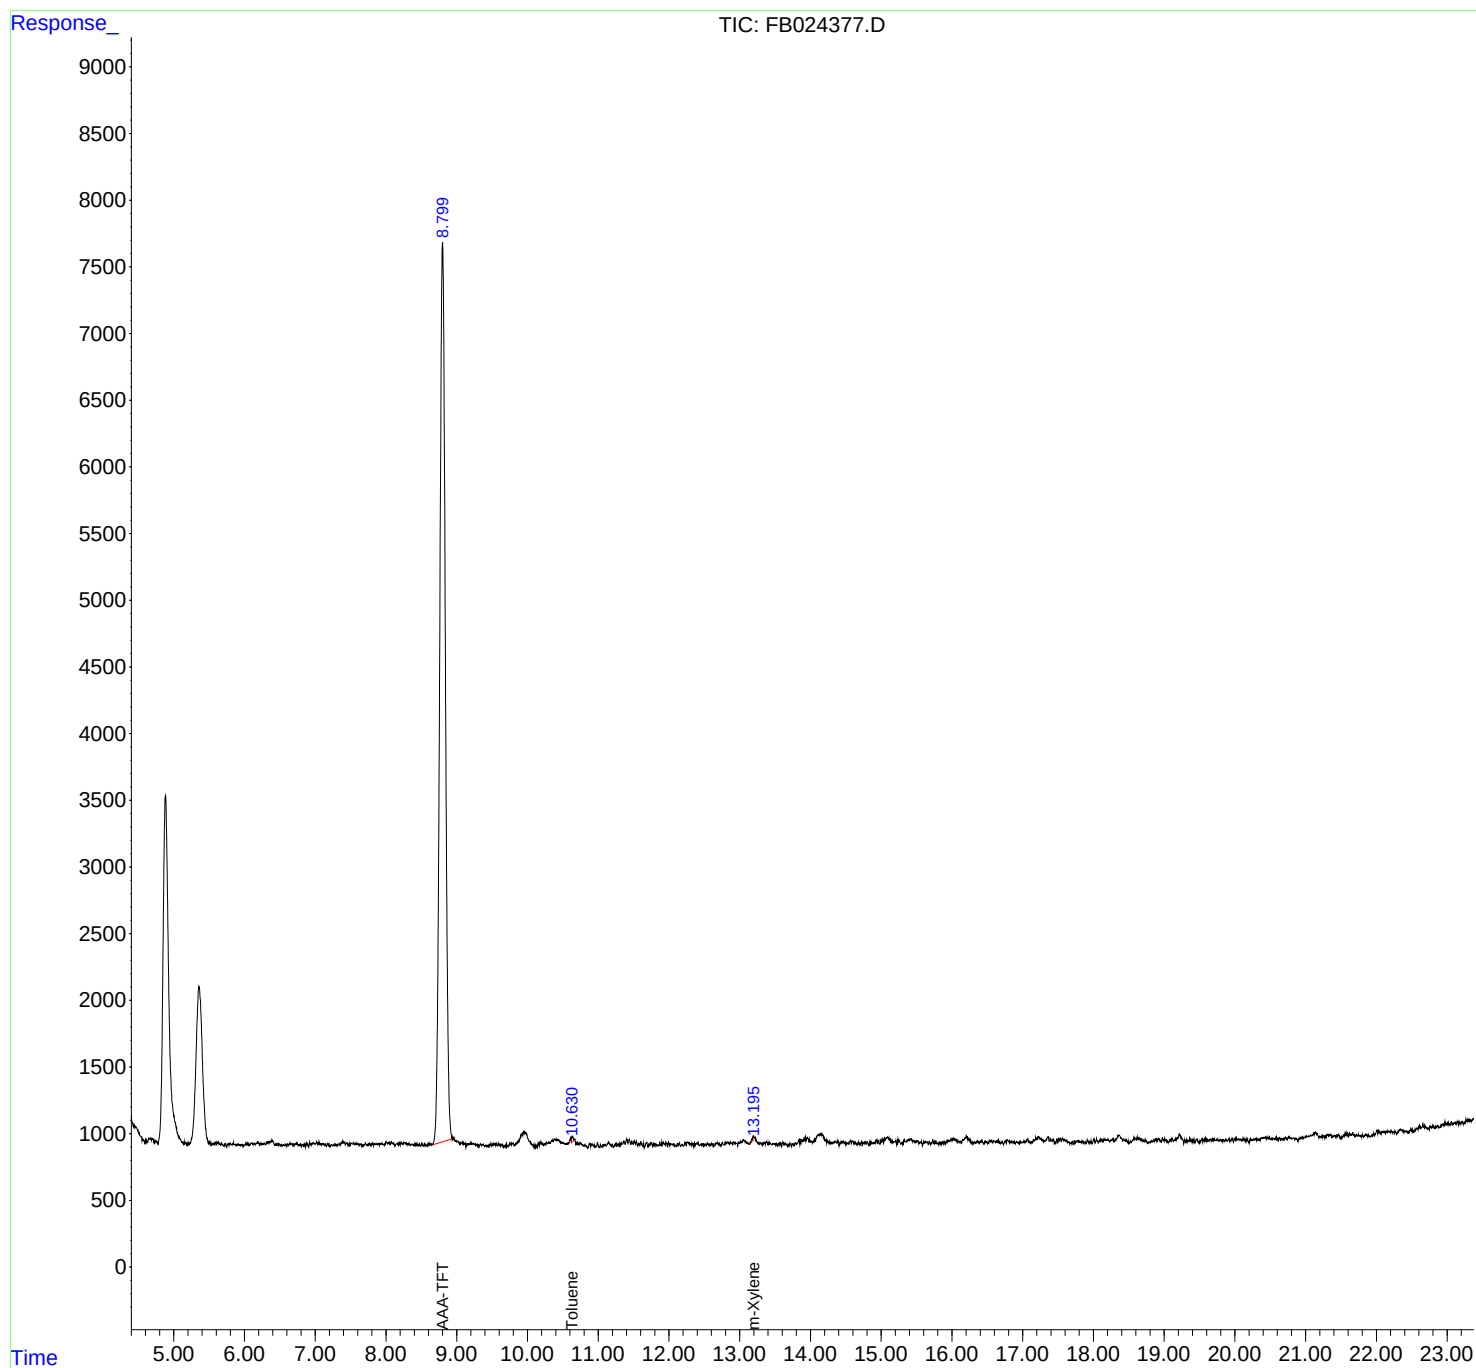

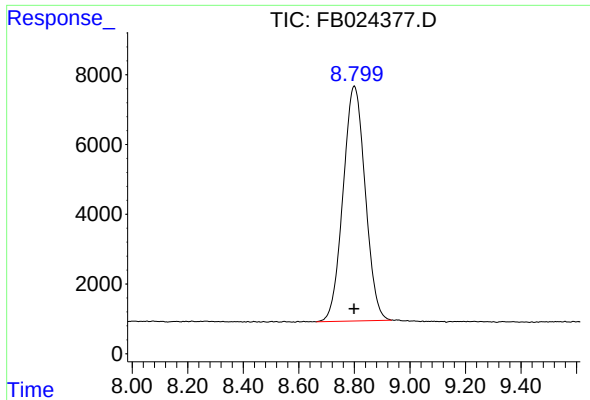


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.001 min
Response: 372747
Conc: 16.88 ng/ml

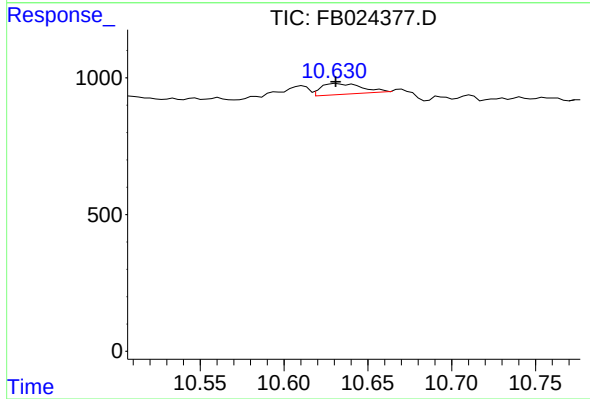

#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 648
Conc: 0.02 ng/ml

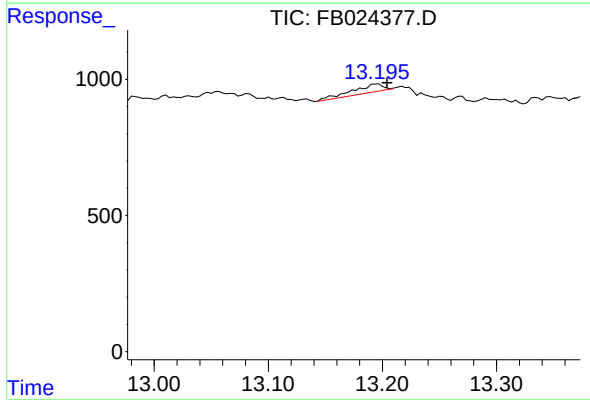

#8 m-Xylene

R.T.: 13.195 min
Delta R.T.: -0.009 min
Response: 524
Conc: 0.02 ng/ml