

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052120\
 Data File : FB024379.D
 Signal(s) : FID2B.CH
 Acq On : 21 May 2020 17:49
 Operator : DD/AJ
 Sample : L2506-15MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 22 04:42:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
 Quant Title :
 QLast Update : Mon May 11 11:14:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	308058	13.951 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	436163	14.780 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	373653	12.231 ng/ml
3) t n-Heptane	7.759	115124	3.800 ng/ml
4) t Benzene	7.894	245708	6.499 ng/ml
6) t Toluene	10.632	667428	18.419 ng/ml
7) t Ethylbenzene	13.072	192939	5.691 ng/ml
8) t m-Xylene	13.204	378689	11.476 ng/ml
9) t O-Xylene	13.932	382845	11.864 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	271519	10.068 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052120\
Data File : FB024379.D
Signal(s) : FID2B.CH
Acq On : 21 May 2020 17:49
Operator : DD/AJ
Sample : L2506-15MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 22 04:42:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

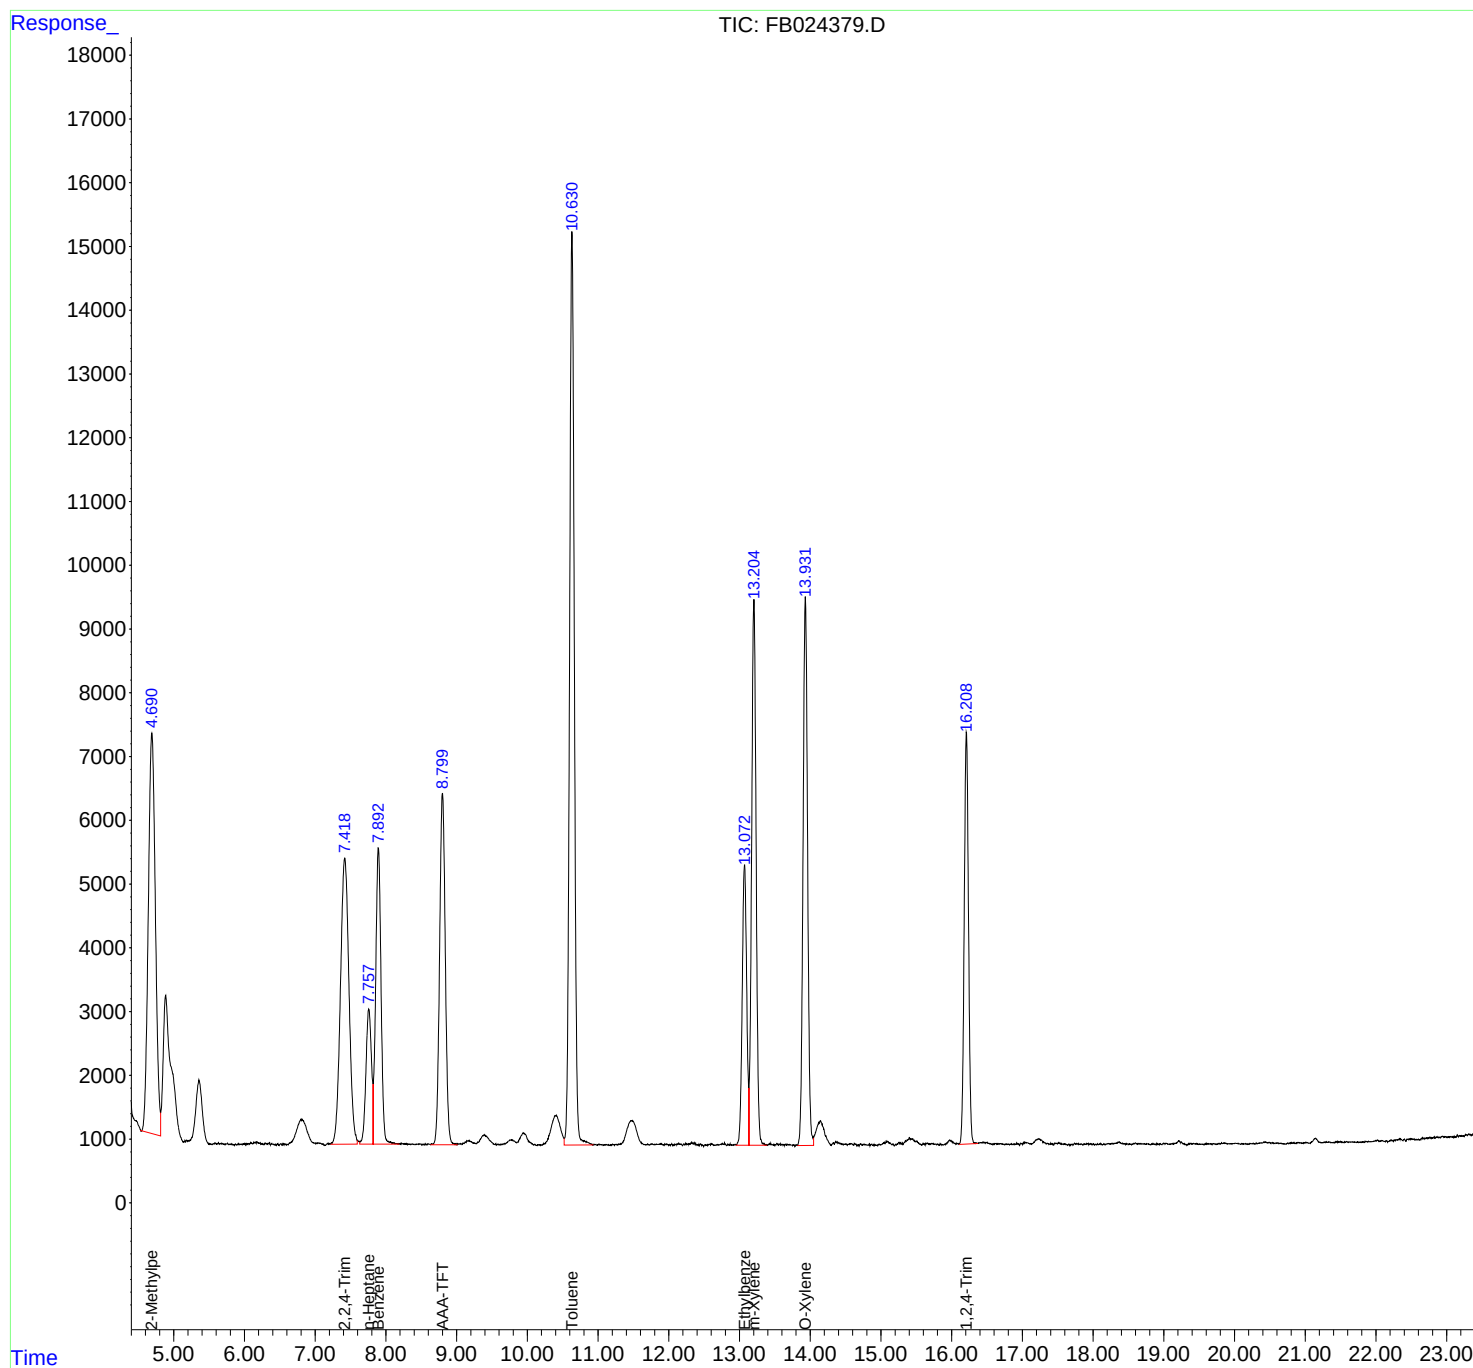

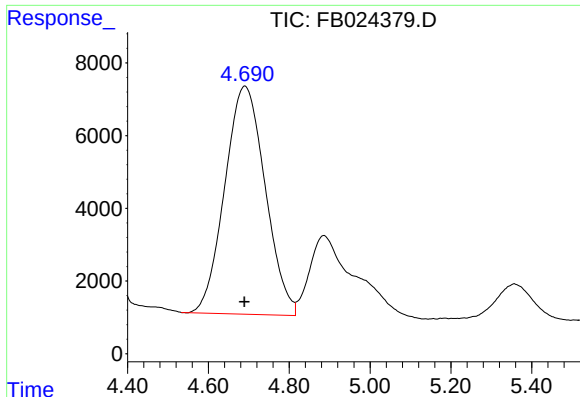


#1 2-Methylpentane

R.T.: 4.691 min
Delta R.T.: 0.002 min
Response: 436163
Conc: 14.78 ng/ml

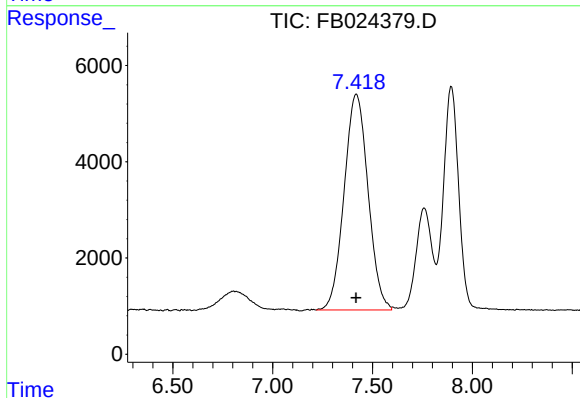


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.002 min
Response: 373653
Conc: 12.23 ng/ml

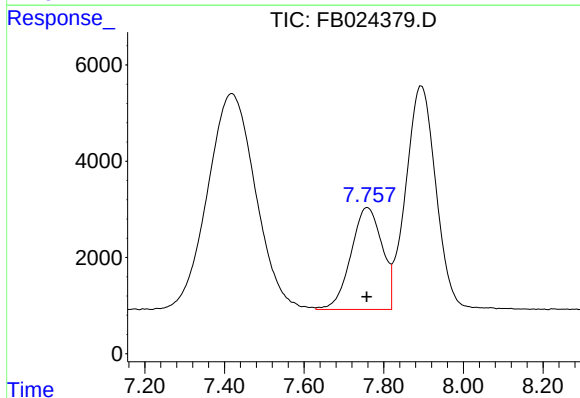


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 115124
Conc: 3.80 ng/ml

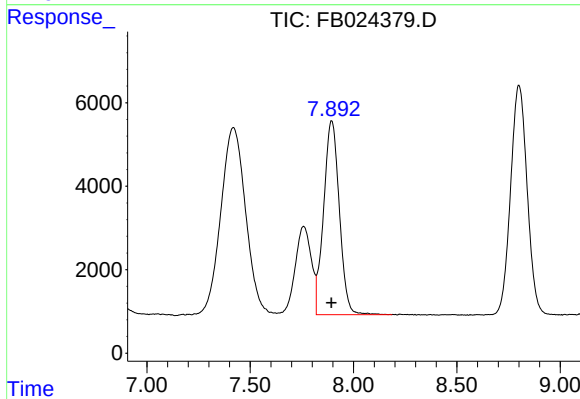


#4 Benzene

R.T.: 7.894 min
Delta R.T.: 0.001 min
Response: 245708
Conc: 6.50 ng/ml

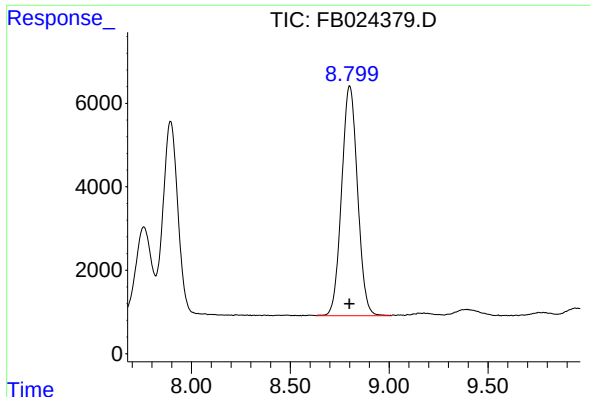


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 308058
Conc: 13.95 ng/ml

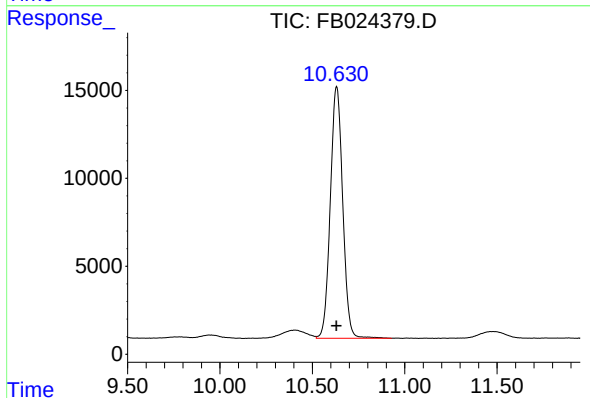


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 667428
Conc: 18.42 ng/ml

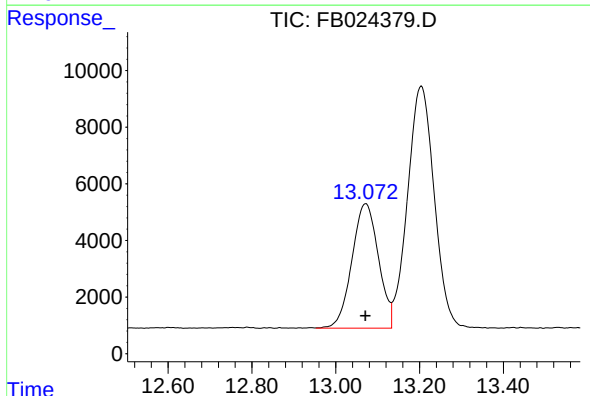


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 192939
Conc: 5.69 ng/ml

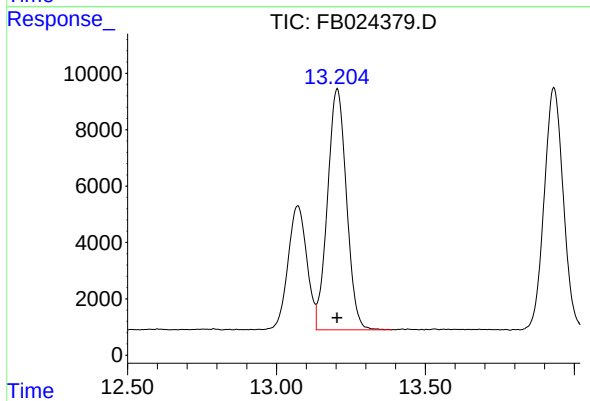


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 378689
Conc: 11.48 ng/ml

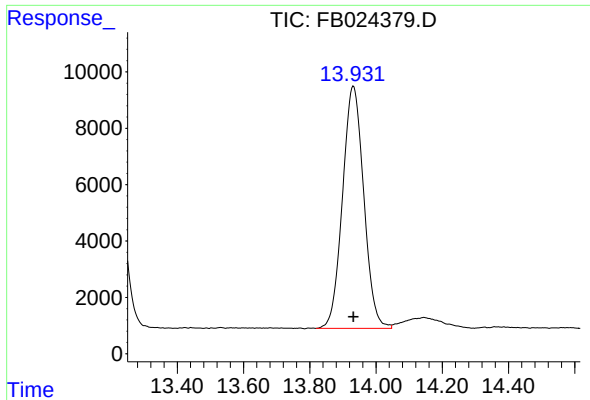

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 382845
Conc: 11.86 ng/ml

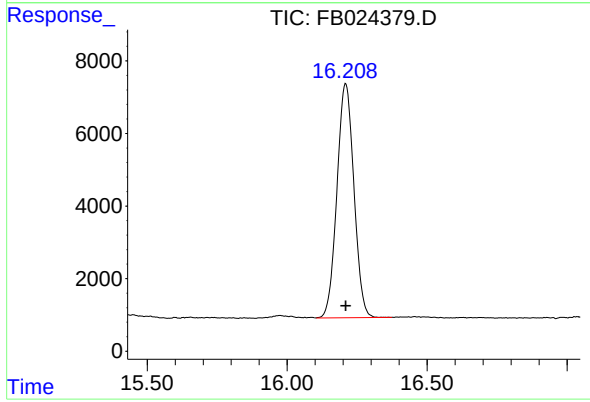

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 271519
Conc: 10.07 ng/ml