

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052125\
Data File : FB031798.D
Signal(s) : FID2B.CH
Acq On : 21 May 2025 9:44
Operator : YP/AJ
Sample : VBF0521S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0521S1

Integration File: Calibration.e
Quant Time: May 22 01:47:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051925.M
Quant Title :
QLast Update : Mon May 19 10:47:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	424510	19.632 ng/ml
Target Compounds			
6) t Toluene	10.619	5355	0.121 ng/ml
8) t m-Xylene	13.191	7998	0.185 ng/ml
9) t O-Xylene	13.915	10689	0.268 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	15610	0.547 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052125\
Data File : FB031798.D
Signal(s) : FID2B.CH
Acq On : 21 May 2025 9:44
Operator : YP/AJ
Sample : VBF0521S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0521S1

Integration File: Calibration.e
Quant Time: May 22 01:47:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051925.M
Quant Title :
QLast Update : Mon May 19 10:47:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

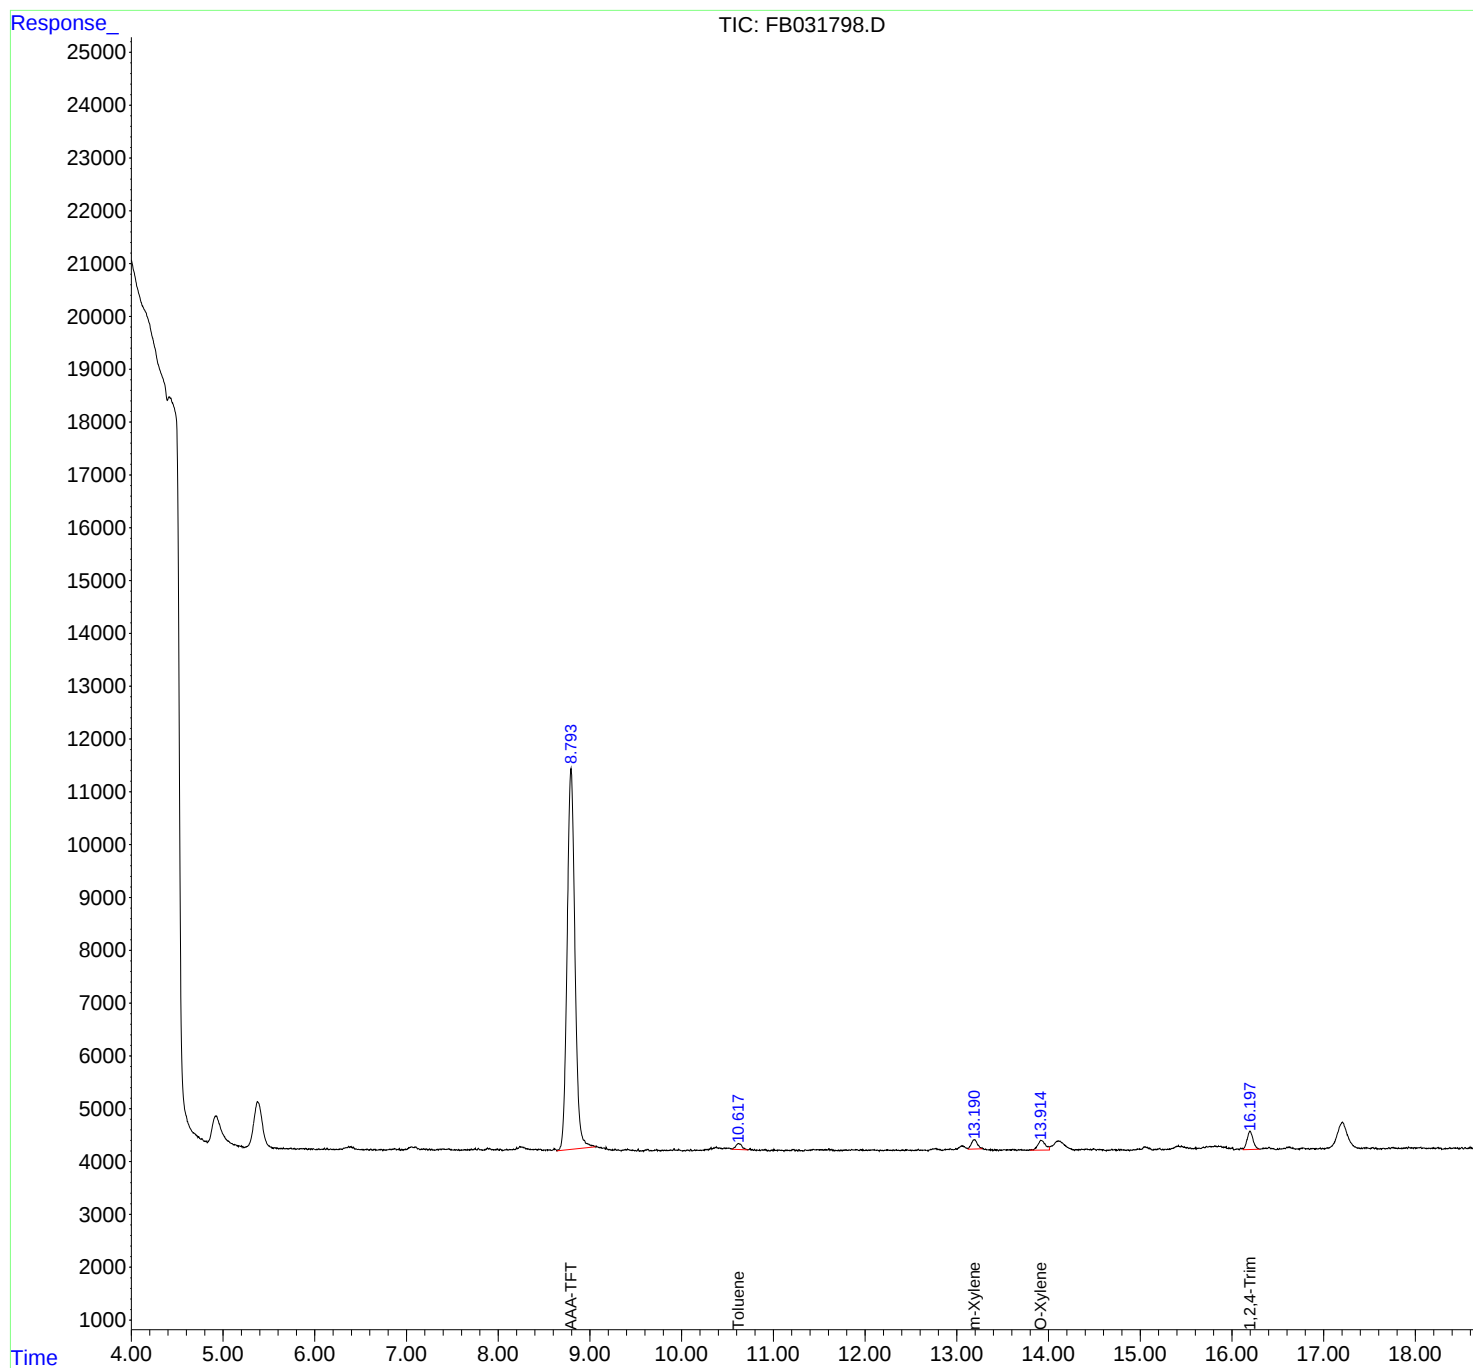


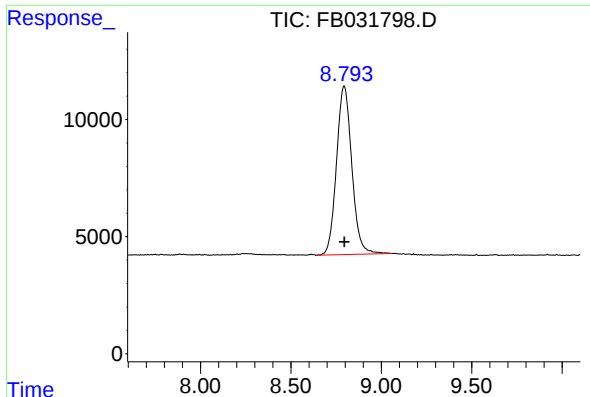

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.001 min
Response: 424510
Conc: 19.63 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0521S1

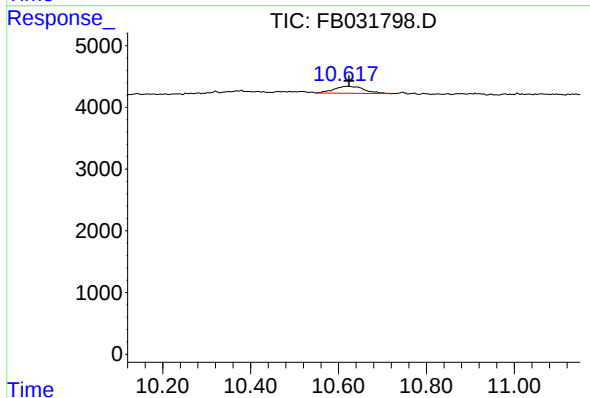


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.005 min
Response: 5355
Conc: 0.12 ng/ml

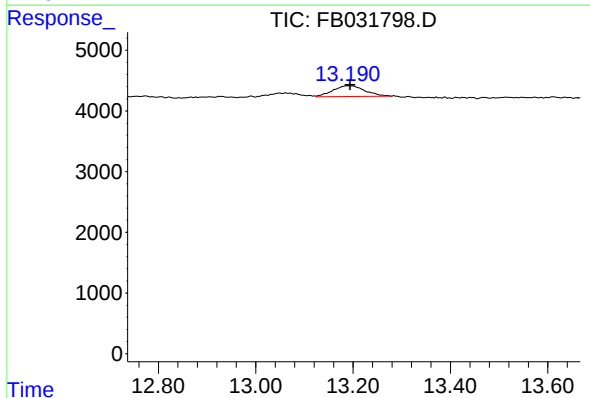


#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: -0.003 min
Response: 7998
Conc: 0.19 ng/ml

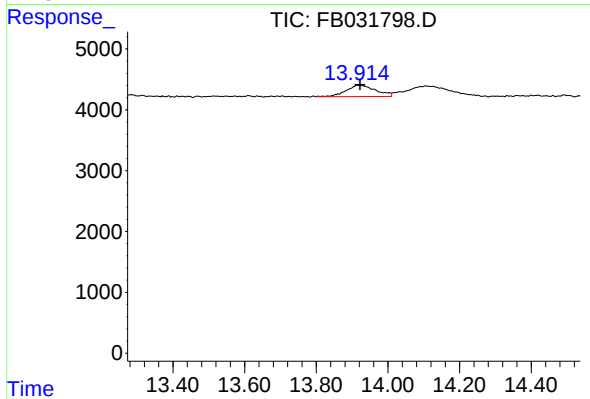

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: -0.007 min
Response: 10689
Conc: 0.27 ng/ml

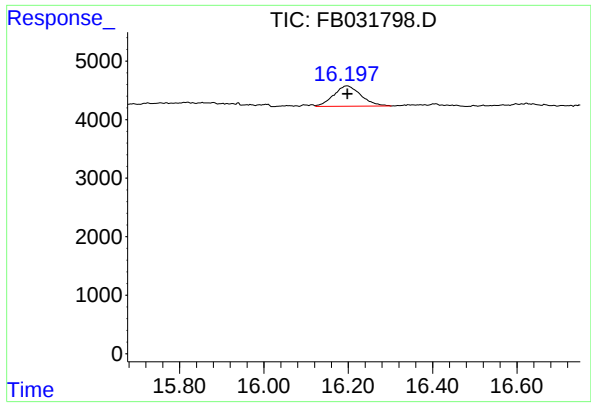

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.000 min
Response: 15610
Conc: 0.55 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0521S1