

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052125\
Data File : FB031801.D
Signal(s) : FID2B.CH
Acq On : 21 May 2025 11:08
Operator : YP/AJ
Sample : Q2074-05 50X
Misc : 6.90G/5.00 ML MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-38

Integration File: Calibration.e
Quant Time: May 22 01:48:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051925.M
Quant Title :
QLast Update : Mon May 19 10:47:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	497848	23.023 ng/ml
Target Compounds			
6) t Toluene	10.632	9240	0.209 ng/ml
8) t m-Xylene	13.190	10515	0.244 ng/ml
9) t O-Xylene	13.933	12764	0.320 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	14370	0.504 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052125\
Data File : FB031801.D
Signal(s) : FID2B.CH
Acq On : 21 May 2025 11:08
Operator : YP/AJ
Sample : Q2074-05 50X
Misc : 6.90G/5.00 ML MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-38

Integration File: Calibration.e
Quant Time: May 22 01:48:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051925.M
Quant Title :
QLast Update : Mon May 19 10:47:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

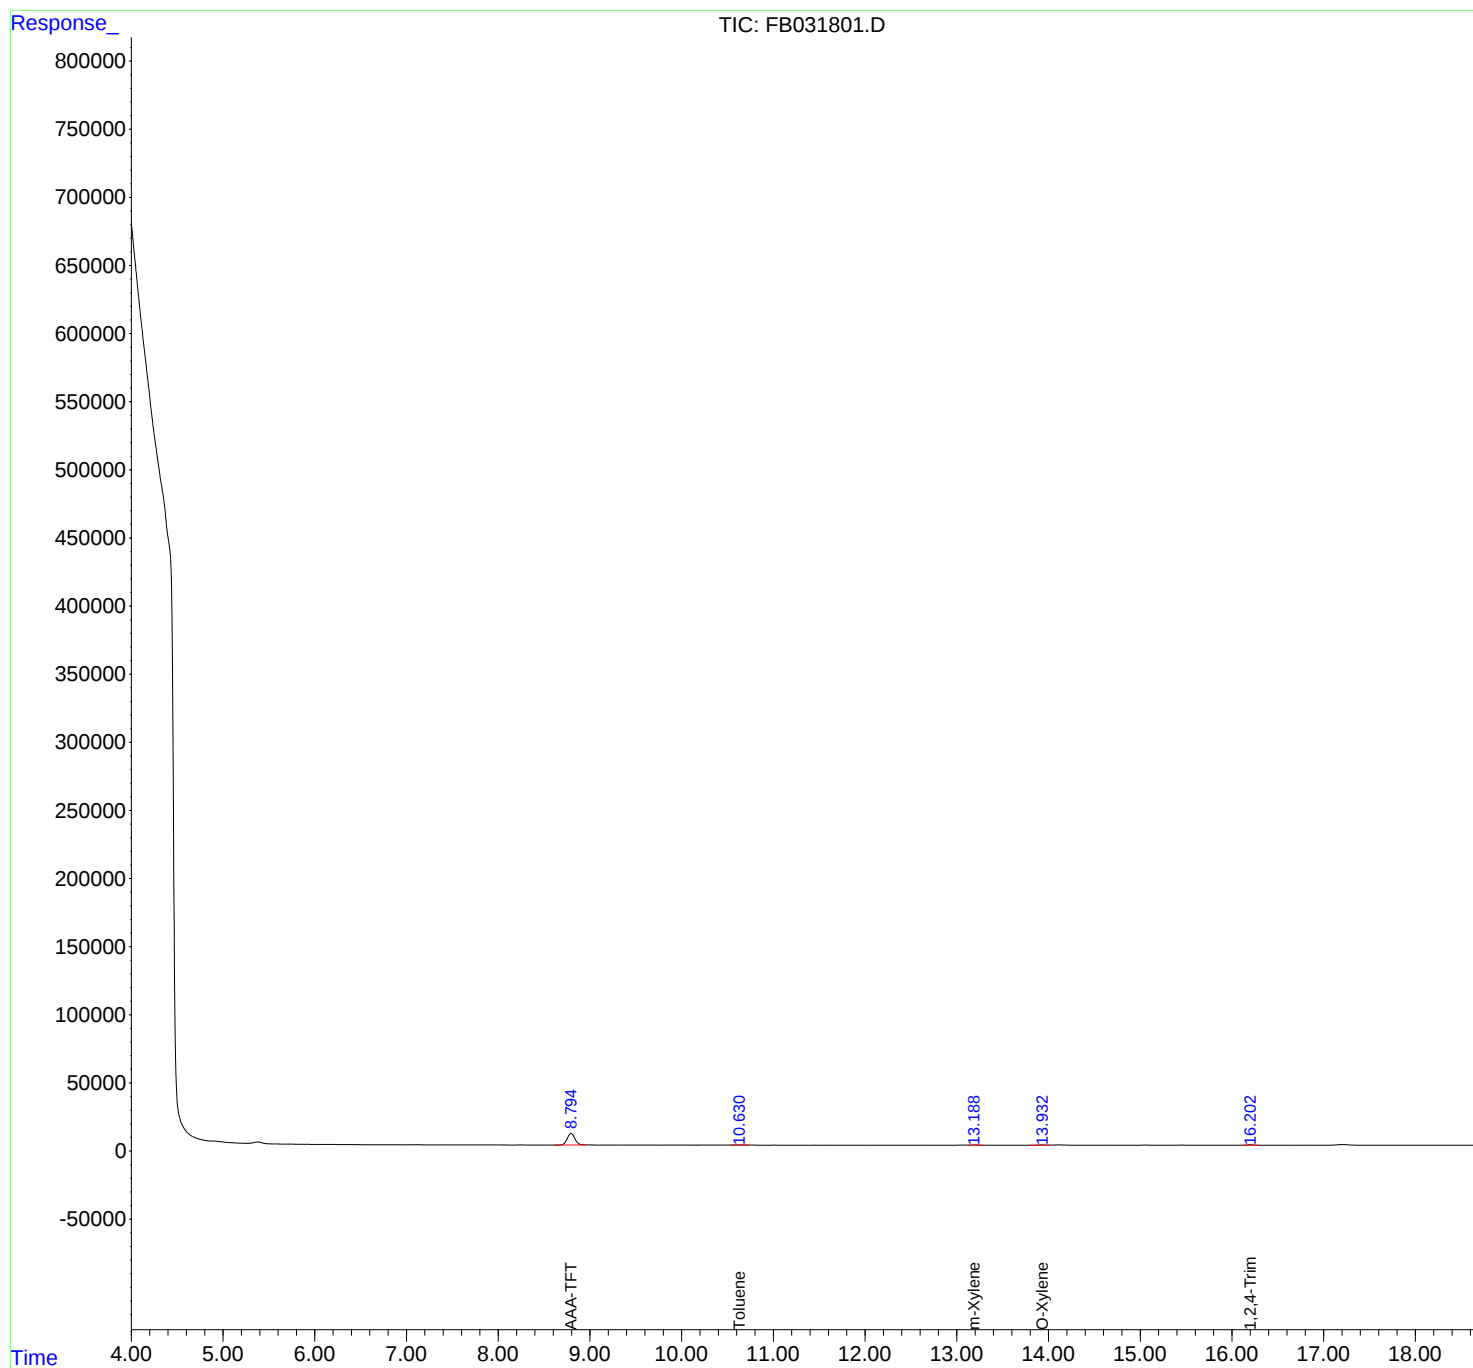


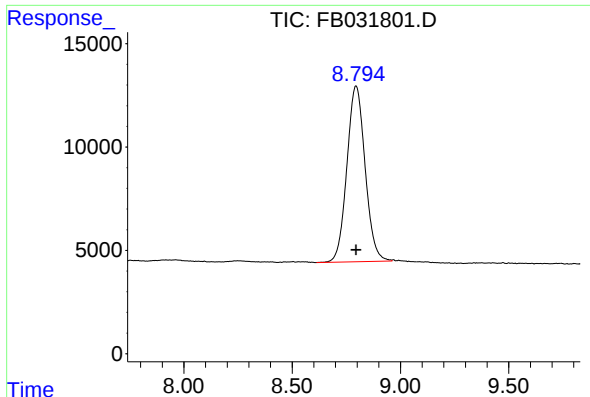

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.000 min
Response: 497848
Conc: 23.02 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-38

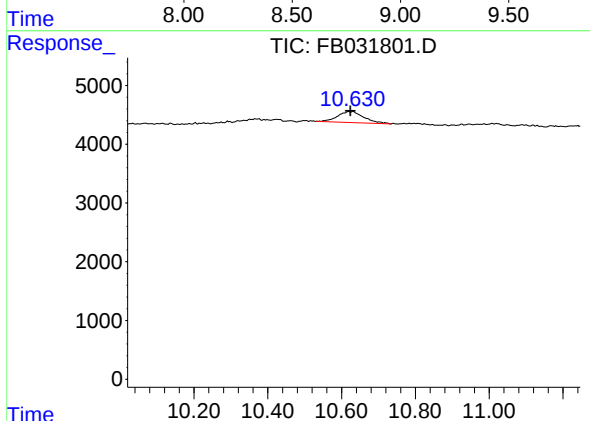


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.008 min
Response: 9240
Conc: 0.21 ng/ml

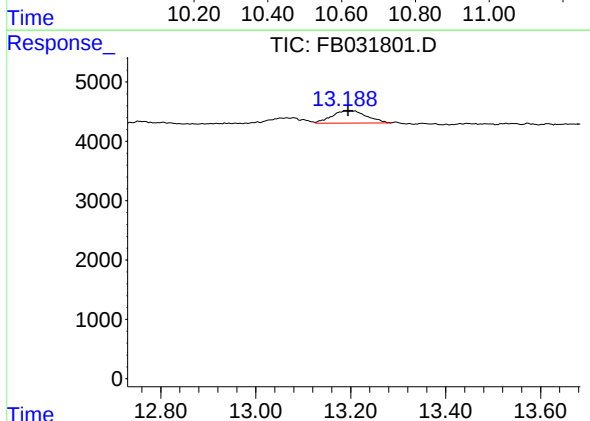


#8 m-Xylene

R.T.: 13.190 min
Delta R.T.: -0.004 min
Response: 10515
Conc: 0.24 ng/ml

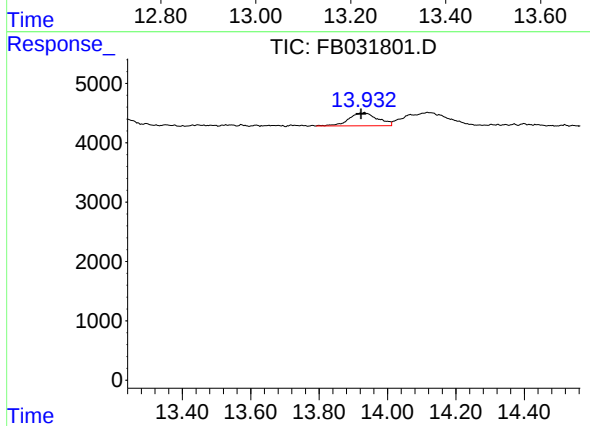

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.011 min
Response: 12764
Conc: 0.32 ng/ml

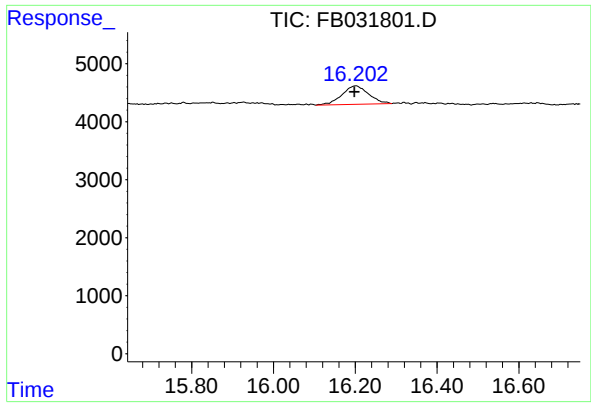

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: 0.005 min
Response: 14370
Conc: 0.50 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-38