

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052125\
Data File : FB031806.D
Signal(s) : FID2B.CH
Acq On : 21 May 2025 14:34
Operator : YP/AJ
Sample : Q2100-01
Misc : 5.77G/5.00 ML DI WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-16

Integration File: Calibration.e
Quant Time: May 22 01:49:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051925.M
Quant Title :
QLast Update : Mon May 19 10:47:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	324621	15.012 ng/ml
Target Compounds			
6) t Toluene	10.630	6162	0.140 ng/ml
8) t m-Xylene	13.201	4645	0.108 ng/ml
9) t O-Xylene	13.919	5434	0.136 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	15667	0.549 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052125\
Data File : FB031806.D
Signal(s) : FID2B.CH
Acq On : 21 May 2025 14:34
Operator : YP/AJ
Sample : Q2100-01
Misc : 5.77G/5.00 ML DI WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-16

Integration File: Calibration.e
Quant Time: May 22 01:49:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051925.M
Quant Title :
QLast Update : Mon May 19 10:47:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

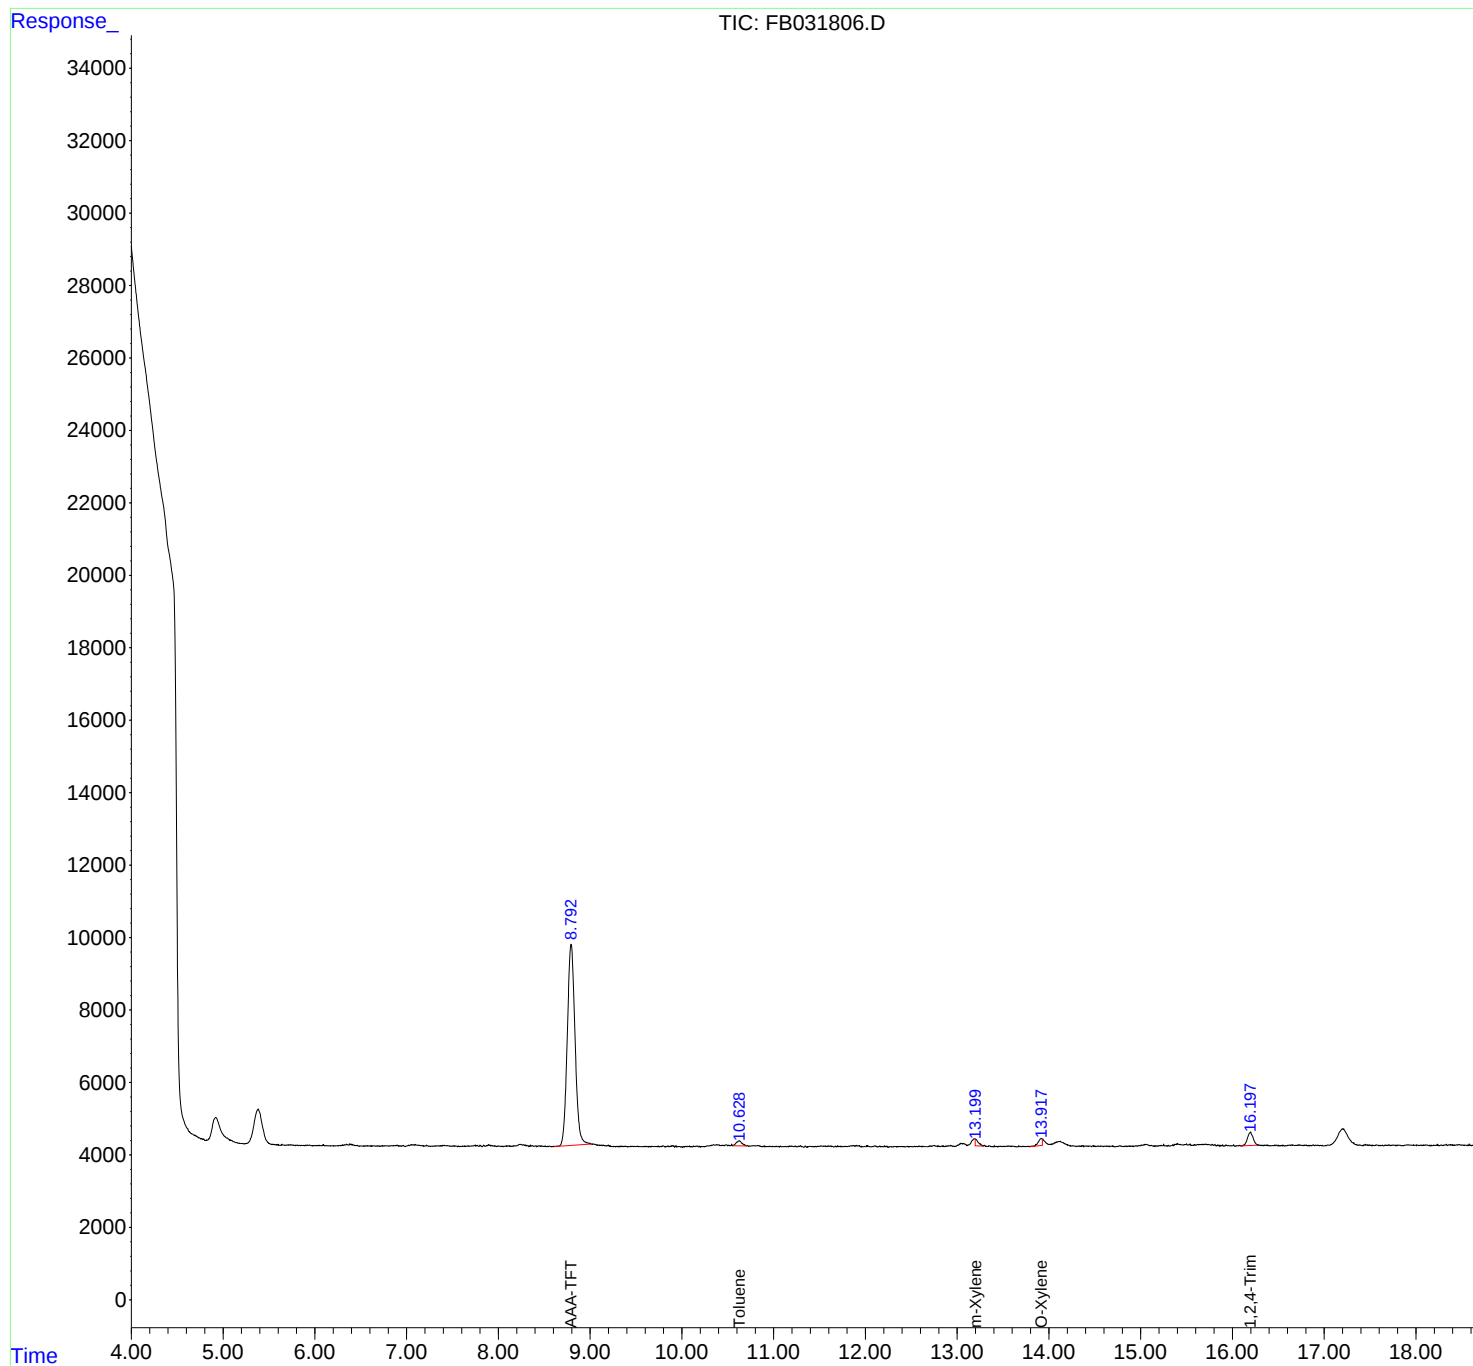


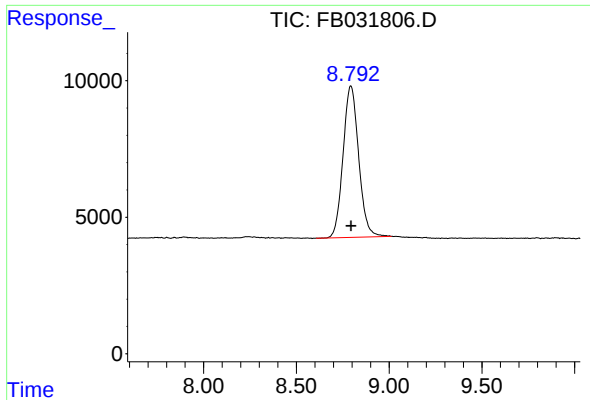

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: -0.002 min
Response: 324621
Conc: 15.01 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-16

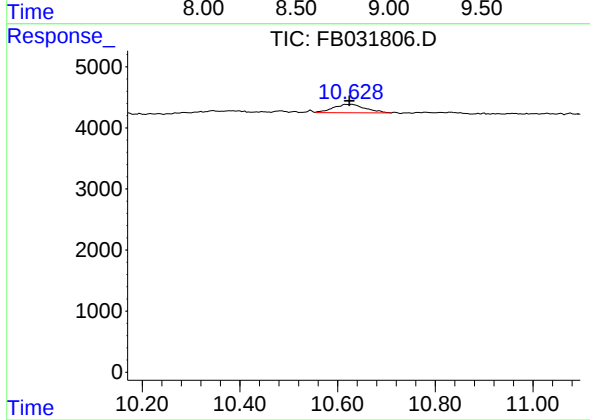


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.005 min
Response: 6162
Conc: 0.14 ng/ml

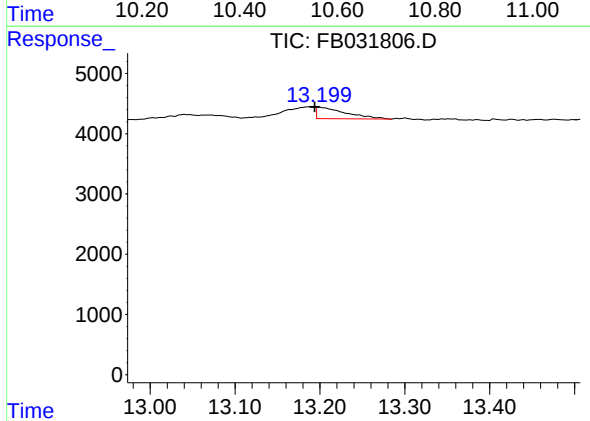


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: 0.007 min
Response: 4645
Conc: 0.11 ng/ml

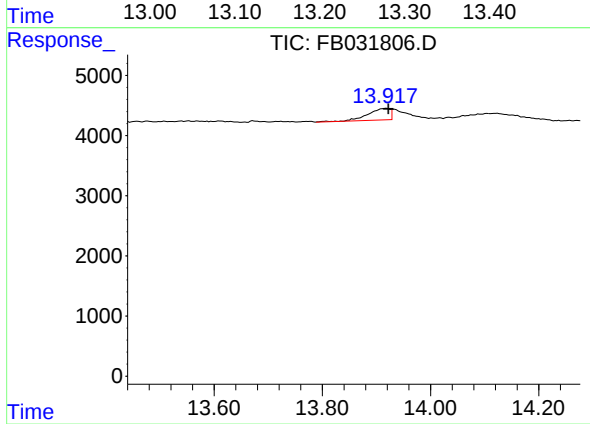

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: -0.003 min
Response: 5434
Conc: 0.14 ng/ml

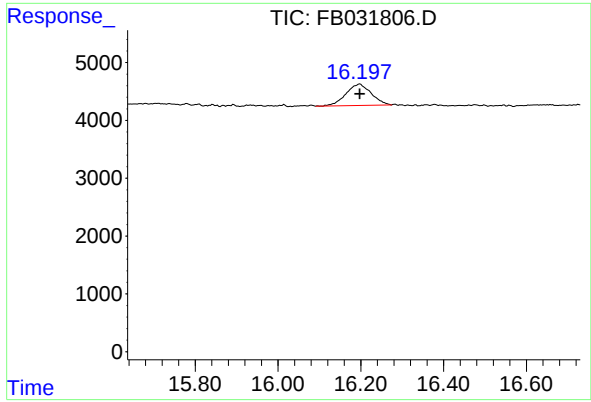

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.000 min
Response: 15667
Conc: 0.55 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-16