

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052219\
 Data File : FB021154.D
 Signal(s) : FID2B.CH
 Acq On : 22 May 2019 12:47
 Operator : MJ/SJ
 Sample : K2978-02MSD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 23 00:55:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
 Quant Title :
 QLast Update : Mon Apr 29 15:53:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.993	305611	17.036 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.855	793851	17.599 ng/ml
2) t 2,2,4-Trimethylpentane	7.610	512955	12.306 ng/ml
3) t n-Heptane	7.949	150553	3.803 ng/ml
4) t Benzene	8.085	352764	8.432 ng/ml
6) t Toluene	10.837	662842	23.928 ng/ml
7) t Ethylbenzene	13.288	200001	7.131 ng/ml
8) t m-Xylene	13.421	425711	14.324 ng/ml
9) t O-Xylene	14.152	447657	14.442 ng/ml
10) t 1,2,4-Trimethylbenzene	16.437	391250	12.615 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052219\
Data File : FB021154.D
Signal(s) : FID2B.CH
Acq On : 22 May 2019 12:47
Operator : MJ/SJ
Sample : K2978-02MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 23 00:55:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
Quant Title :
QLast Update : Mon Apr 29 15:53:58 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

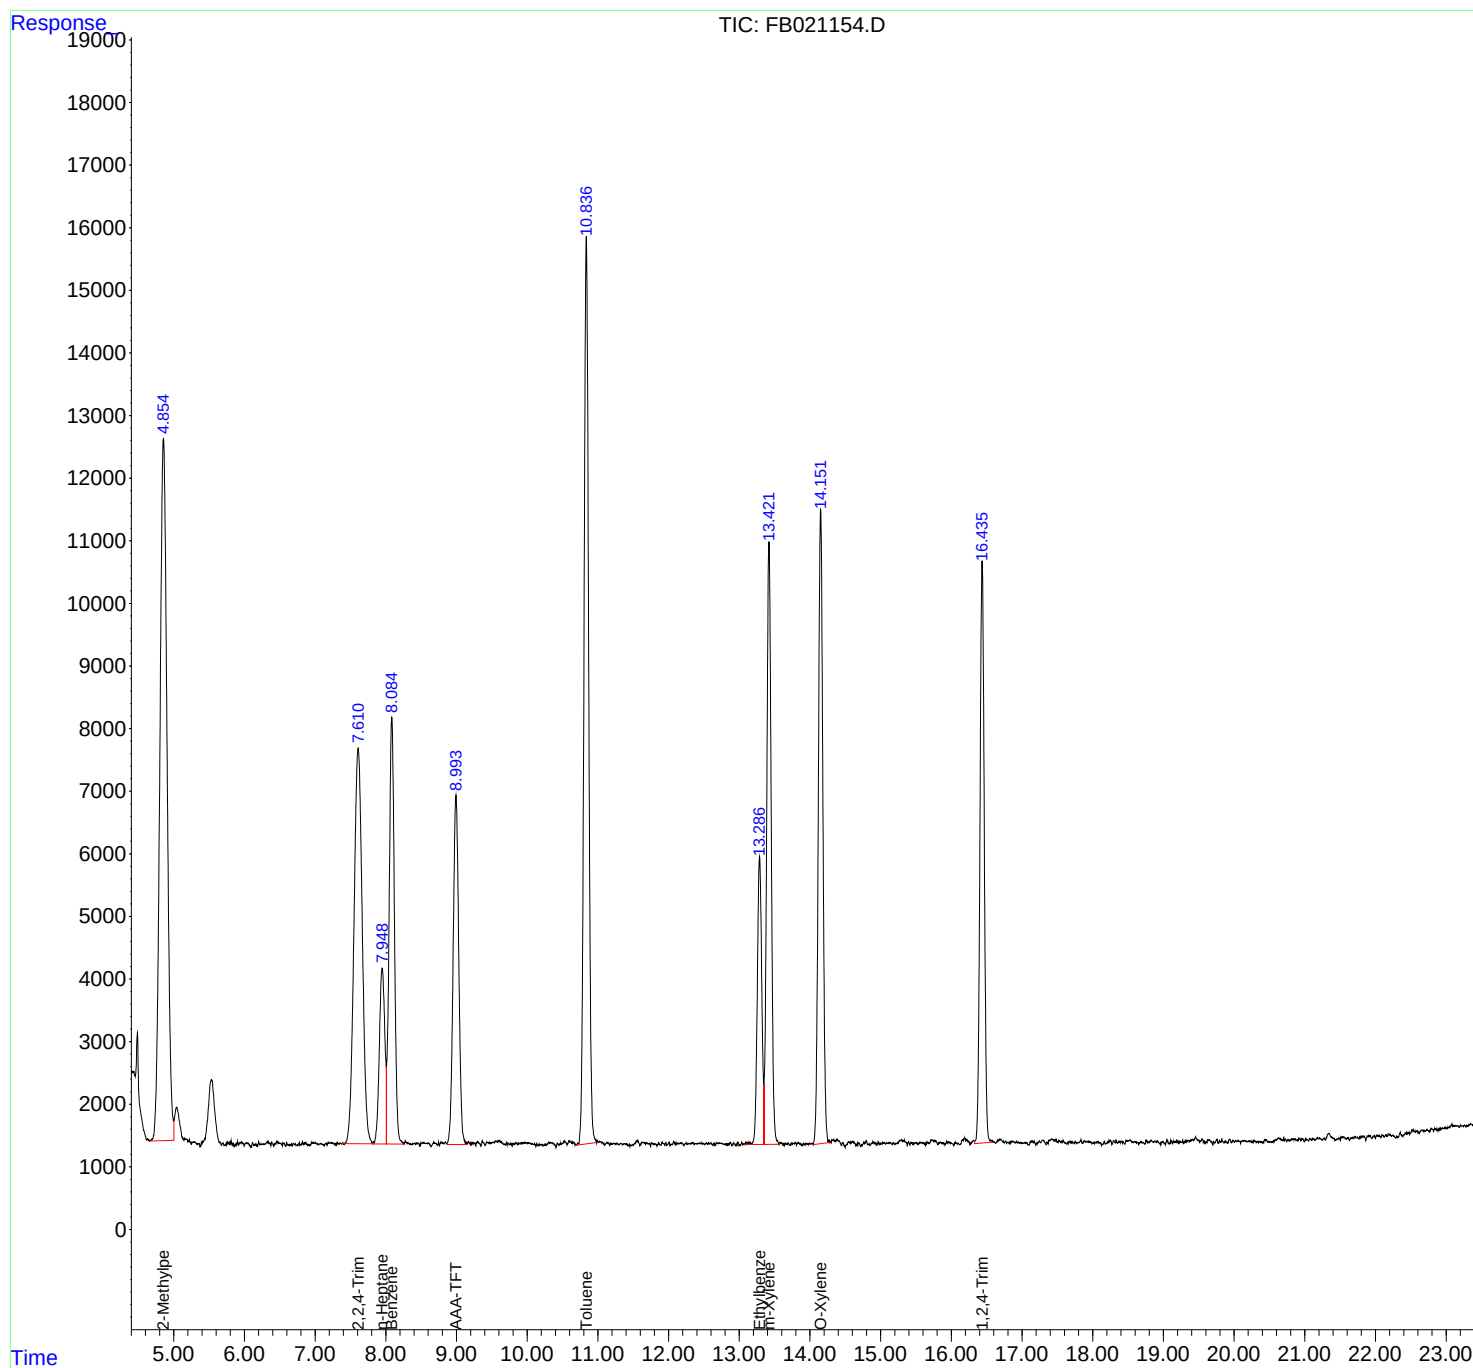

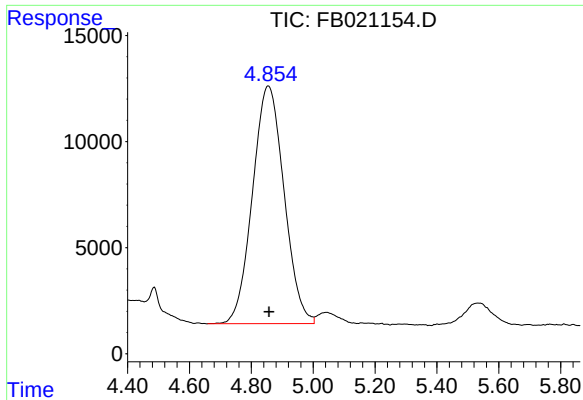


#1 2-Methylpentane

R.T.: 4.855 min
Delta R.T.: -0.002 min
Response: 793851
Conc: 17.60 ng/ml

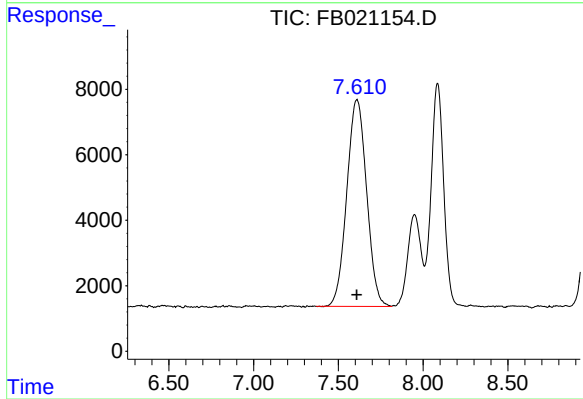


#2 2,2,4-Trimethylpentane

R.T.: 7.610 min
Delta R.T.: 0.000 min
Response: 512955
Conc: 12.31 ng/ml

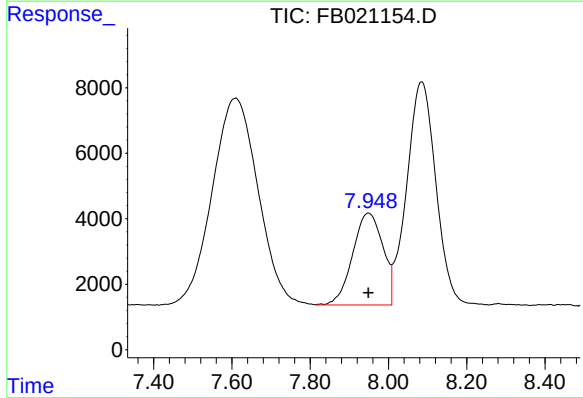


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: 0.000 min
Response: 150553
Conc: 3.80 ng/ml

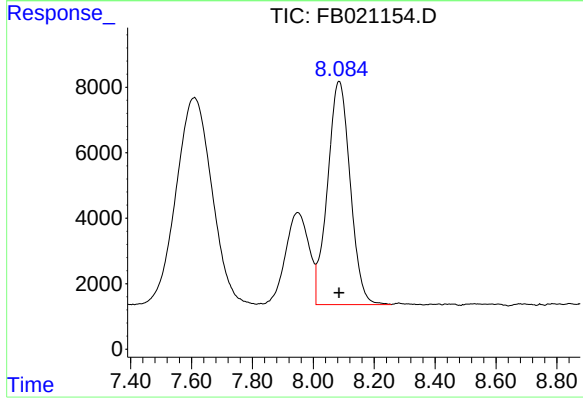


#4 Benzene

R.T.: 8.085 min
Delta R.T.: 0.000 min
Response: 352764
Conc: 8.43 ng/ml

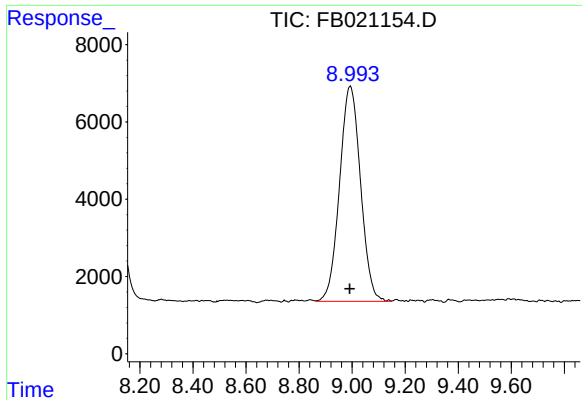


#5 AAA-TFT

R.T.: 8.993 min
Delta R.T.: 0.001 min
Response: 305611
Conc: 17.04 ng/ml

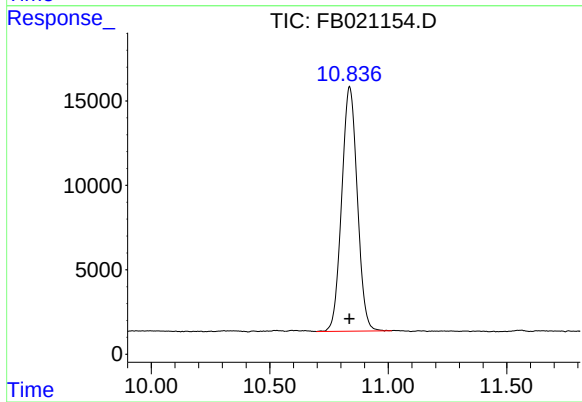


#6 Toluene

R.T.: 10.837 min
Delta R.T.: 0.002 min
Response: 662842
Conc: 23.93 ng/ml

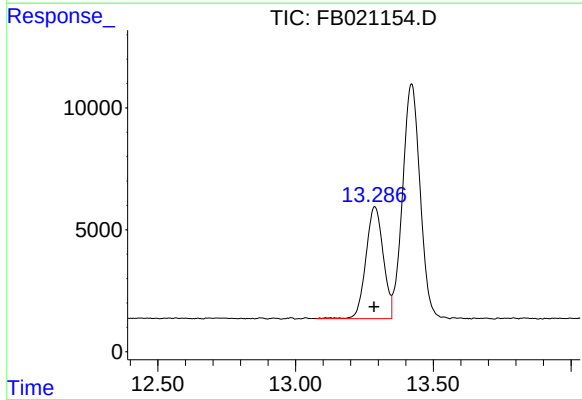


#7 Ethylbenzene

R.T.: 13.288 min
Delta R.T.: 0.002 min
Response: 200001
Conc: 7.13 ng/ml

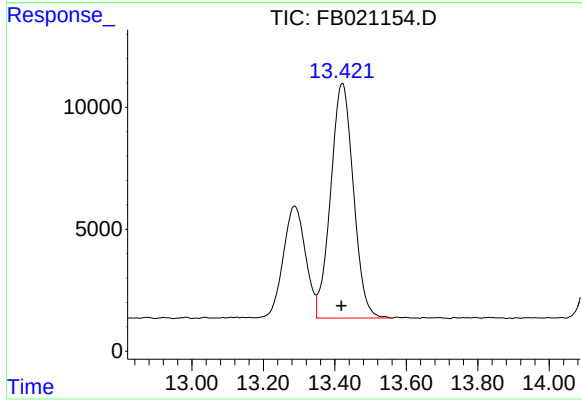

#8 m-Xylene

R.T.: 13.421 min
Delta R.T.: 0.003 min
Response: 425711
Conc: 14.32 ng/ml

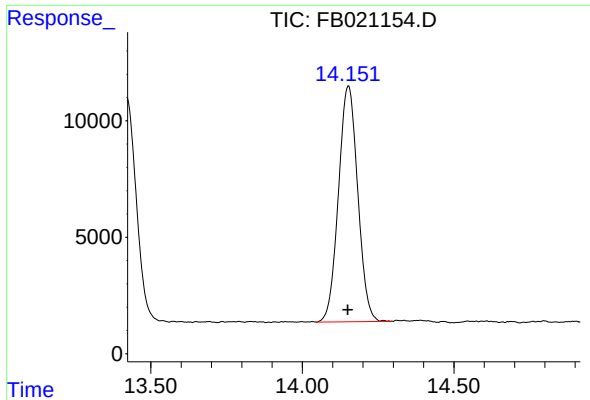


#9 O-Xylene

R.T.: 14.152 min

Delta R.T.: 0.003 min

Response: 447657

Conc: 14.44 ng/ml

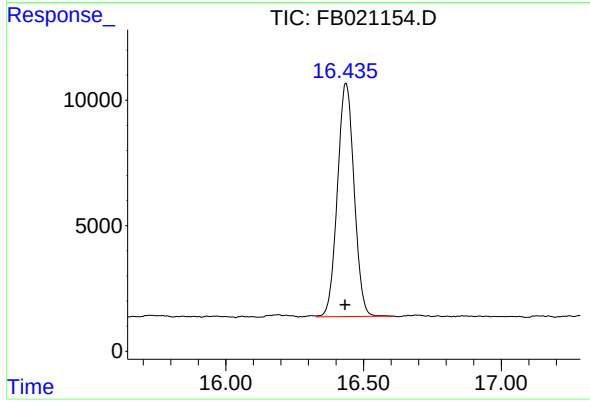

#10 1,2,4-Trimethylbenzene

R.T.: 16.437 min

Delta R.T.: 0.004 min

Response: 391250

Conc: 12.62 ng/ml