

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052219\
 Data File : FB021150.D
 Signal(s) : FID2B.CH
 Acq On : 22 May 2019 9:58
 Operator : MJ/SJ
 Sample : BSF0522S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 23 00:54:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
 Quant Title :
 QLast Update : Mon Apr 29 15:53:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.993	355474	19.815 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.854	1299452	28.807 ng/ml
2) t	2,2,4-Trimethylpentane	7.608	1252694	30.052 ng/ml
3) t	n-Heptane	7.949	392249	9.908 ng/ml
4) t	Benzene	8.085	424991	10.159 ng/ml
6) t	Toluene	10.837	849999	30.684 ng/ml
7) t	Ethylbenzene	13.287	279609	9.970 ng/ml
8) t	m-Xylene	13.420	595742	20.045 ng/ml
9) t	O-Xylene	14.151	619803	19.996 ng/ml
10) t	1,2,4-Trimethylbenzene	16.436	623467	20.103 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052219\
Data File : FB021150.D
Signal(s) : FID2B.CH
Acq On : 22 May 2019 9:58
Operator : MJ/SJ
Sample : BSF0522S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 23 00:54:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
Quant Title :
QLast Update : Mon Apr 29 15:53:58 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

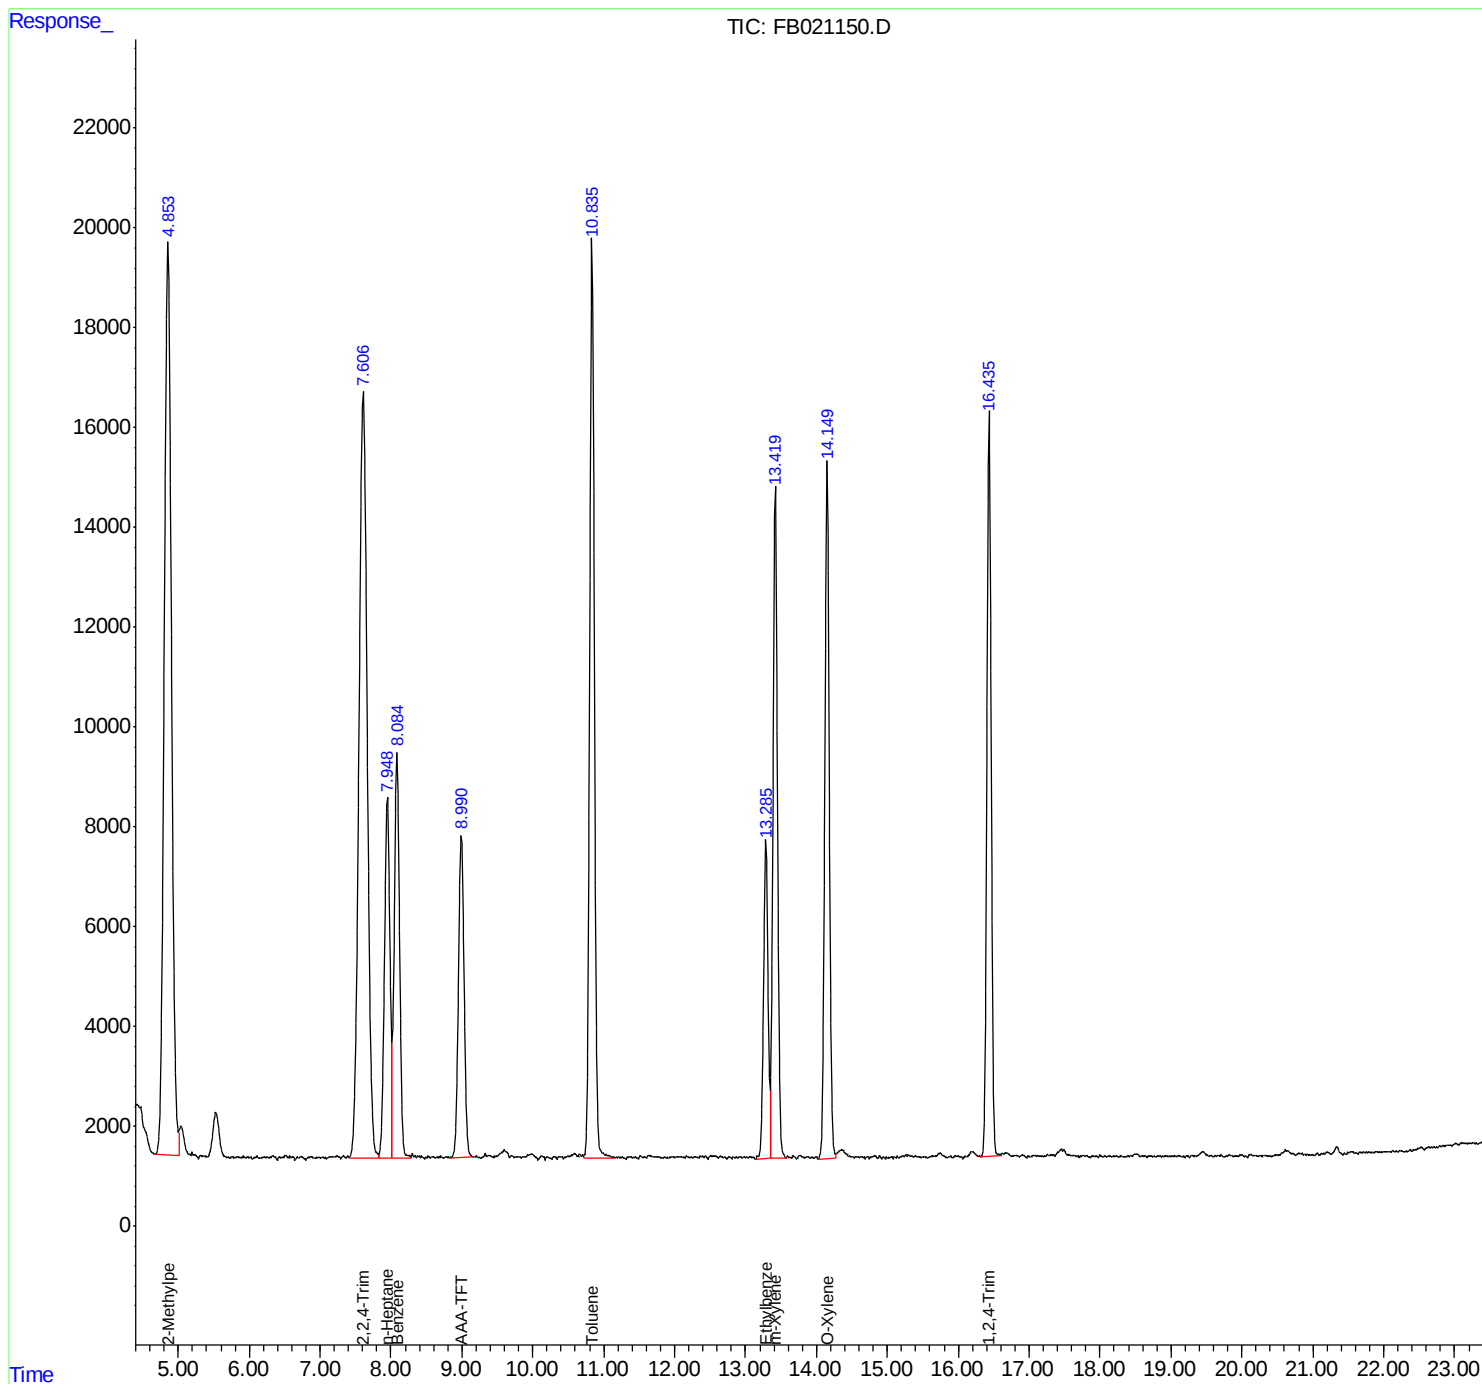

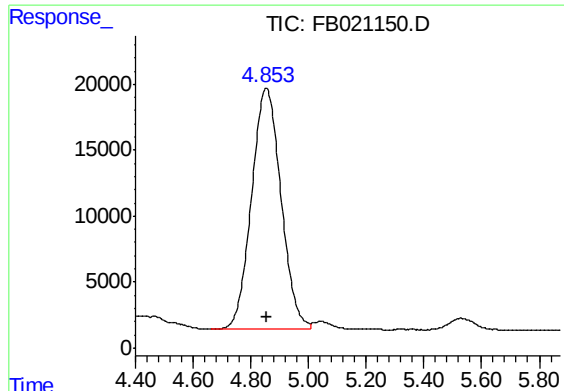


#1 2-Methylpentane

R.T.: 4.854 min
Delta R.T.: -0.003 min
Response: 1299452
Conc: 28.81 ng/ml

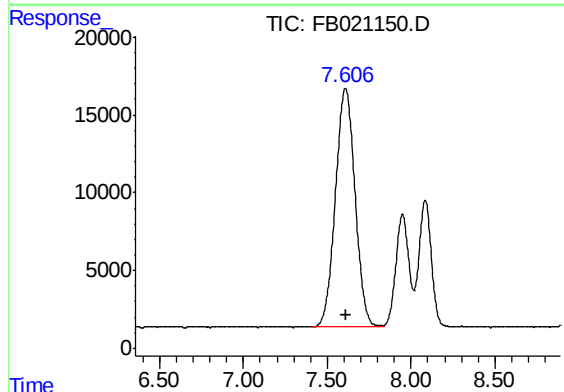


#2 2,2,4-Trimethylpentane

R.T.: 7.608 min
Delta R.T.: 0.000 min
Response: 1252694
Conc: 30.05 ng/ml

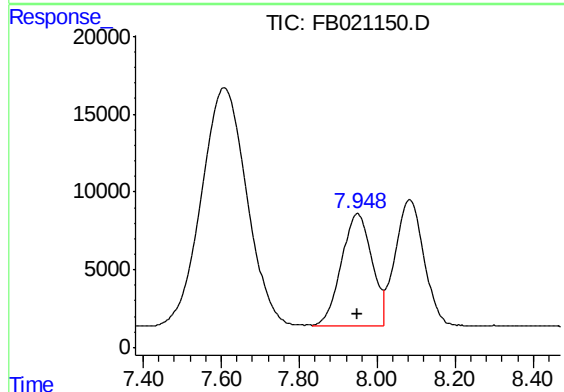


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: 0.000 min
Response: 392249
Conc: 9.91 ng/ml

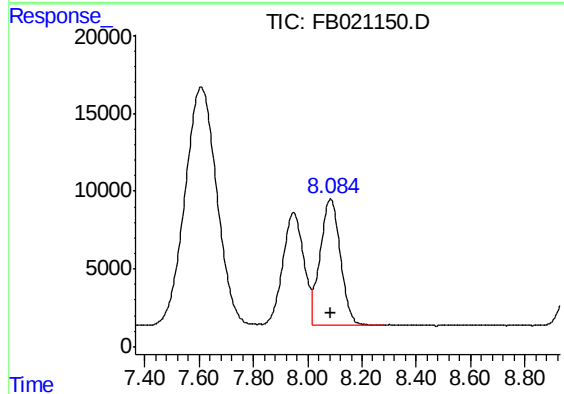


#4 Benzene

R.T.: 8.085 min
Delta R.T.: 0.000 min
Response: 424991
Conc: 10.16 ng/ml

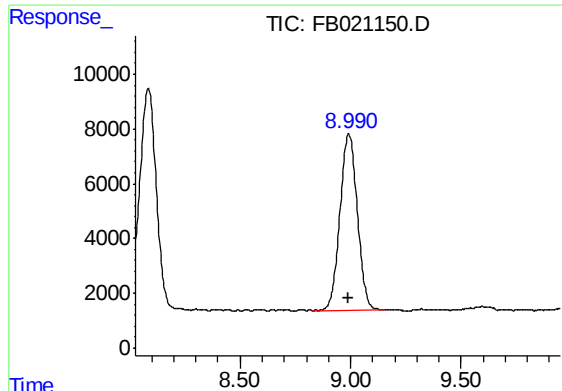


#5 AAA-TFT

R.T.: 8.993 min
Delta R.T.: 0.000 min
Response: 355474
Conc: 19.82 ng/ml

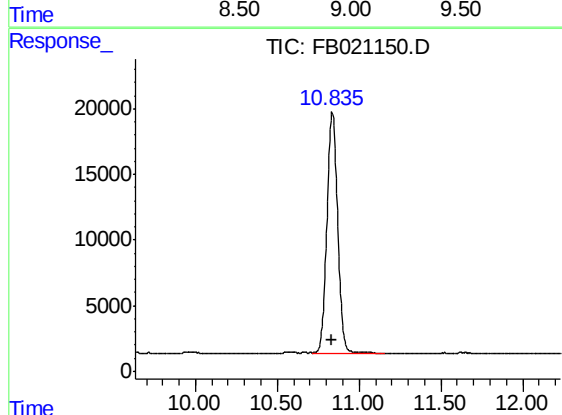


#6 Toluene

R.T.: 10.837 min
Delta R.T.: 0.001 min
Response: 849999
Conc: 30.68 ng/ml

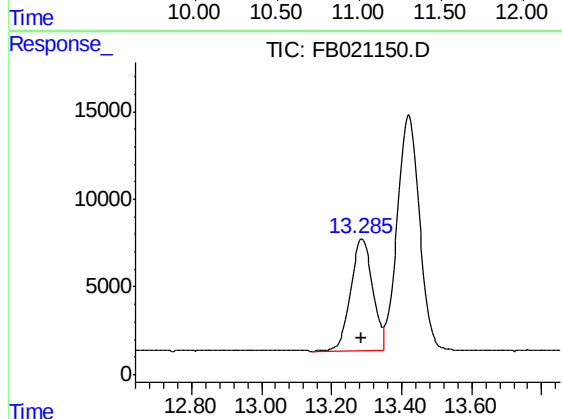


#7 Ethylbenzene

R.T.: 13.287 min
Delta R.T.: 0.001 min
Response: 279609
Conc: 9.97 ng/ml

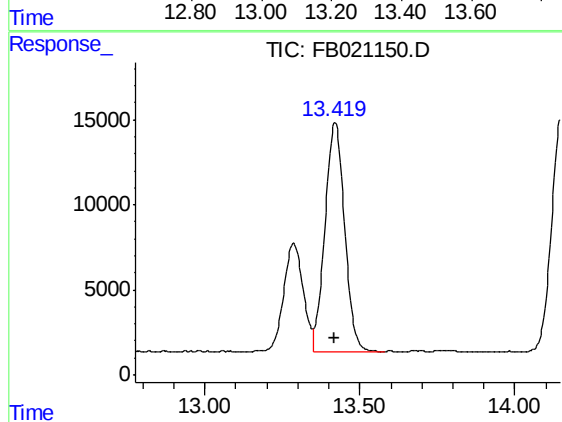


#8 m-Xylene

R.T.: 13.420 min
Delta R.T.: 0.002 min
Response: 595742
Conc: 20.04 ng/ml

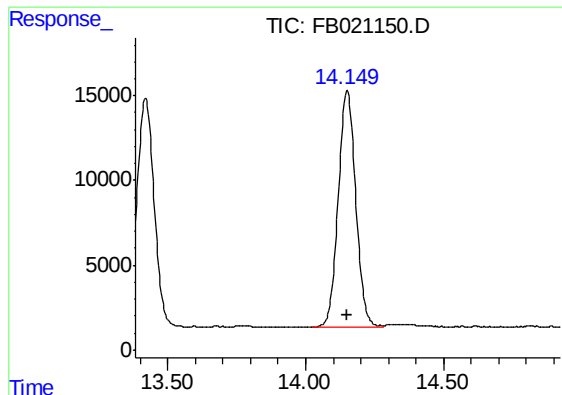

#9 O-Xylene

R.T.: 14.151 min
Delta R.T.: 0.002 min
Response: 619803
Conc: 20.00 ng/ml

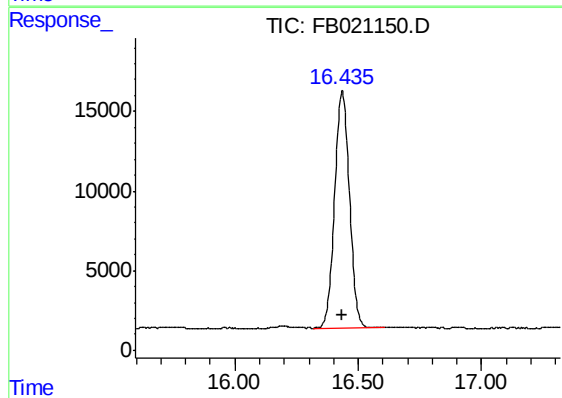

#10 1,2,4-Trimethylbenzene

R.T.: 16.436 min
Delta R.T.: 0.003 min
Response: 623467
Conc: 20.10 ng/ml