

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052319\
 Data File : FB021173.D
 Signal(s) : FID2B.CH
 Acq On : 23 May 2019 12:06
 Operator : MJ/SJ
 Sample : K2647-11MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 24 00:44:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
 Quant Title :
 QLast Update : Mon Apr 29 15:53:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.992	360290	20.084 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.854	1113340	24.681 ng/ml
2) t 2,2,4-Trimethylpentane	7.608	836670	20.072 ng/ml
3) t n-Heptane	7.948	272827	6.892 ng/ml
4) t Benzene	8.084	415557	9.933 ng/ml
6) t Toluene	10.836	809249	29.213 ng/ml
7) t Ethylbenzene	13.287	246895	8.803 ng/ml
8) t m-Xylene	13.419	533335	17.945 ng/ml
9) t O-Xylene	14.151	556149	17.942 ng/ml
10) t 1,2,4-Trimethylbenzene	16.435	566309	18.260 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052319\
Data File : FB021173.D
Signal(s) : FID2B.CH
Acq On : 23 May 2019 12:06
Operator : MJ/SJ
Sample : K2647-11MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 24 00:44:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
Quant Title :
QLast Update : Mon Apr 29 15:53:58 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

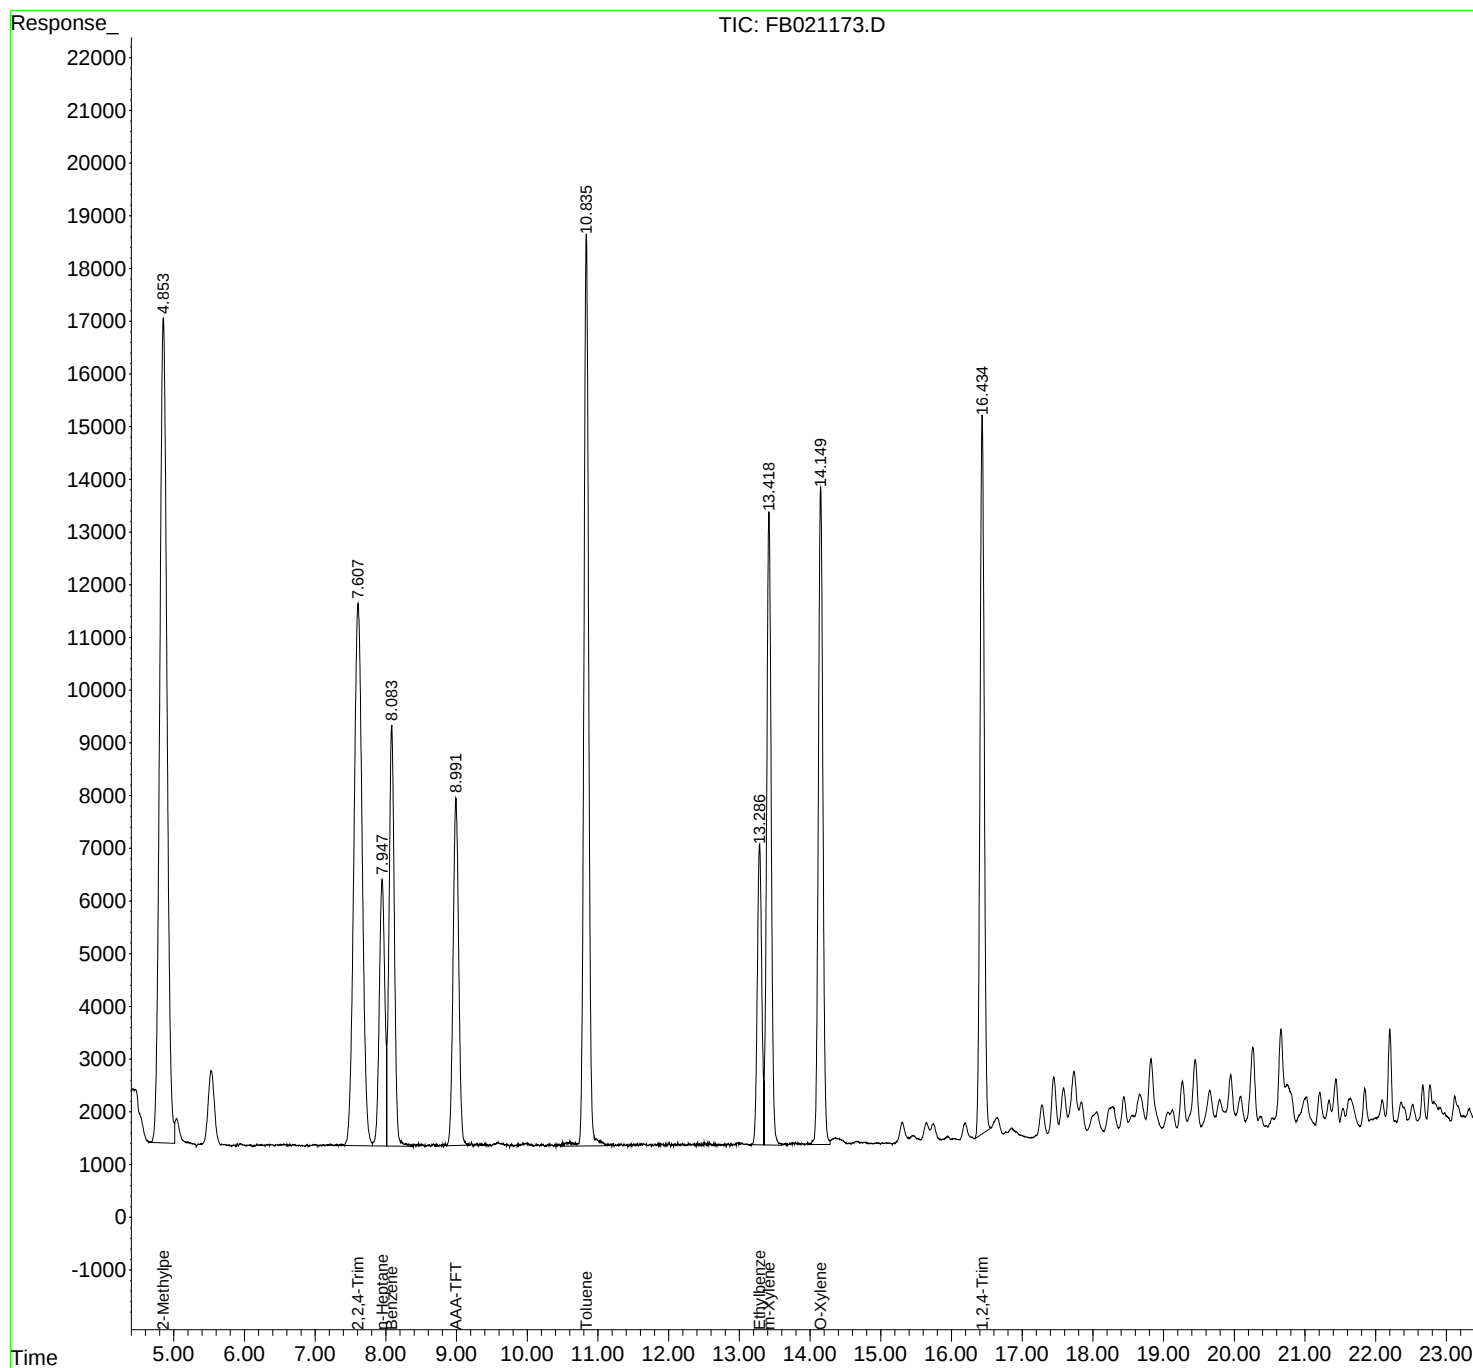

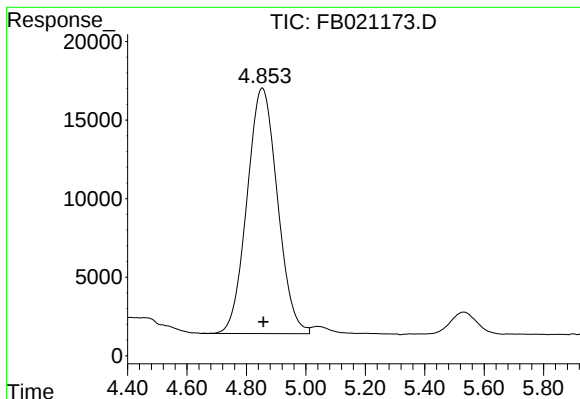


#1 2-Methylpentane

R.T.: 4.854 min
 Delta R.T.: -0.003 min
 Response: 1113340
 Conc: 24.68 ng/ml

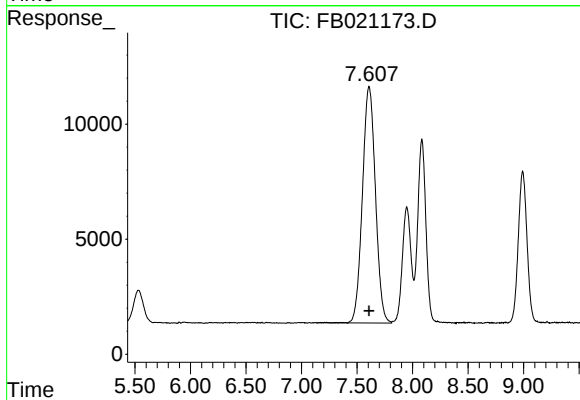


#2 2,2,4-Trimethylpentane

R.T.: 7.608 min
 Delta R.T.: -0.001 min
 Response: 836670
 Conc: 20.07 ng/ml

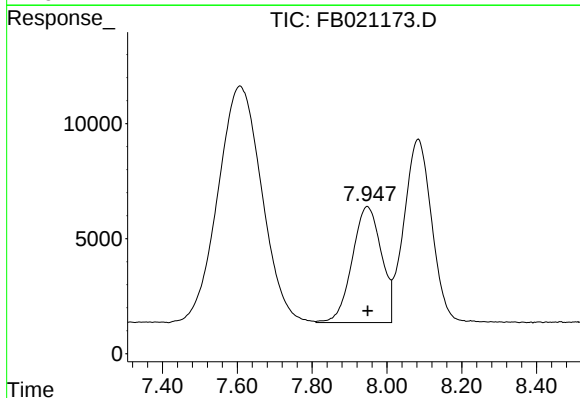


#3 n-Heptane

R.T.: 7.948 min
 Delta R.T.: 0.000 min
 Response: 272827
 Conc: 6.89 ng/ml

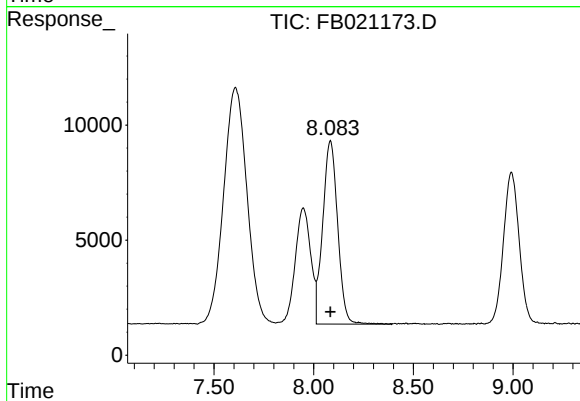


#4 Benzene

R.T.: 8.084 min
 Delta R.T.: 0.000 min
 Response: 415557
 Conc: 9.93 ng/ml

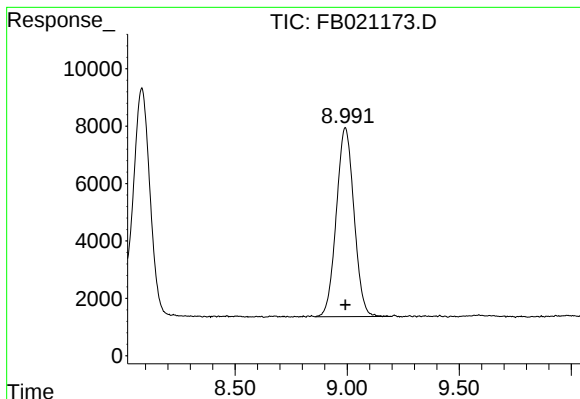


#5 AAA-TFT

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 360290
Conc: 20.08 ng/ml

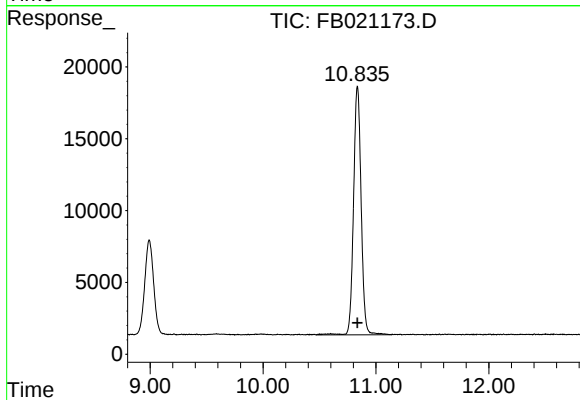


#6 Toluene

R.T.: 10.836 min
Delta R.T.: 0.000 min
Response: 809249
Conc: 29.21 ng/ml

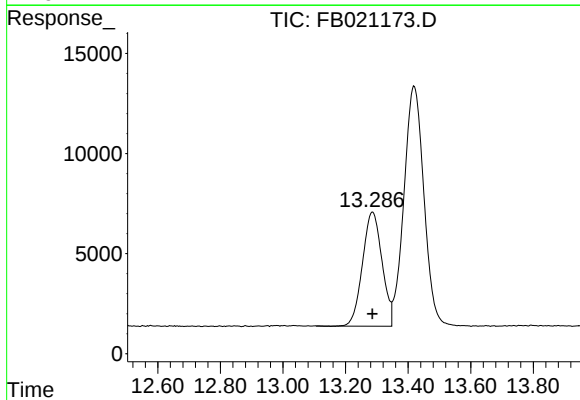


#7 Ethylbenzene

R.T.: 13.287 min
Delta R.T.: 0.000 min
Response: 246895
Conc: 8.80 ng/ml

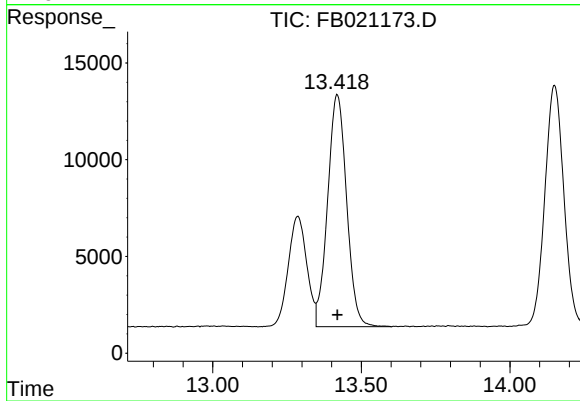


#8 m-Xylene

R.T.: 13.419 min
Delta R.T.: 0.000 min
Response: 533335
Conc: 17.95 ng/ml

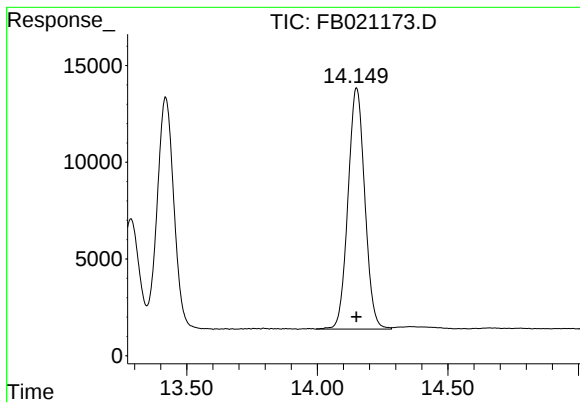

#9 O-Xylene

R.T.: 14.151 min
Delta R.T.: 0.001 min
Response: 556149
Conc: 17.94 ng/ml

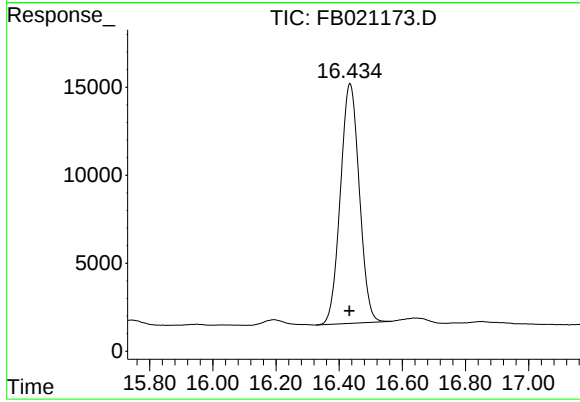

#10 1,2,4-Trimethylbenzene

R.T.: 16.435 min
Delta R.T.: 0.002 min
Response: 566309
Conc: 18.26 ng/ml