

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052419\
 Data File : FB021192.D
 Signal(s) : FID2B.CH
 Acq On : 24 May 2019 9:27
 Operator : MJ/SJ
 Sample : BSF0524S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 24 22:36:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
 Quant Title :
 QLast Update : Mon Apr 29 15:53:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.994	369418	20.593 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.856	1310476	29.052 ng/ml
2) t 2,2,4-Trimethylpentane	7.610	1244562	29.857 ng/ml
3) t n-Heptane	7.950	389423	9.837 ng/ml
4) t Benzene	8.086	418051	9.993 ng/ml
6) t Toluene	10.839	846572	30.560 ng/ml
7) t Ethylbenzene	13.289	275904	9.838 ng/ml
8) t m-Xylene	13.422	592970	19.952 ng/ml
9) t O-Xylene	14.154	620335	20.013 ng/ml
10) t 1,2,4-Trimethylbenzene	16.438	632492	20.394 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052419\
Data File : FB021192.D
Signal(s) : FID2B.CH
Acq On : 24 May 2019 9:27
Operator : MJ/SJ
Sample : BSF0524S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 24 22:36:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
Quant Title :
QLast Update : Mon Apr 29 15:53:58 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

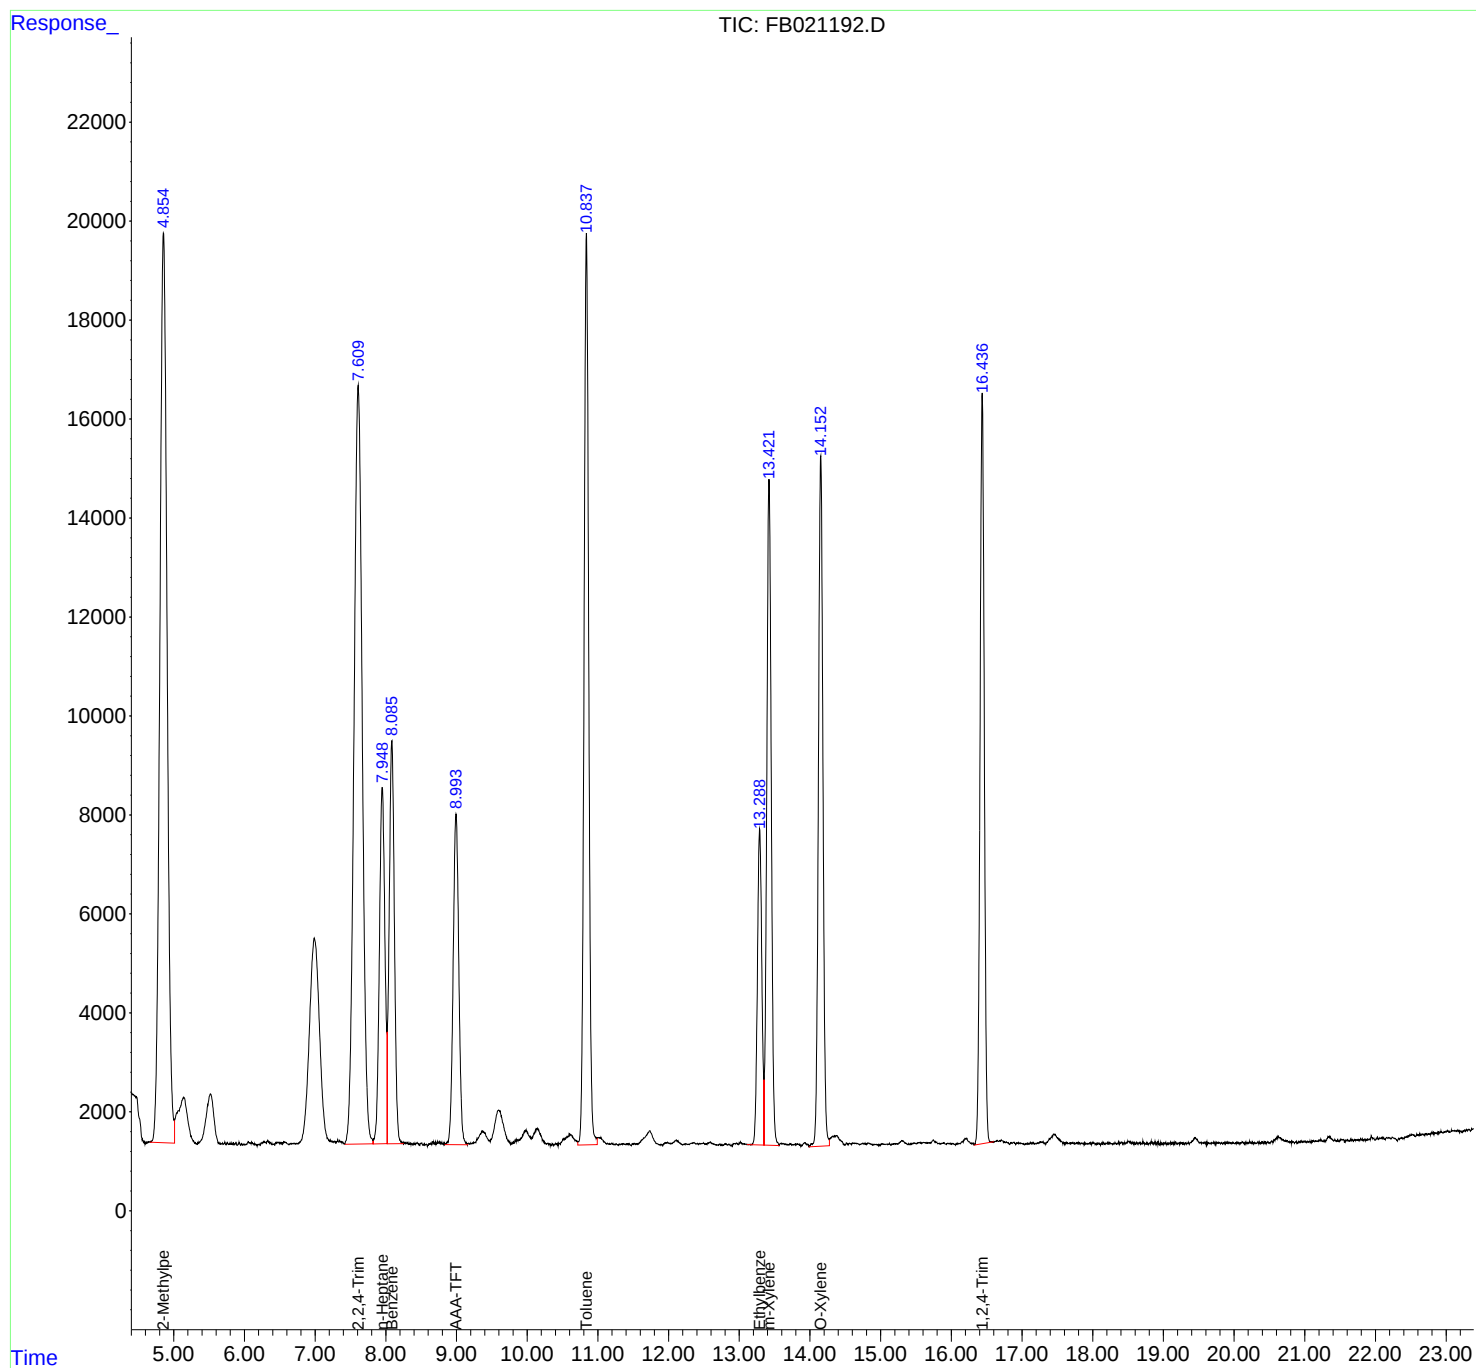

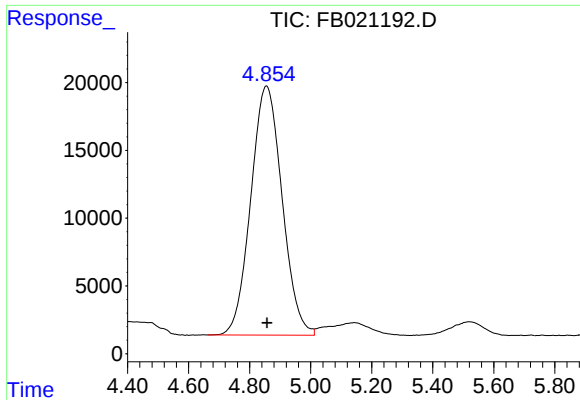


#1 2-Methylpentane

R.T.: 4.856 min
Delta R.T.: -0.001 min
Response: 1310476
Conc: 29.05 ng/ml

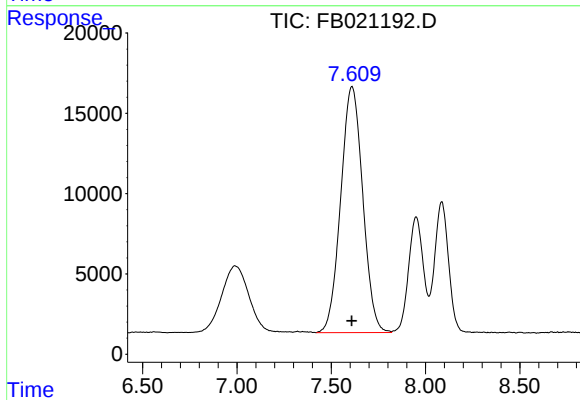


#2 2,2,4-Trimethylpentane

R.T.: 7.610 min
Delta R.T.: 0.000 min
Response: 1244562
Conc: 29.86 ng/ml

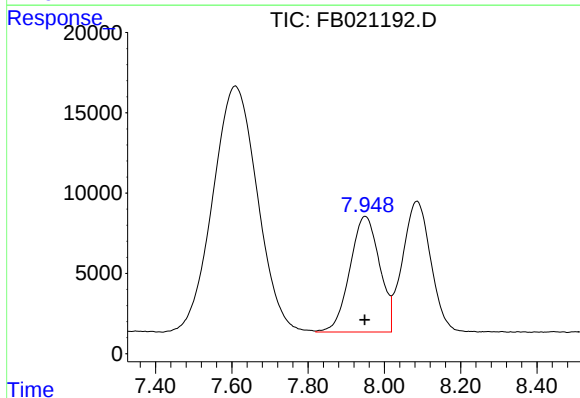


#3 n-Heptane

R.T.: 7.950 min
Delta R.T.: 0.002 min
Response: 389423
Conc: 9.84 ng/ml

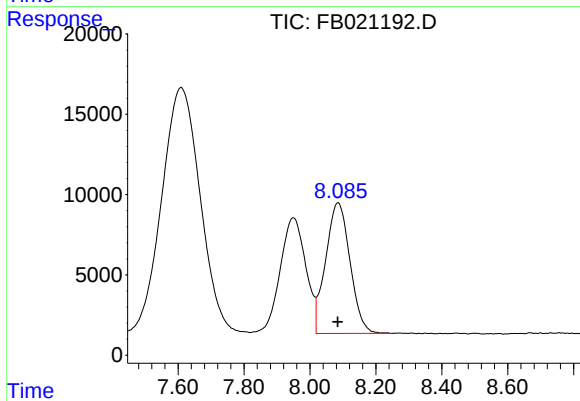


#4 Benzene

R.T.: 8.086 min
Delta R.T.: 0.001 min
Response: 418051
Conc: 9.99 ng/ml

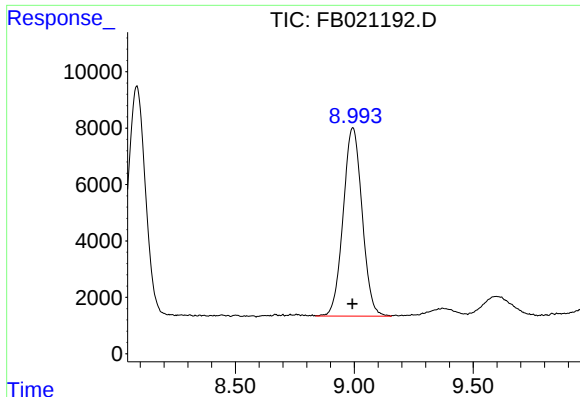


#5 AAA-TFT

R.T.: 8.994 min
Delta R.T.: 0.002 min
Response: 369418
Conc: 20.59 ng/ml

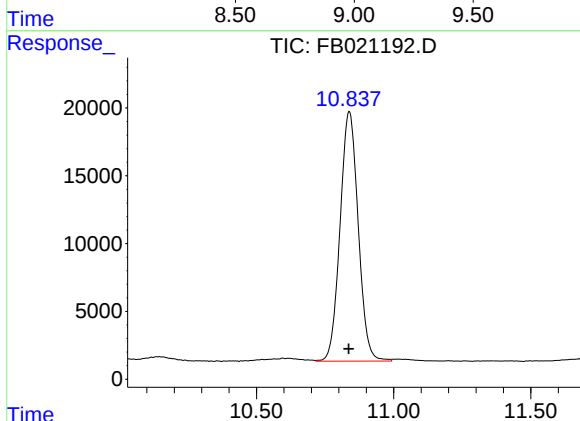


#6 Toluene

R.T.: 10.839 min
Delta R.T.: 0.003 min
Response: 846572
Conc: 30.56 ng/ml

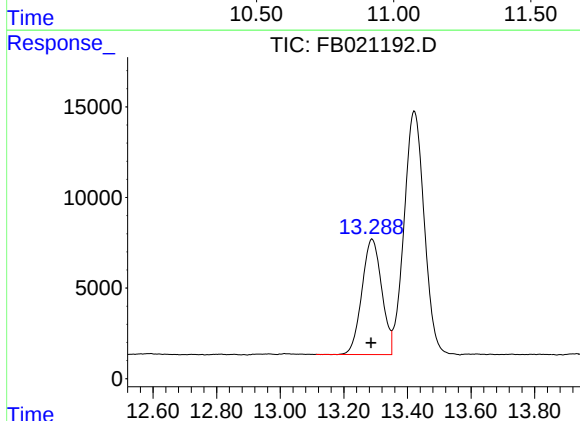


#7 Ethylbenzene

R.T.: 13.289 min
Delta R.T.: 0.004 min
Response: 275904
Conc: 9.84 ng/ml

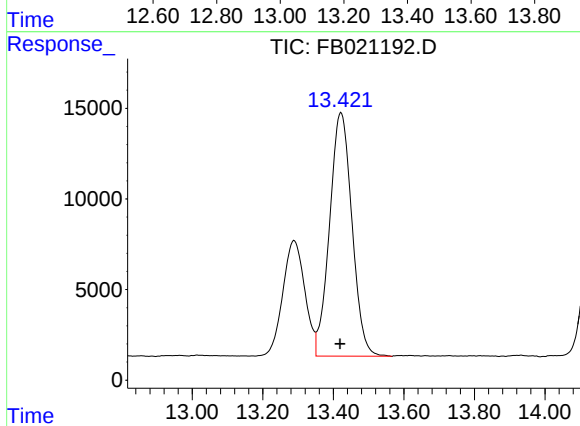


#8 m-Xylene

R.T.: 13.422 min
Delta R.T.: 0.003 min
Response: 592970
Conc: 19.95 ng/ml

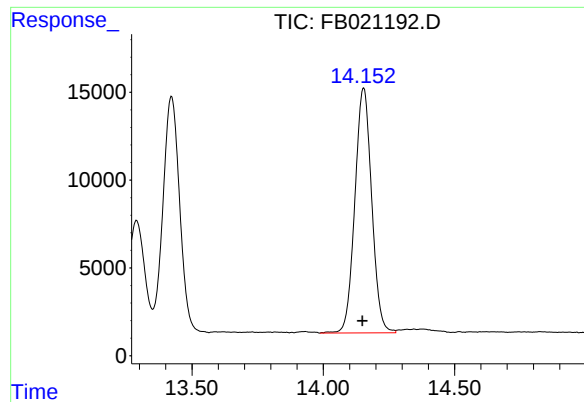

#9 O-Xylene

R.T.: 14.154 min
Delta R.T.: 0.004 min
Response: 620335
Conc: 20.01 ng/ml

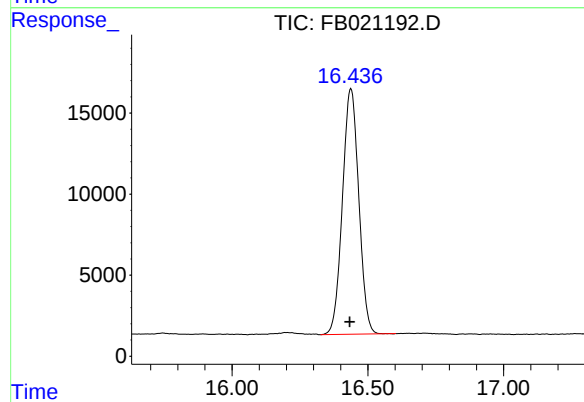

#10 1,2,4-Trimethylbenzene

R.T.: 16.438 min
Delta R.T.: 0.005 min
Response: 632492
Conc: 20.39 ng/ml