

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052423\
 Data File : FB029820.D
 Signal(s) : FID2B.CH
 Acq On : 24 May 2023 19:51
 Operator : YP/AJ
 Sample : 02899-09MSD 50X
 Misc : 5.00G/5.00 ML MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: May 25 06:41:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051123.M
 Quant Title :
 QLast Update : Thu May 11 11:33:20 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	240292	19.732 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.413	478322	28.025 ng/ml
3) t n-Heptane	7.745	161387	9.088 ng/ml
4) t Benzene	7.883	204395	9.757 ng/ml
6) t Toluene	10.616	595762	29.259 ng/ml
7) t Ethylbenzene	13.053	186111	9.711 ng/ml
8) t m-Xylene	13.186	372046	19.309 ng/ml
9) t O-Xylene	13.912	355773	19.125 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	335288	18.025 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052423\
Data File : FB029820.D
Signal(s) : FID2B.CH
Acq On : 24 May 2023 19:51
Operator : YP/AJ
Sample : 02899-09MSD 50X
Misc : 5.00G/5.00 ML MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 25 06:41:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051123.M
Quant Title :
QLast Update : Thu May 11 11:33:20 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

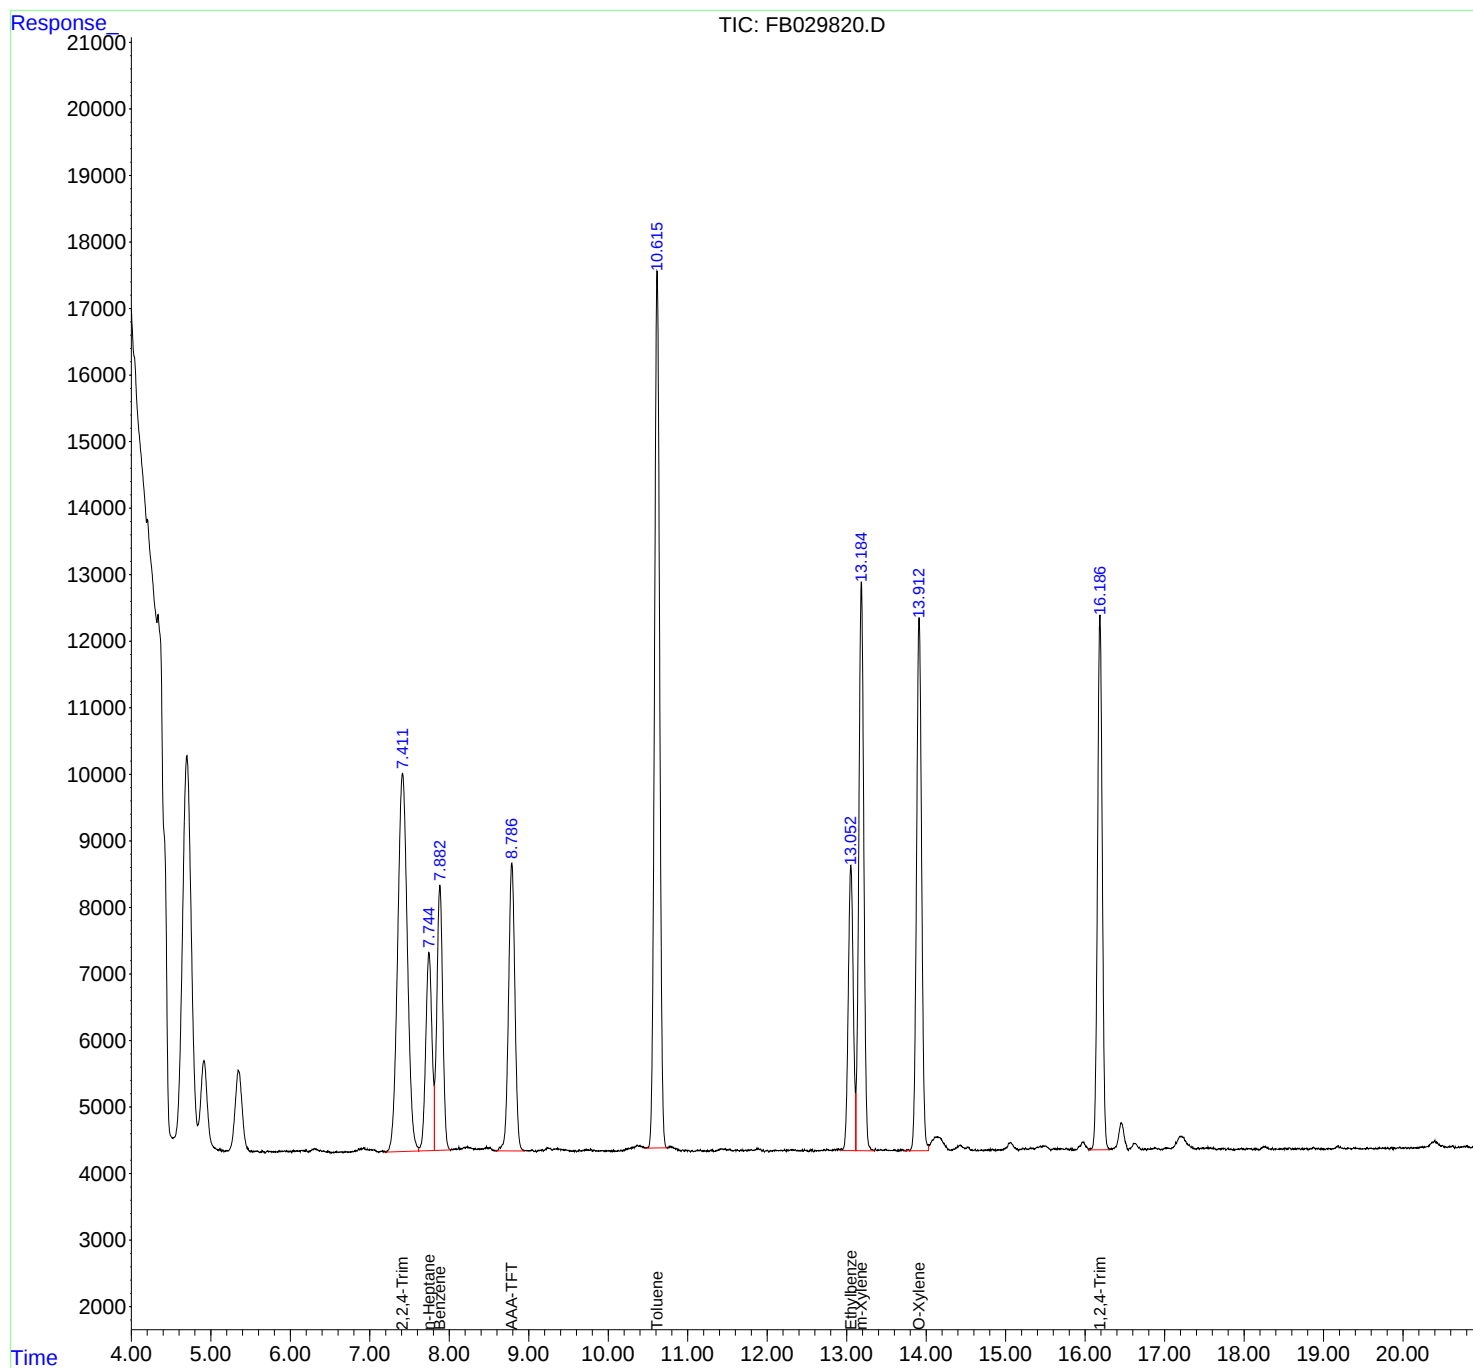


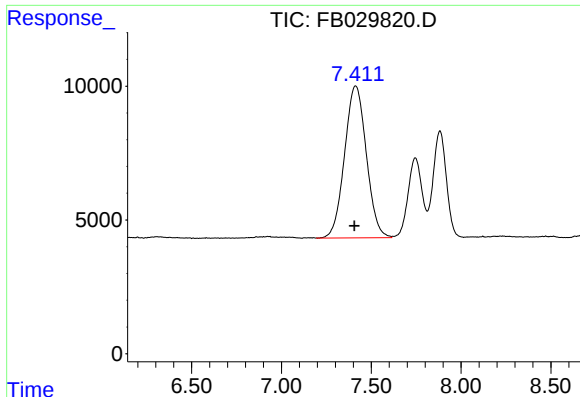

#2 2,2,4-Trimethylpentane


R.T.: 7.413 min
Delta R.T.: 0.006 min
Response: 478322
Conc: 28.03 ng/ml

Instrument :
FID_B
ClientSampleId :

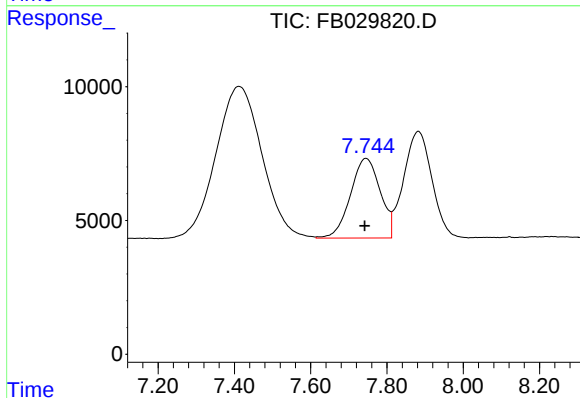


#3 n-Heptane

R.T.: 7.745 min
Delta R.T.: 0.003 min
Response: 161387
Conc: 9.09 ng/ml

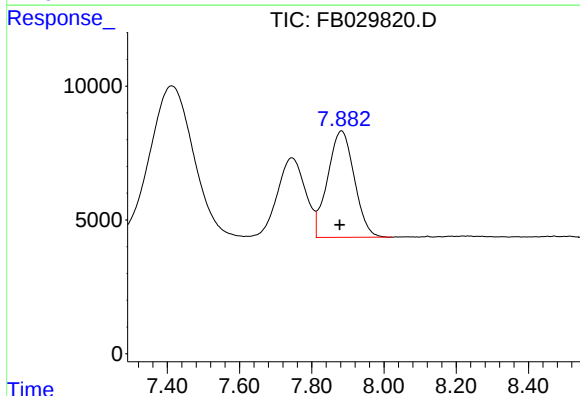


#4 Benzene

R.T.: 7.883 min
Delta R.T.: 0.005 min
Response: 204395
Conc: 9.76 ng/ml

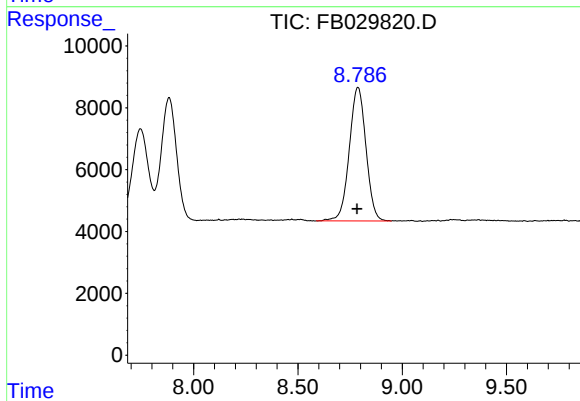

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: 0.005 min
Response: 240292
Conc: 19.73 ng/ml

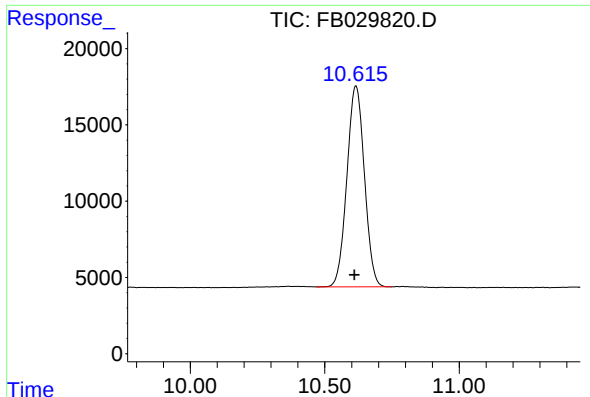

#6 Toluene


R.T.: 10.616 min
Delta R.T.: 0.006 min
Response: 595762
Conc: 29.26 ng/ml

Instrument :
FID_B
ClientSampleId :

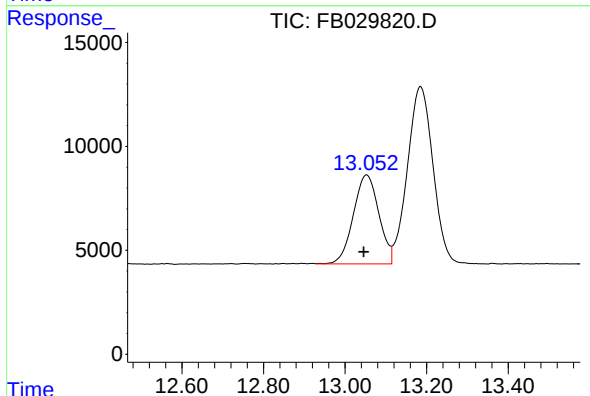


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: 0.007 min
Response: 186111
Conc: 9.71 ng/ml

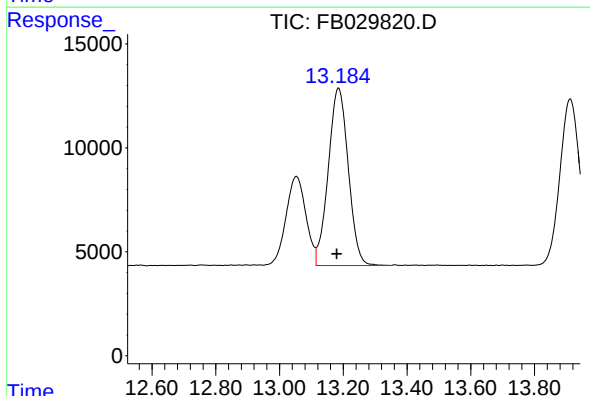


#8 m-Xylene

R.T.: 13.186 min
Delta R.T.: 0.007 min
Response: 372046
Conc: 19.31 ng/ml

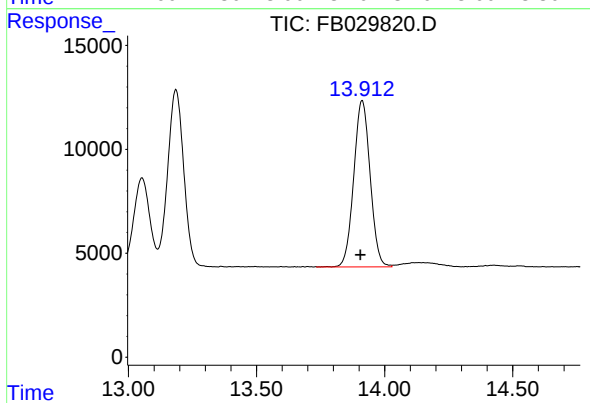

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: 0.006 min
Response: 355773
Conc: 19.13 ng/ml

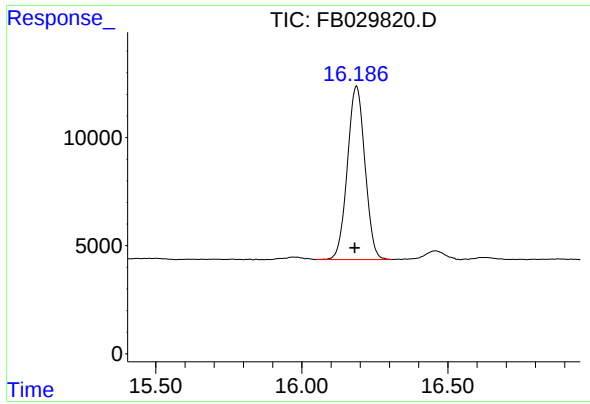

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: 0.006 min
Response: 335288
Conc: 18.03 ng/ml

Instrument :
FID_B
ClientSampleId :