

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052423\
 Data File : FB029822.D
 Signal(s) : FID2B.CH
 Acq On : 24 May 2023 21:06
 Operator : YP/AJ
 Sample : BSF0524S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: May 25 06:41:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051123.M
 Quant Title :
 QLast Update : Thu May 11 11:33:20 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	228266	18.745 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	470089	27.436 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	471167	27.606 ng/ml
3) t n-Heptane	7.747	162457	9.148 ng/ml
4) t Benzene	7.884	197663	9.436 ng/ml
6) t Toluene	10.616	585446	28.752 ng/ml
7) t Ethylbenzene	13.053	183456	9.573 ng/ml
8) t m-Xylene	13.185	364791	18.933 ng/ml
9) t O-Xylene	13.912	350141	18.823 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	347302	18.671 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052423\
Data File : FB029822.D
Signal(s) : FID2B.CH
Acq On : 24 May 2023 21:06
Operator : YP/AJ
Sample : BSF0524S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 25 06:41:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051123.M
Quant Title :
QLast Update : Thu May 11 11:33:20 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

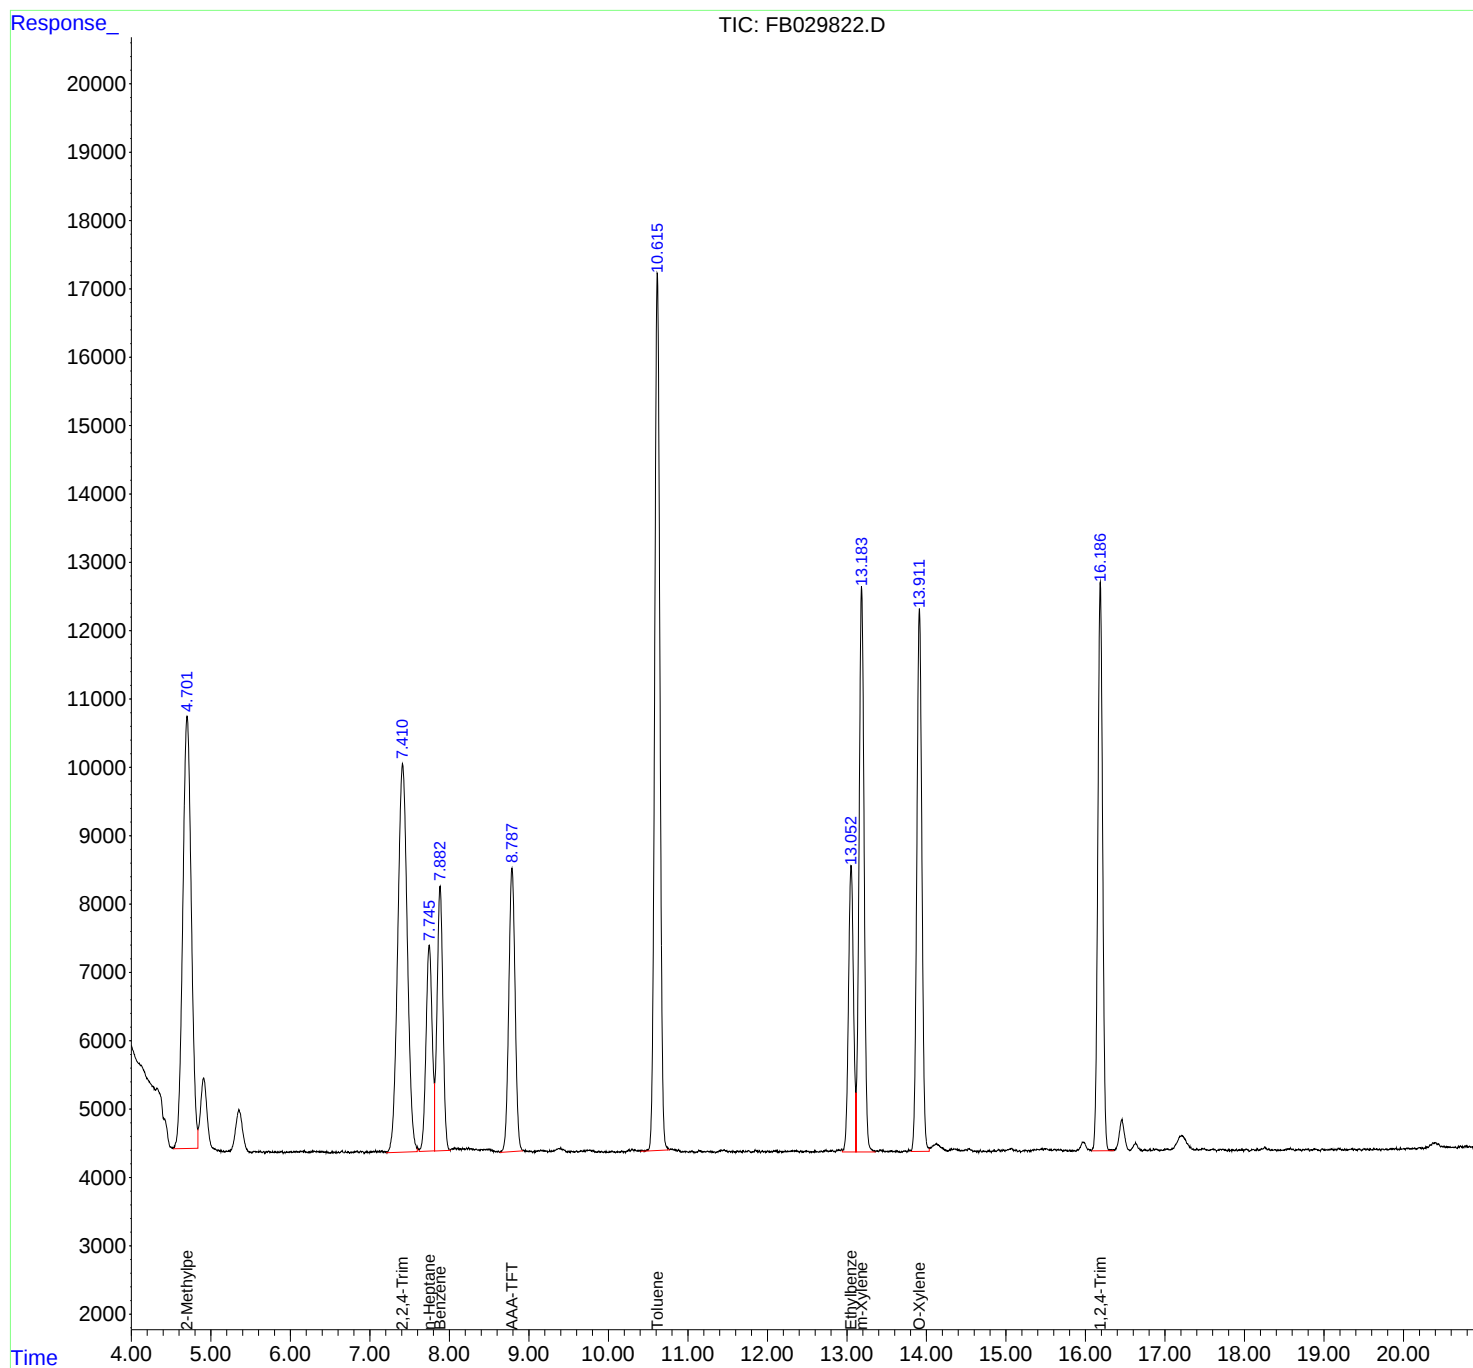


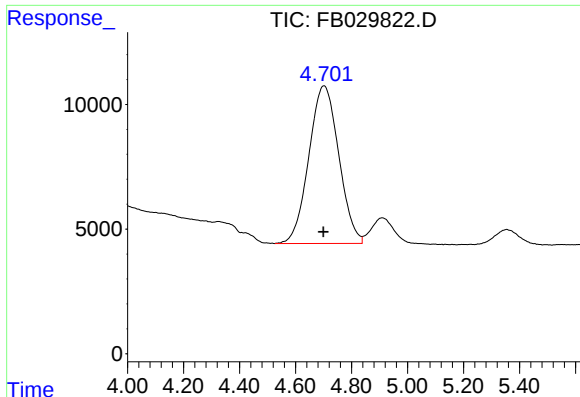

#1 2-Methylpentane


R.T.: 4.702 min
Delta R.T.: 0.003 min
Response: 470089
Conc: 27.44 ng/ml

Instrument :
FID_B
ClientSampleId :

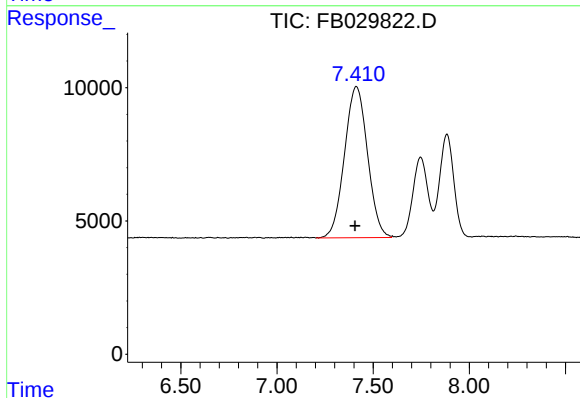


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: 0.006 min
Response: 471167
Conc: 27.61 ng/ml

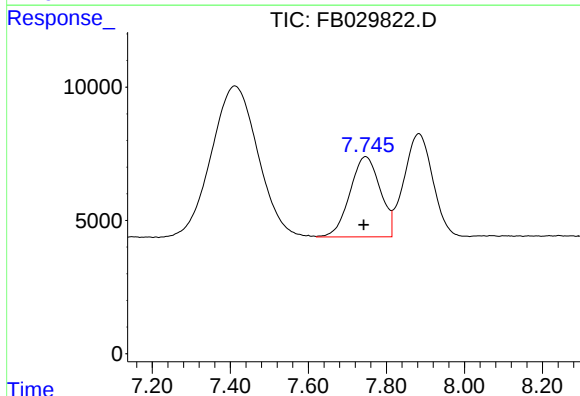


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: 0.005 min
Response: 162457
Conc: 9.15 ng/ml

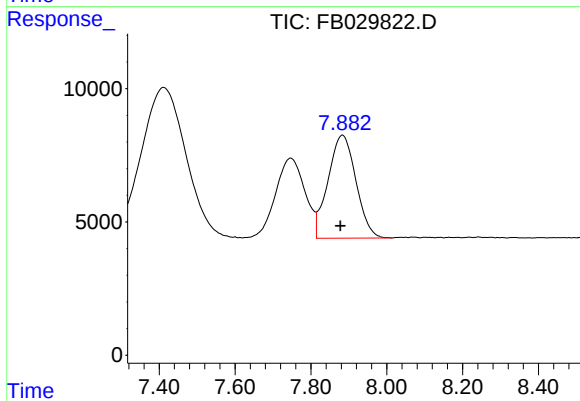

#4 Benzene


R.T.: 7.884 min
Delta R.T.: 0.006 min
Response: 197663
Conc: 9.44 ng/ml

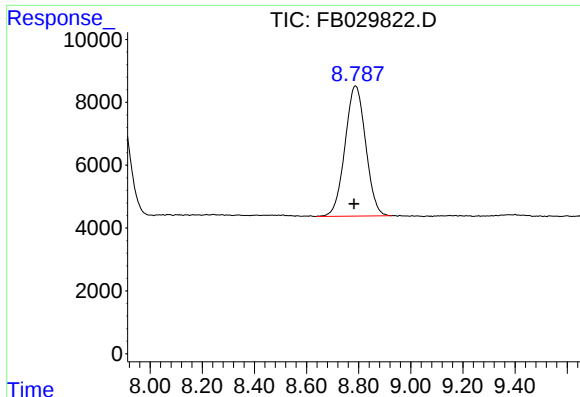

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: 0.006 min
Response: 228266
Conc: 18.74 ng/ml

Instrument :
FID_B
ClientSampleId :

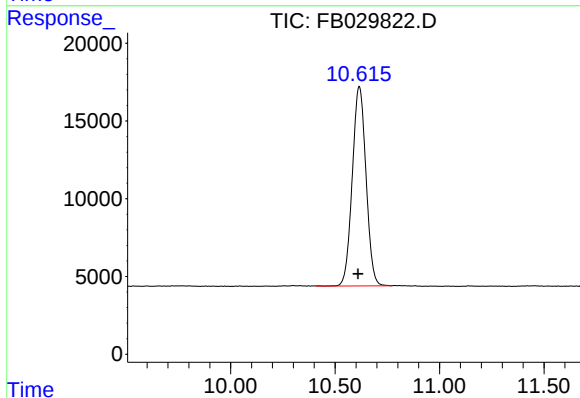


#6 Toluene

R.T.: 10.616 min
Delta R.T.: 0.006 min
Response: 585446
Conc: 28.75 ng/ml

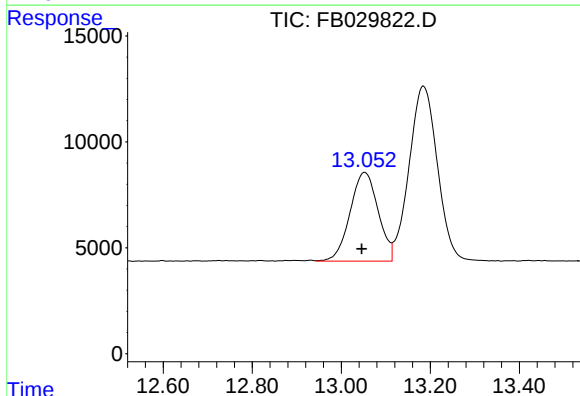


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: 0.007 min
Response: 183456
Conc: 9.57 ng/ml

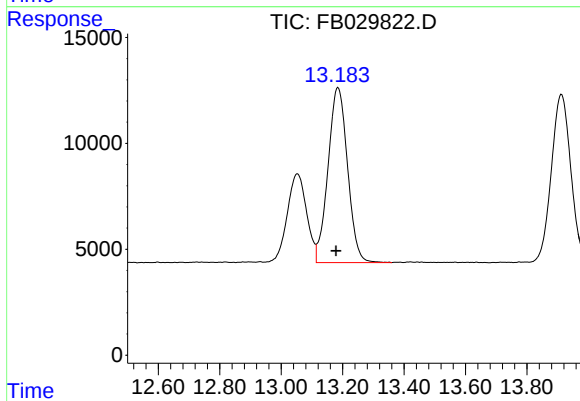

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: 0.006 min
Response: 364791
Conc: 18.93 ng/ml

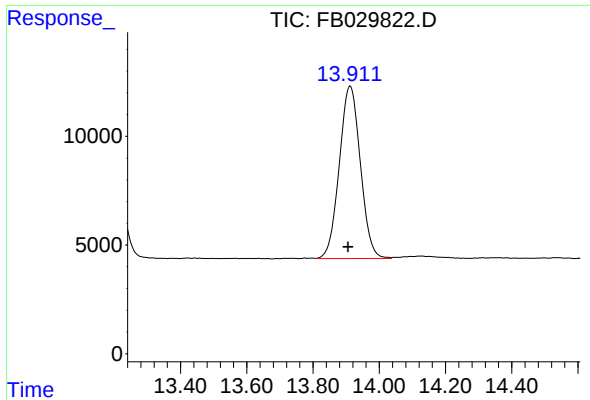

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: 0.006 min
Response: 350141
Conc: 18.82 ng/ml

Instrument :
FID_B
ClientSampleId :

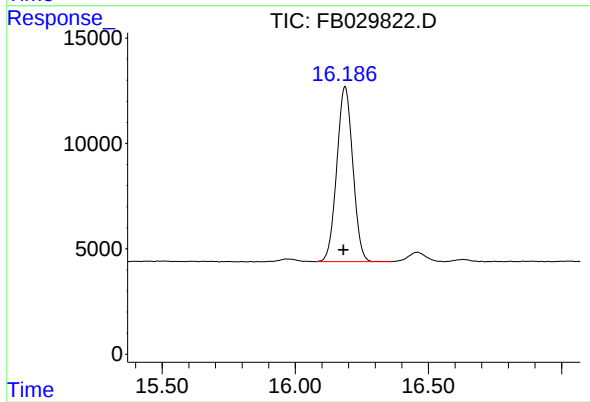

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: 0.006 min
Response: 347302
Conc: 18.67 ng/ml