

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052423\
 Data File : FB029832.D
 Signal(s) : FID2B.CH
 Acq On : 25 May 2023 4:28
 Operator : YP/AJ
 Sample : BSF0524S3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: May 25 06:42:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051123.M
 Quant Title :
 QLast Update : Thu May 11 11:33:20 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.784	244062	20.042 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.699	466288	27.214 ng/ml
2) t 2,2,4-Trimethylpentane	7.408	469430	27.504 ng/ml
3) t n-Heptane	7.743	160326	9.028 ng/ml
4) t Benzene	7.880	197028	9.405 ng/ml
6) t Toluene	10.612	573522	28.167 ng/ml
7) t Ethylbenzene	13.048	179630	9.373 ng/ml
8) t m-Xylene	13.181	359054	18.635 ng/ml
9) t O-Xylene	13.908	346840	18.645 ng/ml
10) t 1,2,4-Trimethylbenzene	16.182	346431	18.624 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052423\
Data File : FB029832.D
Signal(s) : FID2B.CH
Acq On : 25 May 2023 4:28
Operator : YP/AJ
Sample : BSF0524S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 25 06:42:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051123.M
Quant Title :
QLast Update : Thu May 11 11:33:20 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

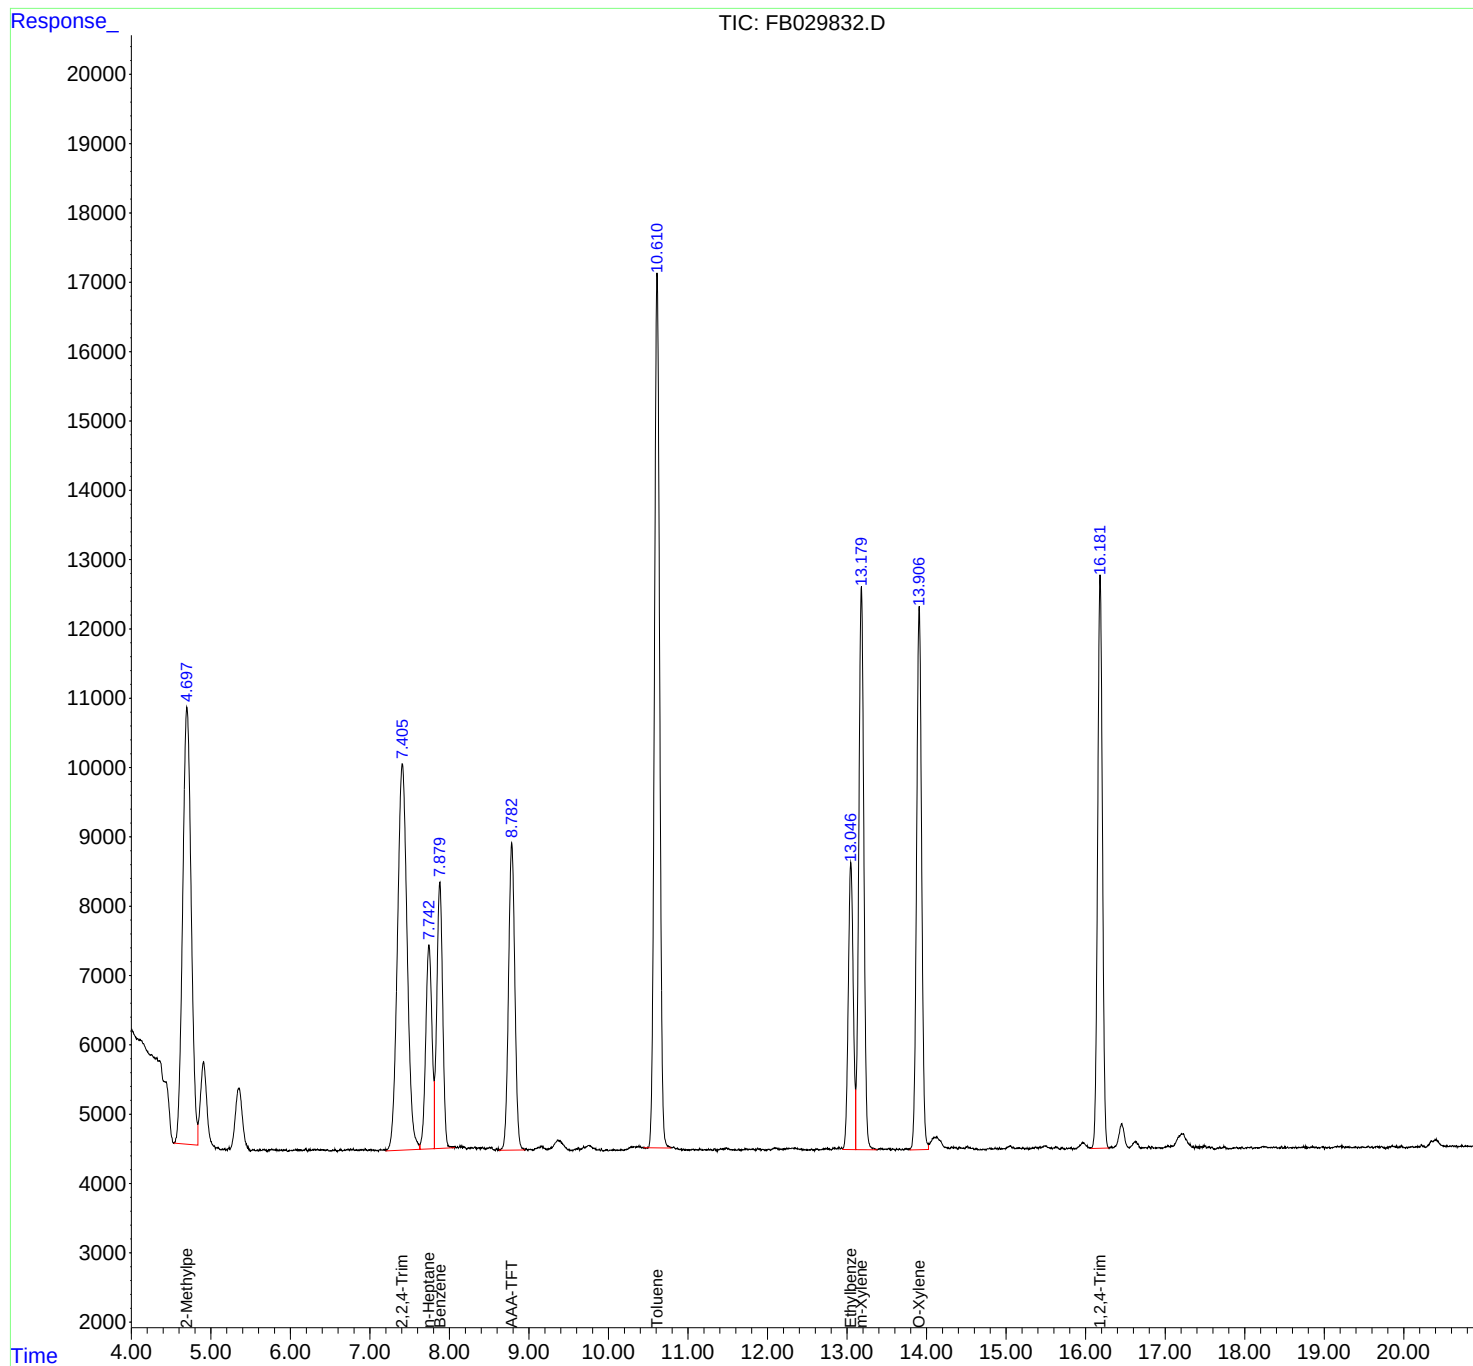


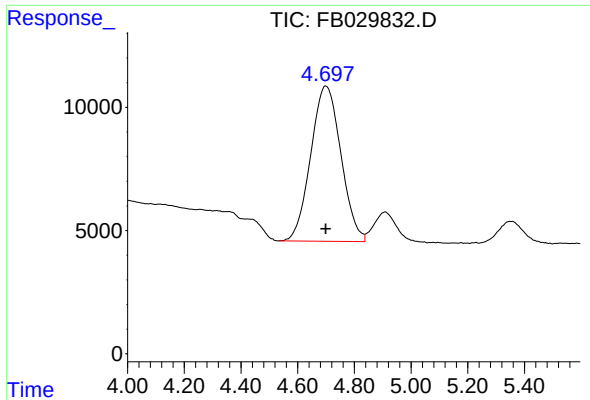

#1 2-Methylpentane


R.T.: 4.699 min
Delta R.T.: 0.000 min
Response: 466288
Conc: 27.21 ng/ml

Instrument :
FID_B
ClientSampleId :

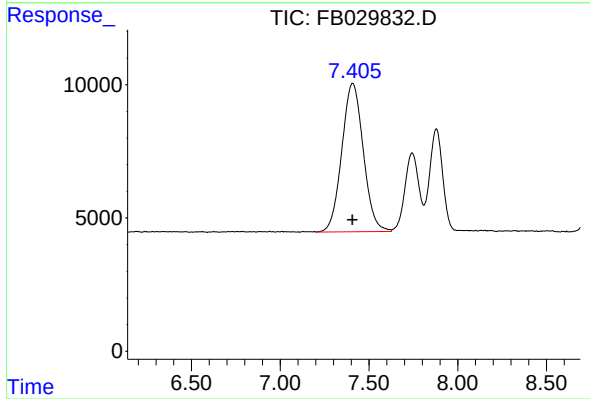


#2 2,2,4-Trimethylpentane

R.T.: 7.408 min
Delta R.T.: 0.001 min
Response: 469430
Conc: 27.50 ng/ml

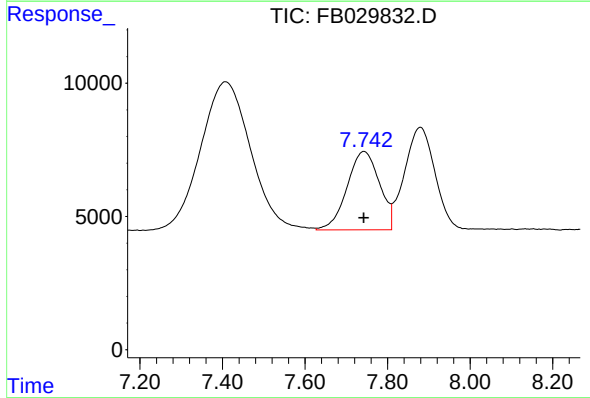


#3 n-Heptane

R.T.: 7.743 min
Delta R.T.: 0.001 min
Response: 160326
Conc: 9.03 ng/ml

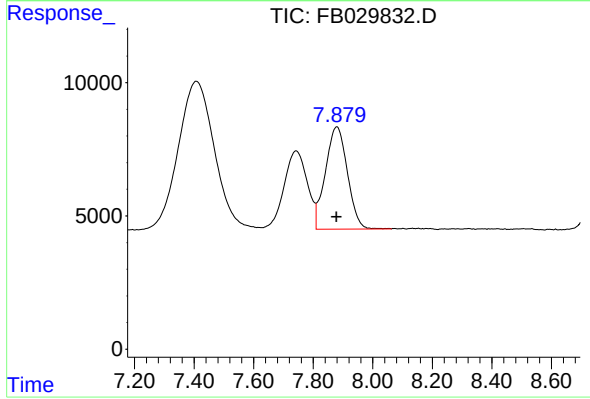

#4 Benzene


R.T.: 7.880 min
Delta R.T.: 0.002 min
Response: 197028
Conc: 9.41 ng/ml

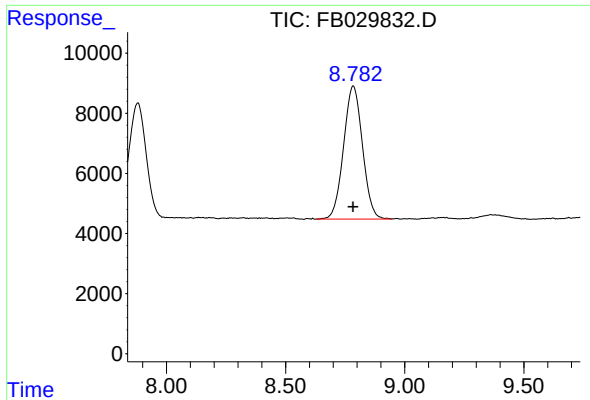

#5 AAA-TFT


R.T.: 8.784 min
Delta R.T.: 0.002 min
Response: 244062
Conc: 20.04 ng/ml

Instrument :
FID_B
ClientSampleId :

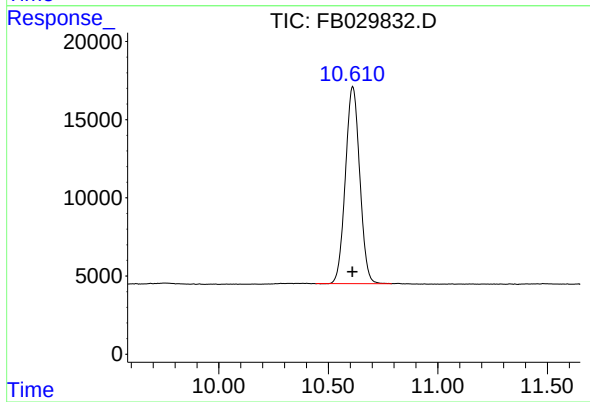


#6 Toluene

R.T.: 10.612 min
Delta R.T.: 0.001 min
Response: 573522
Conc: 28.17 ng/ml

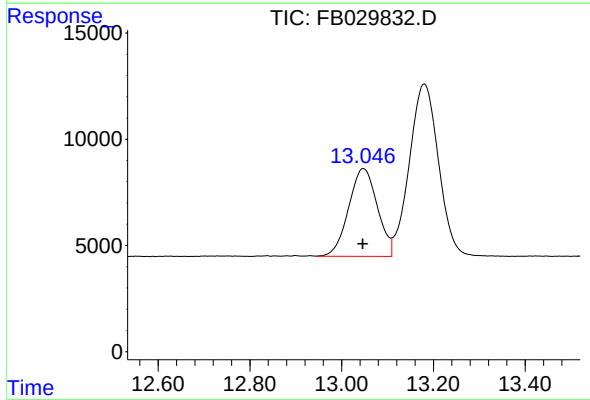


#7 Ethylbenzene

R.T.: 13.048 min
Delta R.T.: 0.002 min
Response: 179630
Conc: 9.37 ng/ml

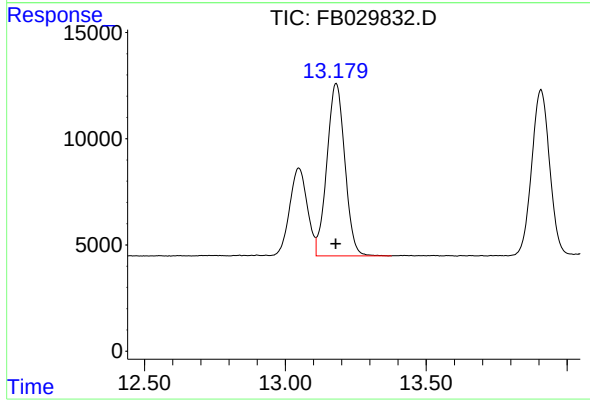

#8 m-Xylene


R.T.: 13.181 min
Delta R.T.: 0.002 min
Response: 359054
Conc: 18.64 ng/ml

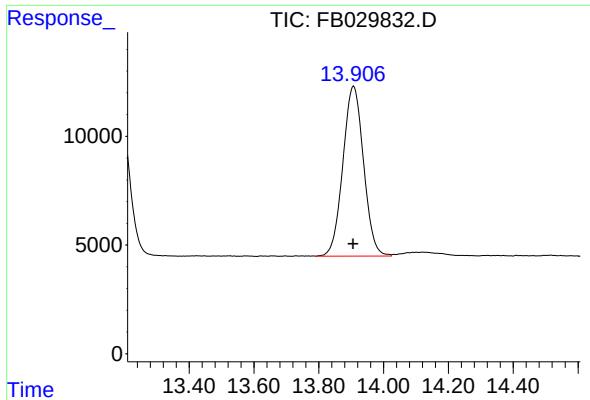

#9 O-Xylene

R.T.: 13.908 min
Delta R.T.: 0.002 min
Response: 346840
Conc: 18.65 ng/ml

Instrument :
FID_B
ClientSampleId :

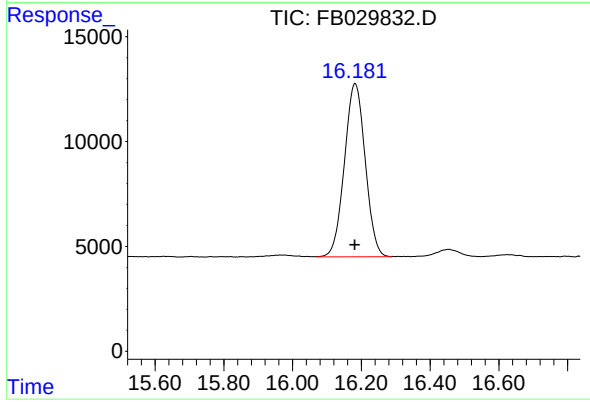

#10 1,2,4-Trimethylbenzene

R.T.: 16.182 min
Delta R.T.: 0.001 min
Response: 346431
Conc: 18.62 ng/ml