

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052523\
 Data File : FB029837.D
 Signal(s) : FID2B.CH
 Acq On : 25 May 2023 11:27
 Operator : YP/AJ
 Sample : BSF0525S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0525S1

Integration File: Calibration.e
 Quant Time: May 26 03:26:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051123.M
 Quant Title :
 QLast Update : Thu May 11 11:33:20 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.784	278898	22.902 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.701	496097	28.954 ng/ml
2) t 2,2,4-Trimethylpentane	7.408	488880	28.644 ng/ml
3) t n-Heptane	7.742	170430	9.597 ng/ml
4) t Benzene	7.879	208632	9.959 ng/ml
6) t Toluene	10.611	607617	29.841 ng/ml
7) t Ethylbenzene	13.048	193172	10.080 ng/ml
8) t m-Xylene	13.180	386821	20.076 ng/ml
9) t O-Xylene	13.907	375490	20.185 ng/ml
10) t 1,2,4-Trimethylbenzene	16.182	382066	20.540 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052523\
Data File : FB029837.D
Signal(s) : FID2B.CH
Acq On : 25 May 2023 11:27
Operator : YP/AJ
Sample : BSF0525S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0525S1

Integration File: Calibration.e
Quant Time: May 26 03:26:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051123.M
Quant Title :
QLast Update : Thu May 11 11:33:20 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

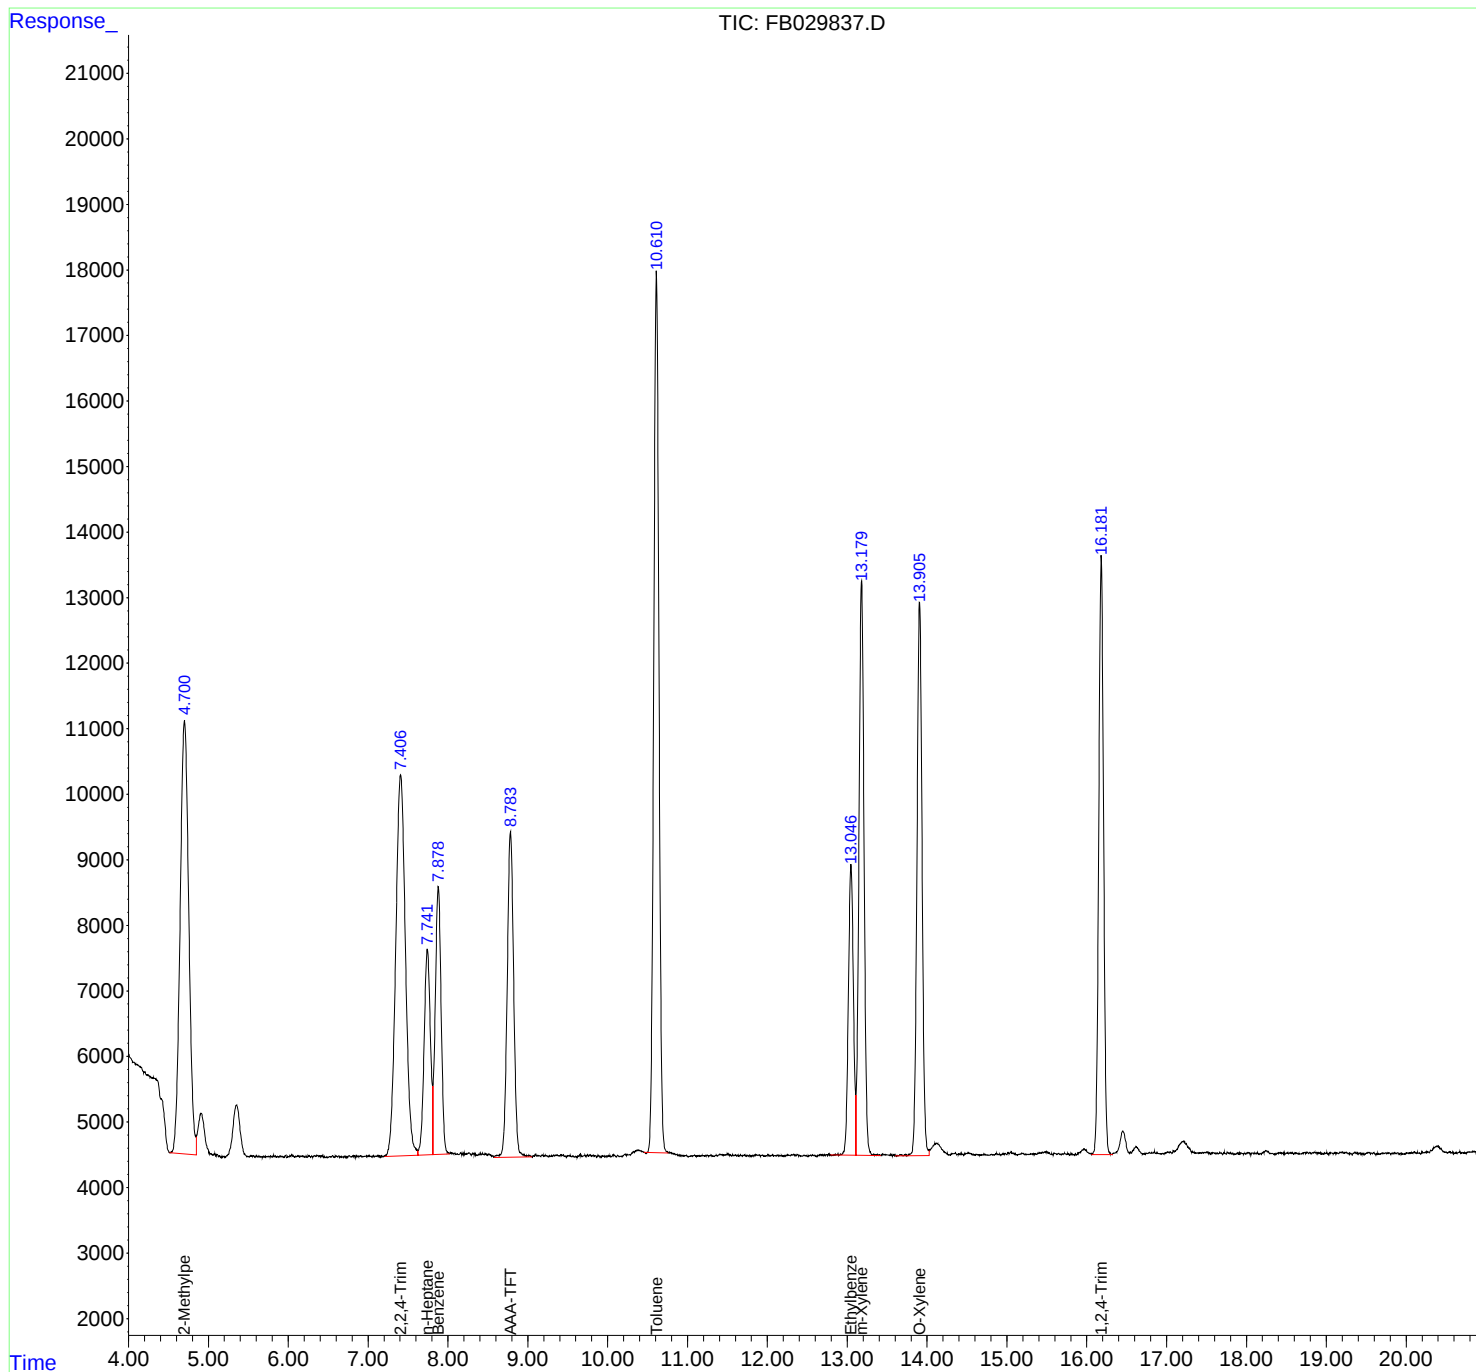


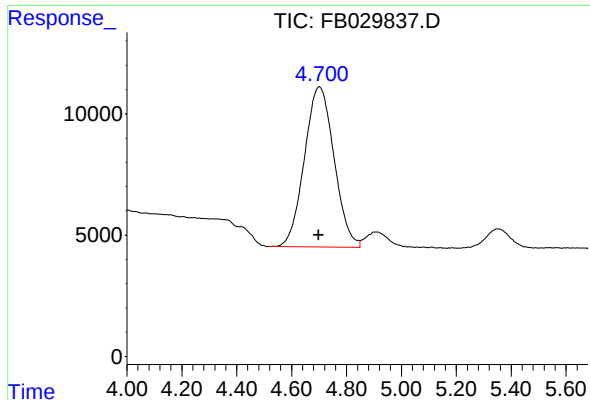

#1 2-Methylpentane


R.T.: 4.701 min
Delta R.T.: 0.002 min
Response: 496097
Conc: 28.95 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0525S1

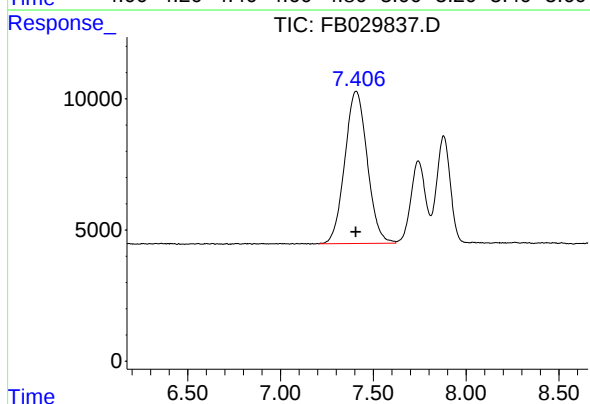


#2 2,2,4-Trimethylpentane

R.T.: 7.408 min
Delta R.T.: 0.002 min
Response: 488880
Conc: 28.64 ng/ml

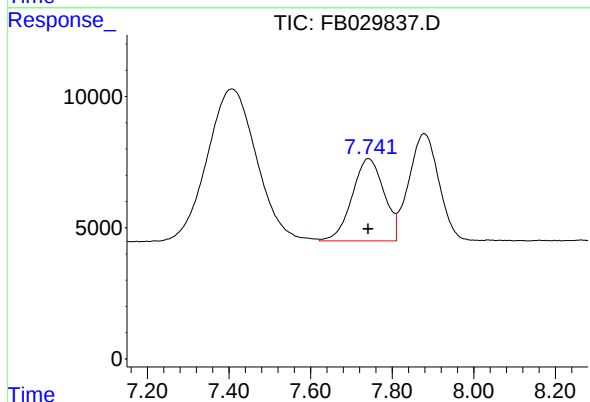


#3 n-Heptane

R.T.: 7.742 min
Delta R.T.: 0.000 min
Response: 170430
Conc: 9.60 ng/ml

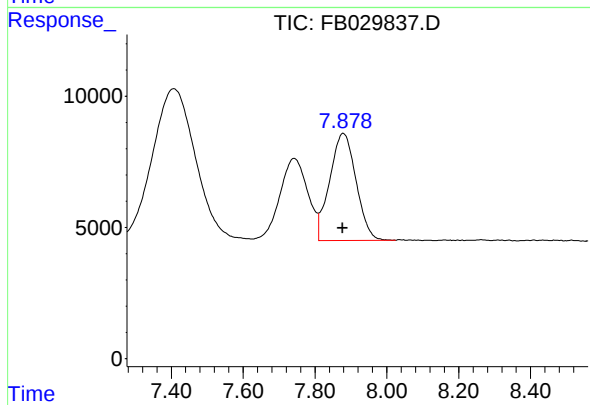

#4 Benzene


R.T.: 7.879 min
Delta R.T.: 0.001 min
Response: 208632
Conc: 9.96 ng/ml

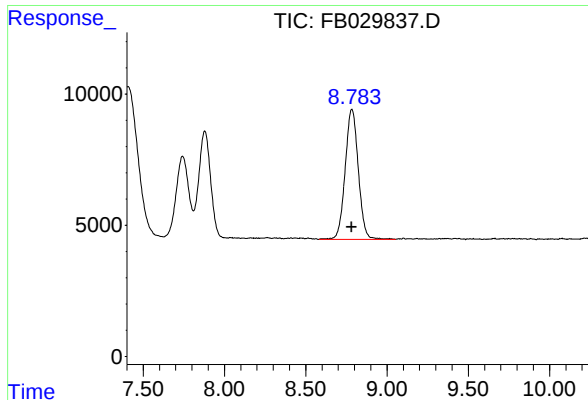

#5 AAA-TFT


R.T.: 8.784 min
Delta R.T.: 0.001 min
Response: 278898
Conc: 22.90 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0525S1

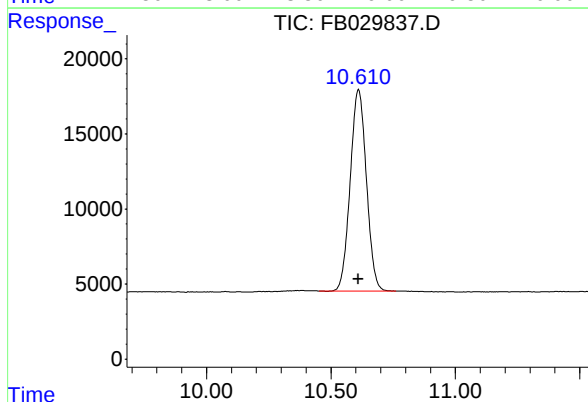


#6 Toluene

R.T.: 10.611 min
Delta R.T.: 0.000 min
Response: 607617
Conc: 29.84 ng/ml

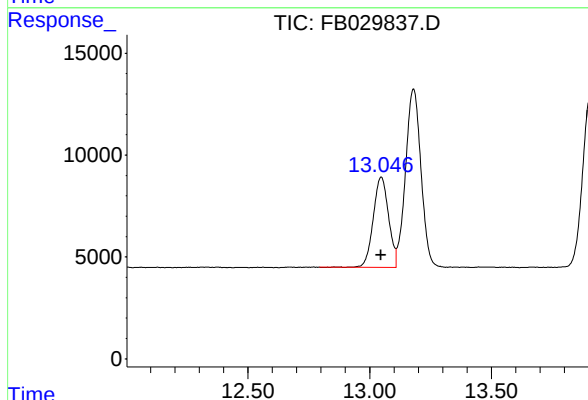


#7 Ethylbenzene

R.T.: 13.048 min
Delta R.T.: 0.002 min
Response: 193172
Conc: 10.08 ng/ml

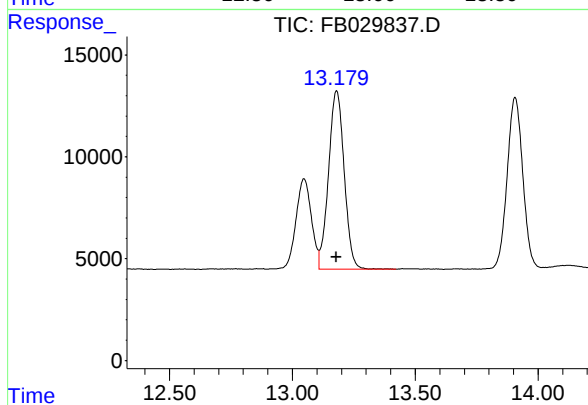

#8 m-Xylene


R.T.: 13.180 min
Delta R.T.: 0.001 min
Response: 386821
Conc: 20.08 ng/ml

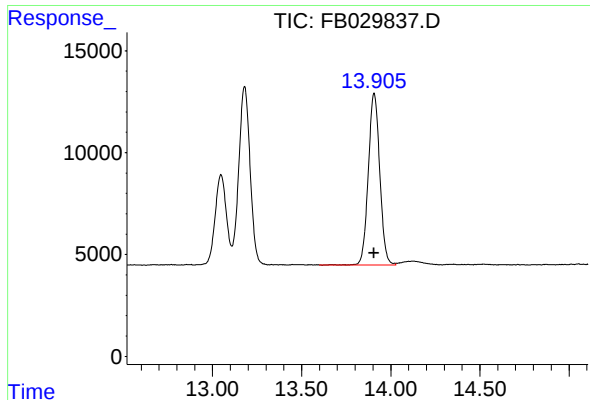

#9 O-Xylene

R.T.: 13.907 min
Delta R.T.: 0.000 min
Response: 375490
Conc: 20.19 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0525S1

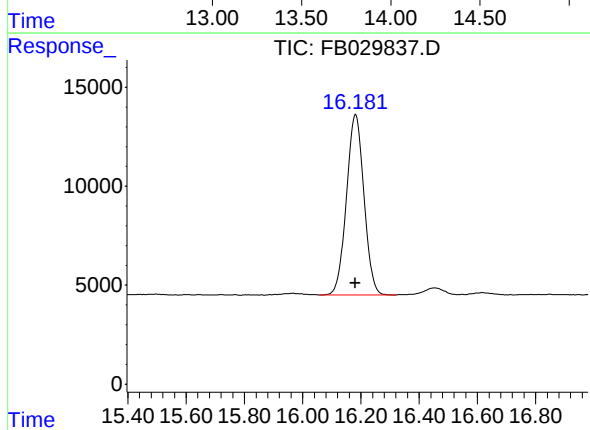

#10 1,2,4-Trimethylbenzene

R.T.: 16.182 min
Delta R.T.: 0.000 min
Response: 382066
Conc: 20.54 ng/ml