

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052523\
 Data File : FB029842.D
 Signal(s) : FID2B.CH
 Acq On : 25 May 2023 14:34
 Operator : YP/AJ
 Sample : 02937-01MS 50X
 Misc : 5.07G/5.00 ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 AU-06-052423MS

Integration File: Calibration.e
 Quant Time: May 26 03:26:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051123.M
 Quant Title :
 QLast Update : Thu May 11 11:33:20 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.784	222492	18.271 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.696	467099	27.262 ng/ml
2) t 2,2,4-Trimethylpentane	7.407	524820	30.750 ng/ml
3) t n-Heptane	7.742	172356	9.706 ng/ml
4) t Benzene	7.878	220935	10.547 ng/ml
6) t Toluene	10.612	619590	30.429 ng/ml
7) t Ethylbenzene	13.049	198336	10.349 ng/ml
8) t m-Xylene	13.182	394350	20.467 ng/ml
9) t O-Xylene	13.909	375570	20.190 ng/ml
10) t 1,2,4-Trimethylbenzene	16.184	359399	19.321 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052523\
Data File : FB029842.D
Signal(s) : FID2B.CH
Acq On : 25 May 2023 14:34
Operator : YP/AJ
Sample : 02937-01MS 50X
Misc : 5.07G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
AU-06-052423MS

Integration File: Calibration.e
Quant Time: May 26 03:26:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051123.M
Quant Title :
QLast Update : Thu May 11 11:33:20 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

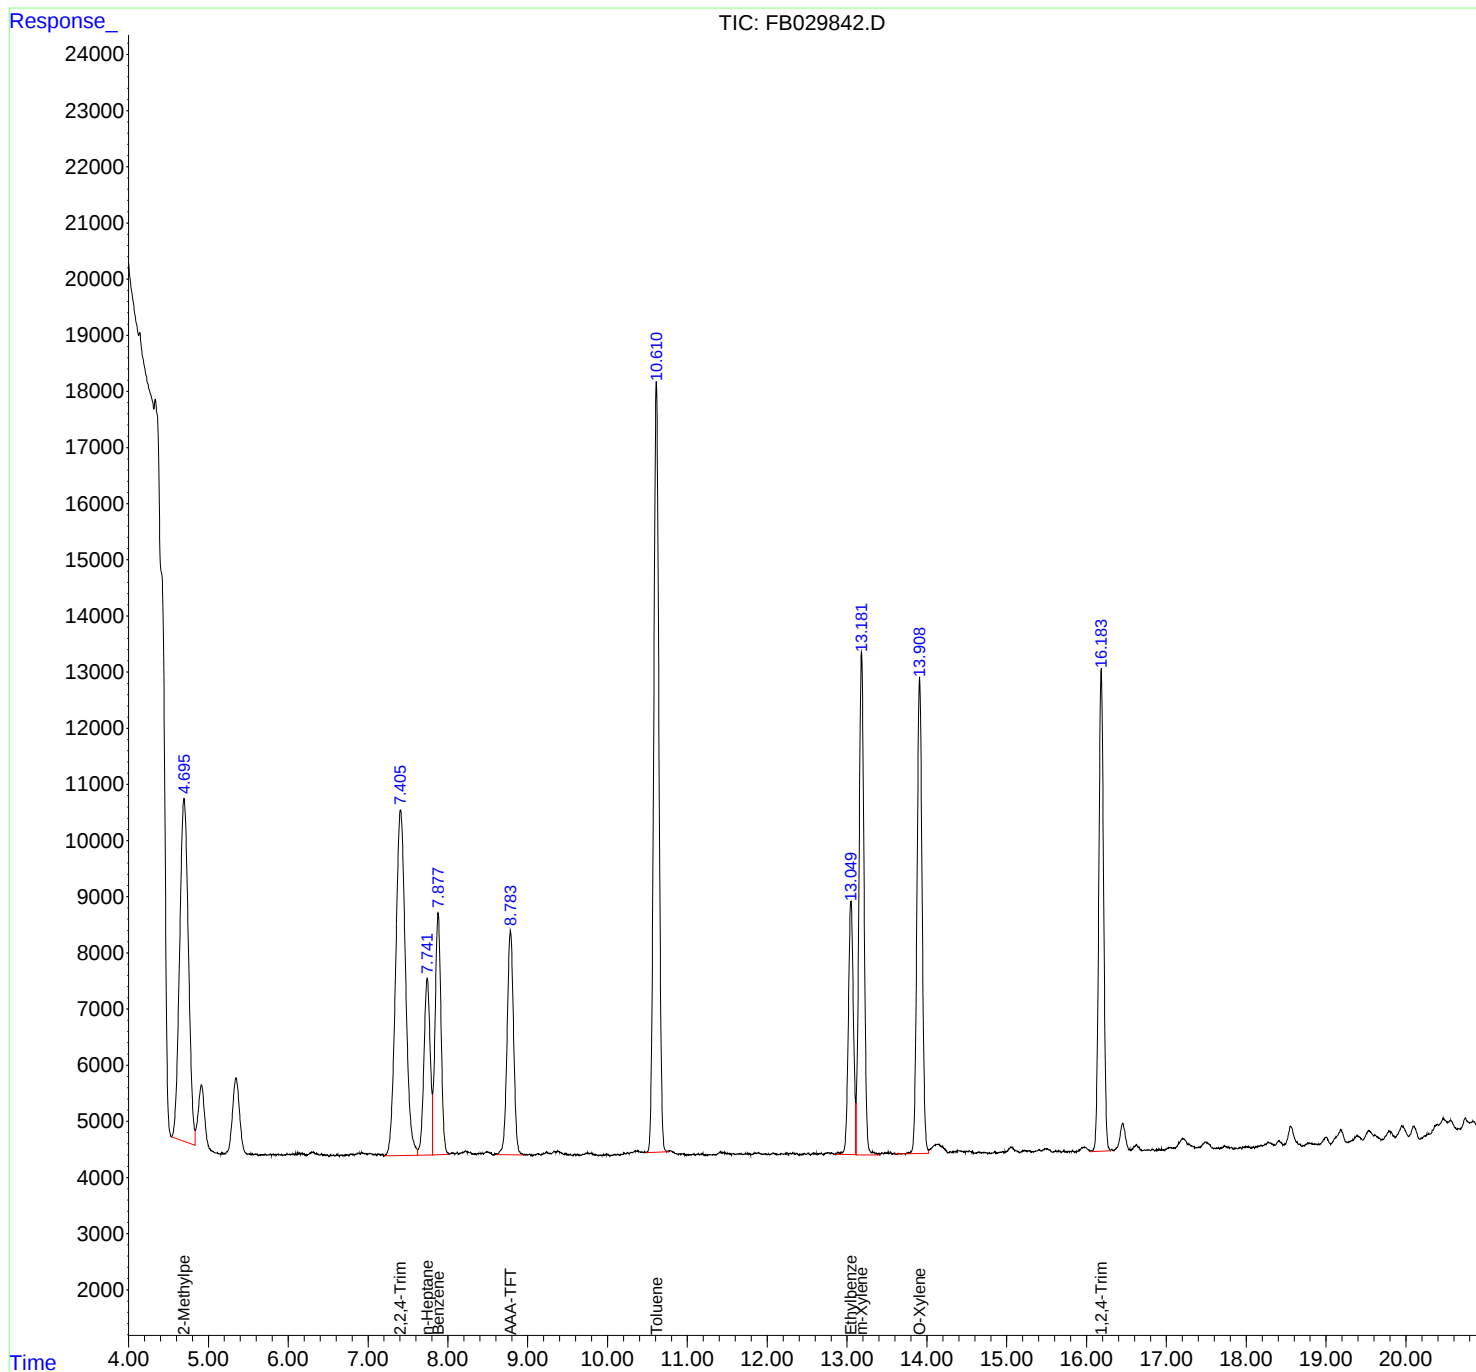


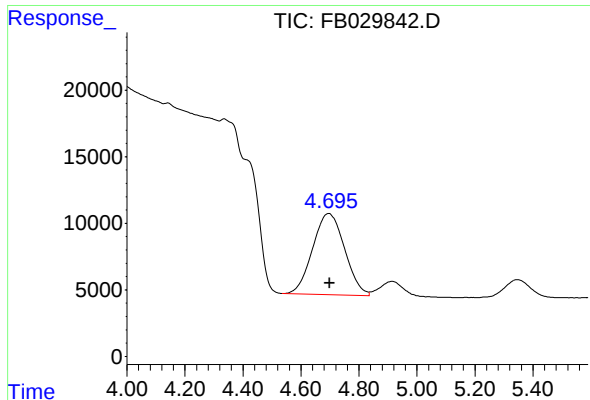

#1 2-Methylpentane


R.T.: 4.696 min
Delta R.T.: -0.003 min
Response: 467099
Conc: 27.26 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-052423MS

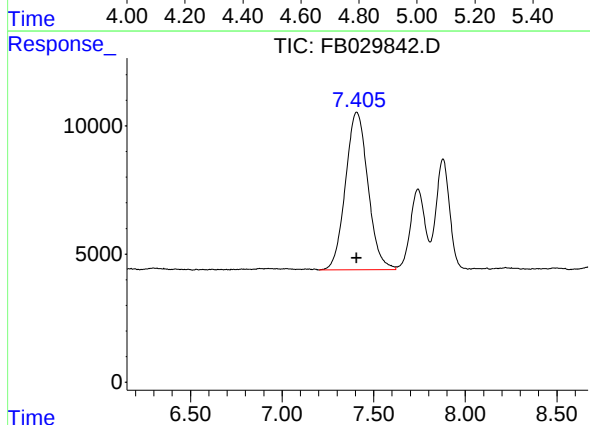


#2 2,2,4-Trimethylpentane

R.T.: 7.407 min
Delta R.T.: 0.000 min
Response: 524820
Conc: 30.75 ng/ml

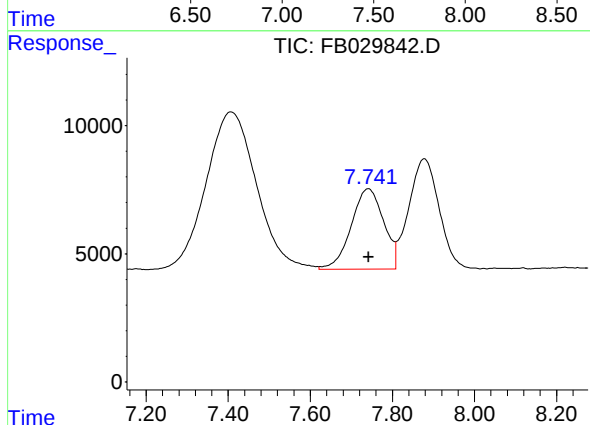


#3 n-Heptane

R.T.: 7.742 min
Delta R.T.: 0.000 min
Response: 172356
Conc: 9.71 ng/ml

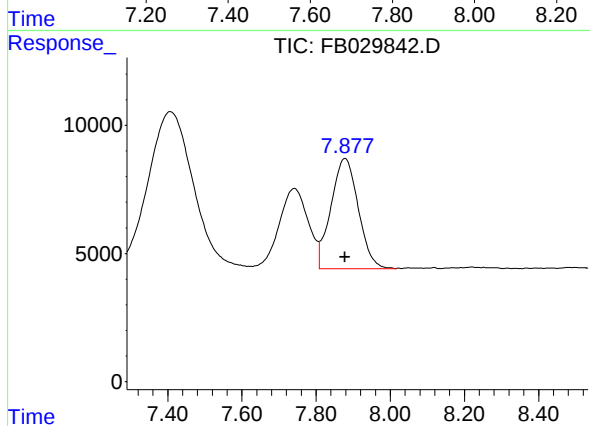

#4 Benzene


R.T.: 7.878 min
Delta R.T.: 0.000 min
Response: 220935
Conc: 10.55 ng/ml

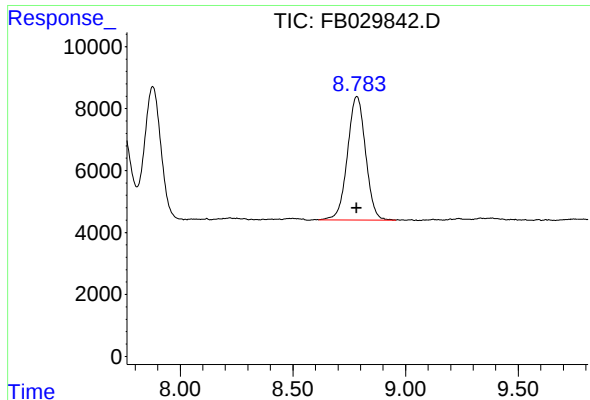

#5 AAA-TFT


R.T.: 8.784 min
Delta R.T.: 0.002 min
Response: 222492
Conc: 18.27 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-052423MS

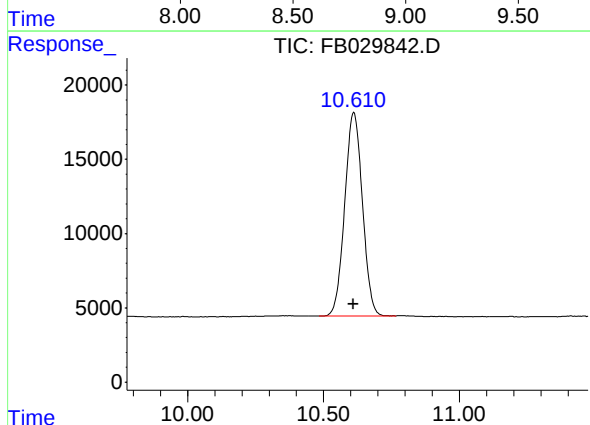


#6 Toluene

R.T.: 10.612 min
Delta R.T.: 0.002 min
Response: 619590
Conc: 30.43 ng/ml

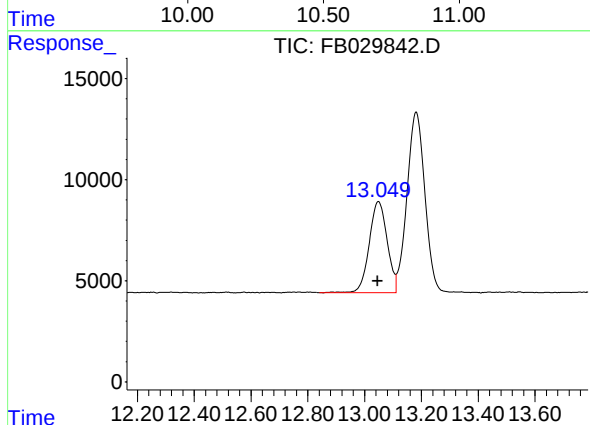


#7 Ethylbenzene

R.T.: 13.049 min
Delta R.T.: 0.003 min
Response: 198336
Conc: 10.35 ng/ml

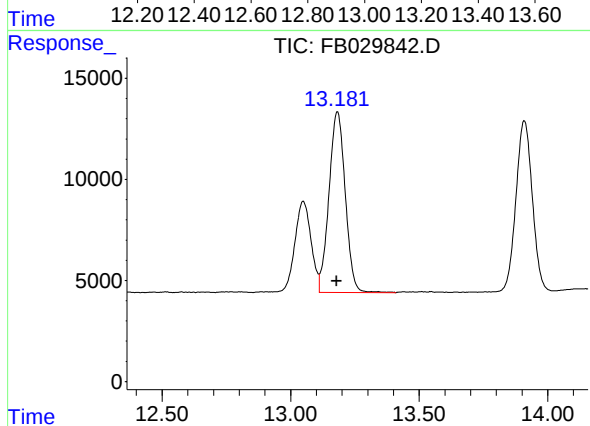

#8 m-Xylene


R.T.: 13.182 min
Delta R.T.: 0.003 min
Response: 394350
Conc: 20.47 ng/ml

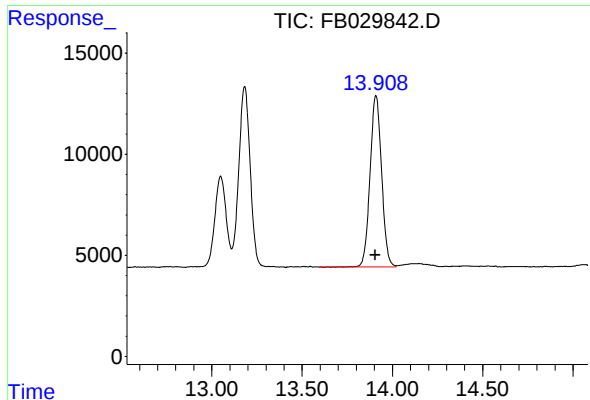

#9 O-Xylene

R.T.: 13.909 min
Delta R.T.: 0.003 min
Response: 375570
Conc: 20.19 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-052423MS

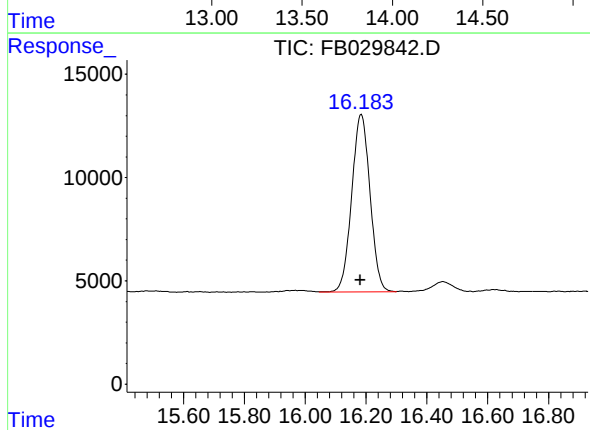

#10 1,2,4-Trimethylbenzene

R.T.: 16.184 min
Delta R.T.: 0.003 min
Response: 359399
Conc: 19.32 ng/ml