

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052523\
 Data File : FB029843.D
 Signal(s) : FID2B.CH
 Acq On : 25 May 2023 15:11
 Operator : YP/AJ
 Sample : 02937-01MSD 50X
 Misc : 5.08G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 AU-06-052423MSD

Integration File: Calibration.e
 Quant Time: May 26 03:27:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051123.M
 Quant Title :
 QLast Update : Thu May 11 11:33:20 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.784	226327	18.585 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.696	439705	25.663 ng/ml
2) t 2,2,4-Trimethylpentane	7.408	477421	27.972 ng/ml
3) t n-Heptane	7.741	158186	8.908 ng/ml
4) t Benzene	7.879	207212	9.892 ng/ml
6) t Toluene	10.613	577227	28.349 ng/ml
7) t Ethylbenzene	13.050	180725	9.430 ng/ml
8) t m-Xylene	13.182	358740	18.619 ng/ml
9) t O-Xylene	13.909	341575	18.362 ng/ml
10) t 1,2,4-Trimethylbenzene	16.184	327822	17.624 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052523\
Data File : FB029843.D
Signal(s) : FID2B.CH
Acq On : 25 May 2023 15:11
Operator : YP/AJ
Sample : 02937-01MSD 50X
Misc : 5.08G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
AU-06-052423MSD

Integration File: Calibration.e
Quant Time: May 26 03:27:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051123.M
Quant Title :
QLast Update : Thu May 11 11:33:20 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

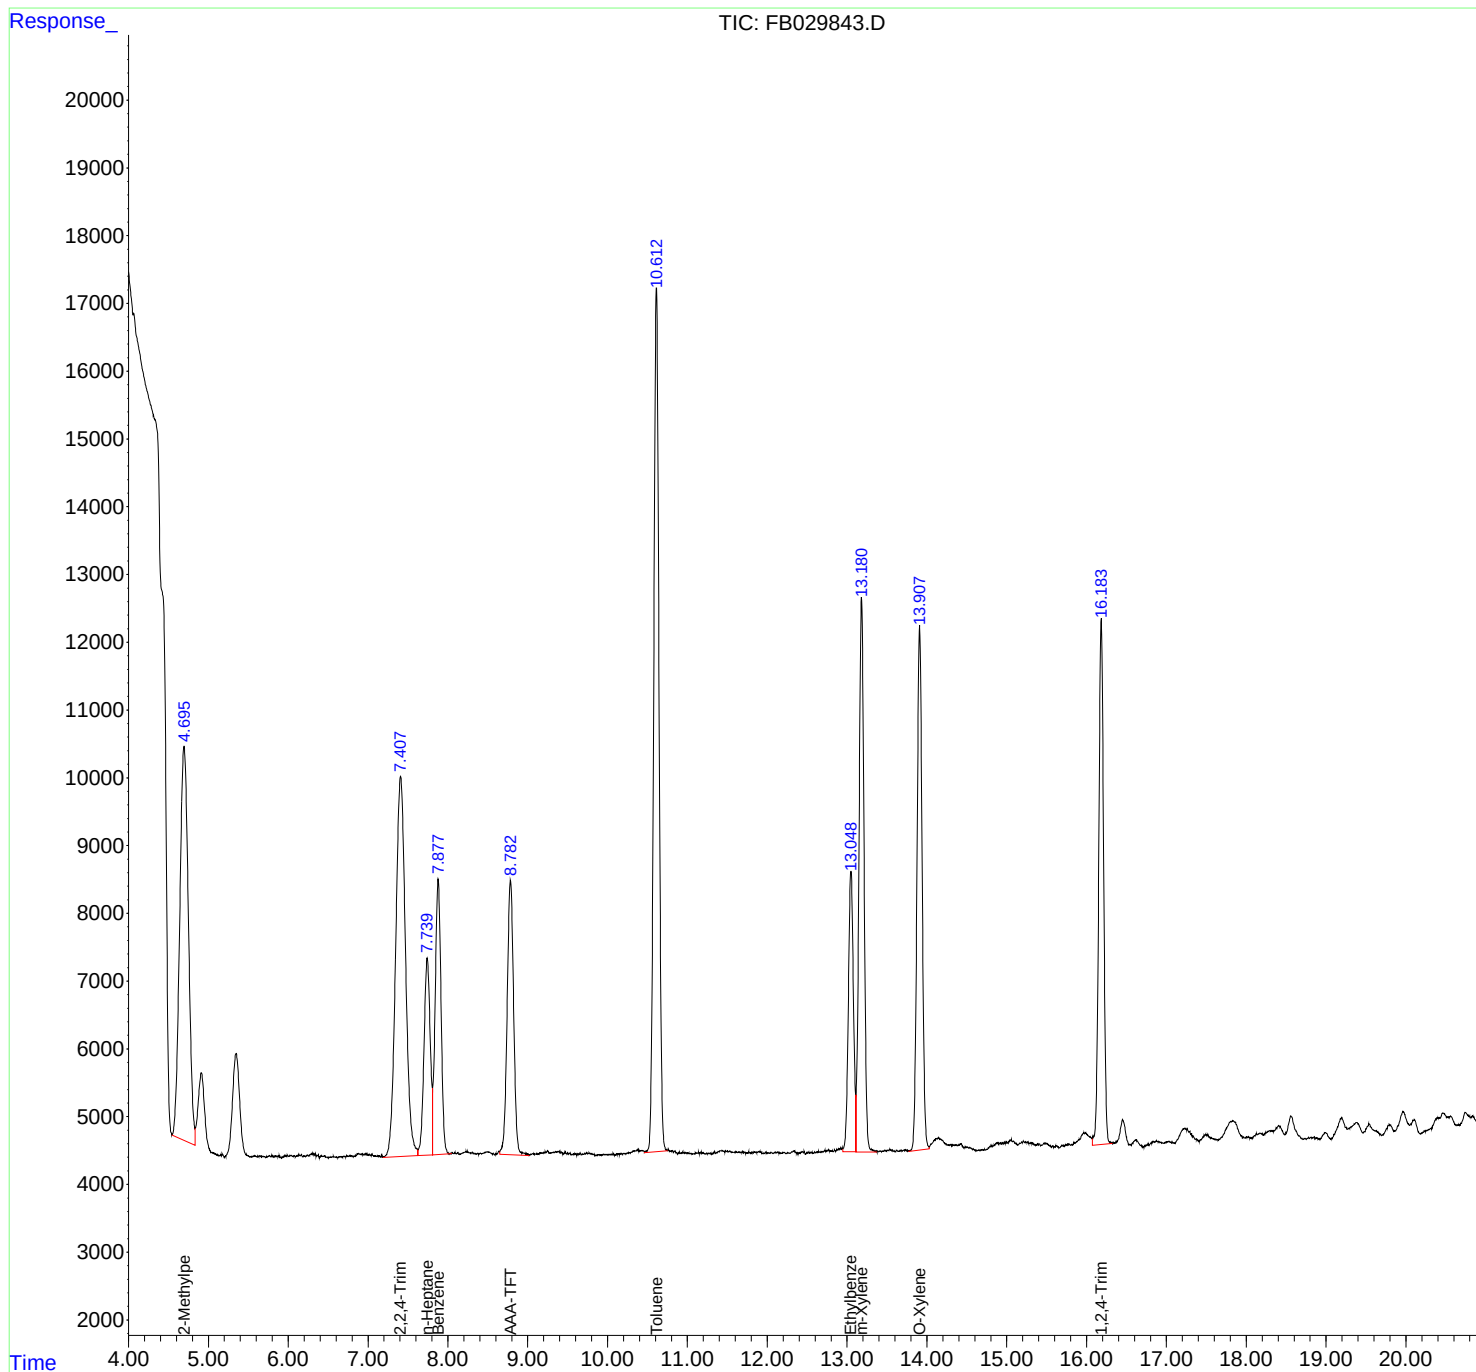


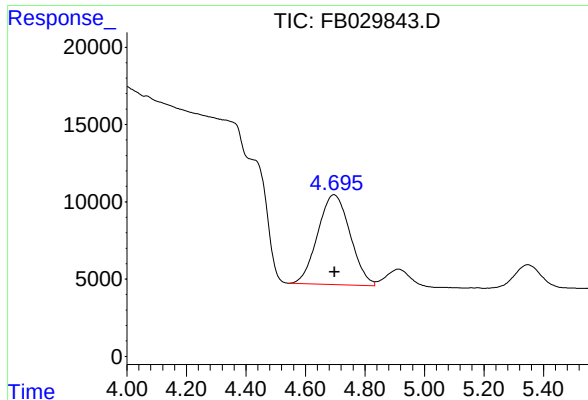

#1 2-Methylpentane


R.T.: 4.696 min
Delta R.T.: -0.003 min
Response: 439705
Conc: 25.66 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-052423MSD

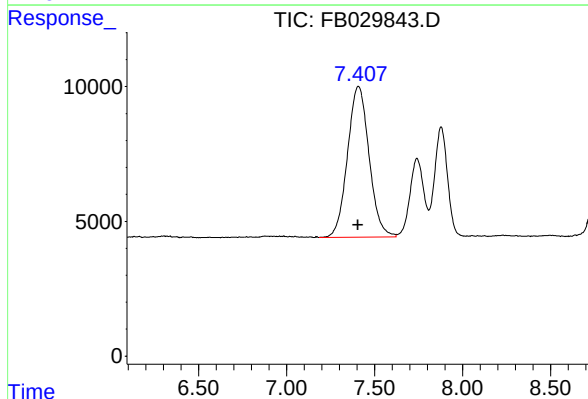


#2 2,2,4-Trimethylpentane

R.T.: 7.408 min
Delta R.T.: 0.002 min
Response: 477421
Conc: 27.97 ng/ml

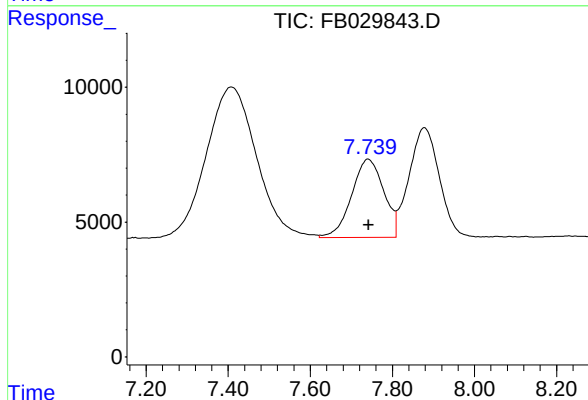


#3 n-Heptane

R.T.: 7.741 min
Delta R.T.: -0.001 min
Response: 158186
Conc: 8.91 ng/ml

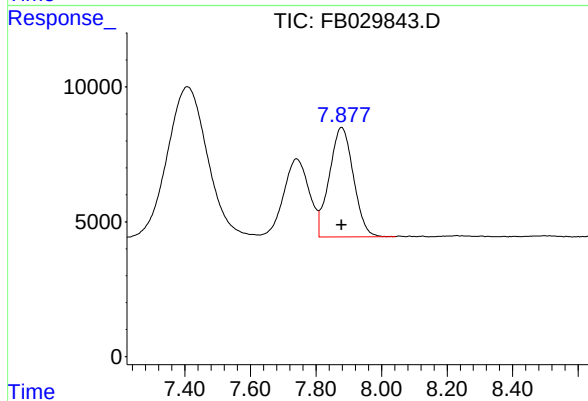

#4 Benzene


R.T.: 7.879 min
Delta R.T.: 0.000 min
Response: 207212
Conc: 9.89 ng/ml

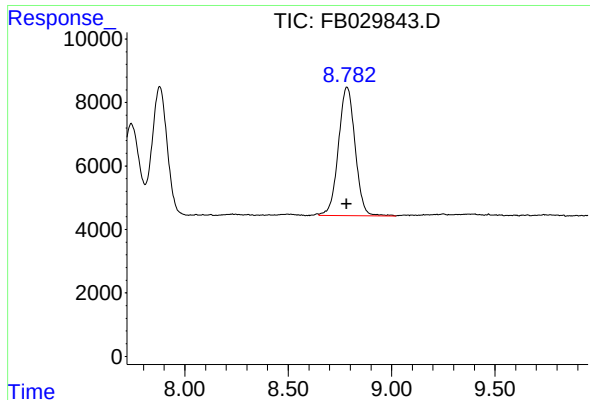

#5 AAA-TFT


R.T.: 8.784 min
Delta R.T.: 0.002 min
Response: 226327
Conc: 18.59 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-052423MSD

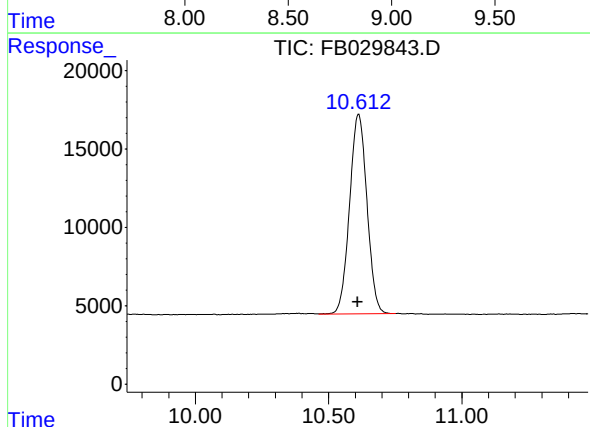


#6 Toluene

R.T.: 10.613 min
Delta R.T.: 0.003 min
Response: 577227
Conc: 28.35 ng/ml

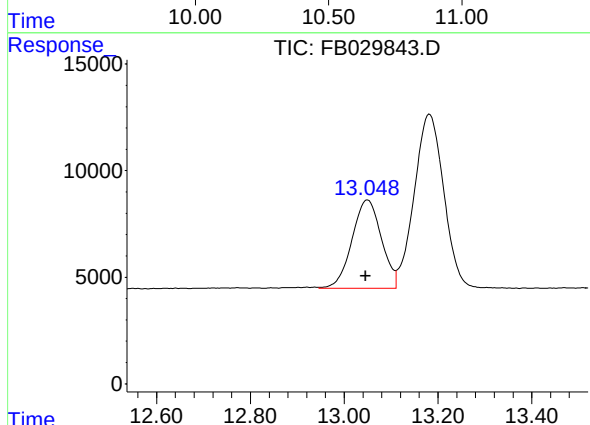


#7 Ethylbenzene

R.T.: 13.050 min
Delta R.T.: 0.004 min
Response: 180725
Conc: 9.43 ng/ml

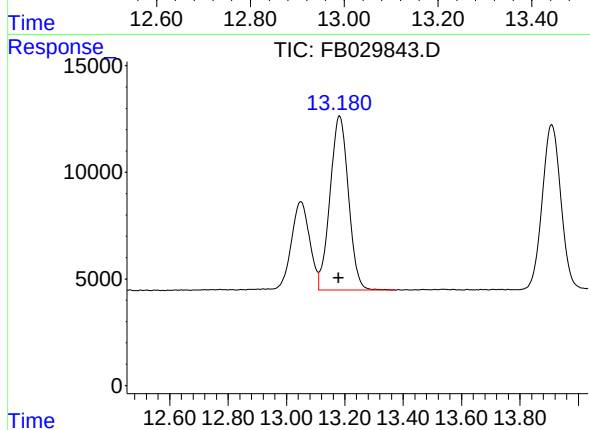

#8 m-Xylene


R.T.: 13.182 min
Delta R.T.: 0.003 min
Response: 358740
Conc: 18.62 ng/ml

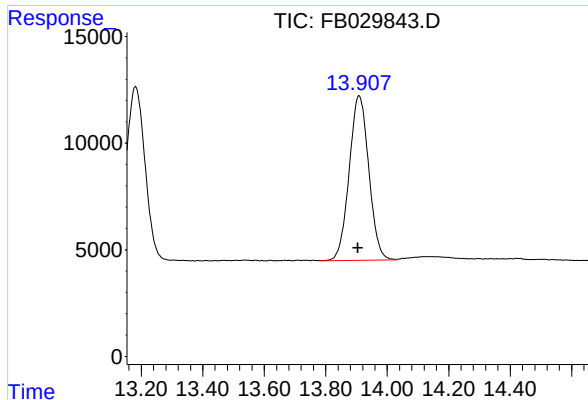

#9 O-Xylene

R.T.: 13.909 min
Delta R.T.: 0.003 min
Response: 341575
Conc: 18.36 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-052423MSD

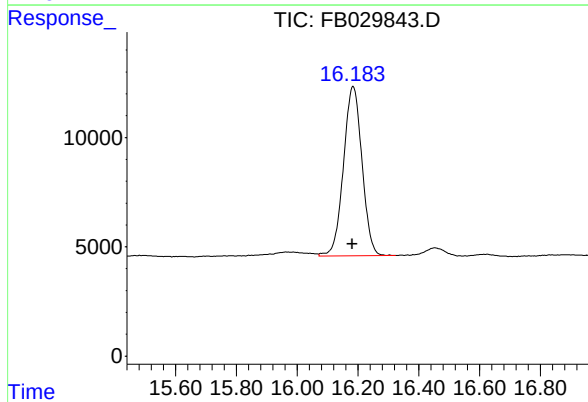

#10 1,2,4-Trimethylbenzene

R.T.: 16.184 min
Delta R.T.: 0.003 min
Response: 327822
Conc: 17.62 ng/ml