

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052620\
 Data File : FB024384.D
 Signal(s) : FID2B.CH
 Acq On : 26 May 2020 11:55
 Operator : DD/AJ
 Sample : 20 PPB GRO STD
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 1 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 27 00:55:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
 Quant Title :
 QLast Update : Mon May 11 11:14:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.801	479359	21.708 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.693	992466	33.631 ng/ml
2) t	2,2,4-Trimethylpentane	7.419	1036988	33.945 ng/ml
3) t	n-Heptane	7.759	343781	11.348 ng/ml
4) t	Benzene	7.894	445866	11.794 ng/ml
6) t	Toluene	10.632	1265490	34.923 ng/ml
7) t	Ethylbenzene	13.072	372892	10.999 ng/ml
8) t	m-Xylene	13.205	730354	22.132 ng/ml
9) t	O-Xylene	13.932	716141	22.192 ng/ml
10) t	1,2,4-Trimethylbenzene	16.209	606473	22.487 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052620\
Data File : FB024384.D
Signal(s) : FID2B.CH
Acq On : 26 May 2020 11:55
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 27 00:55:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

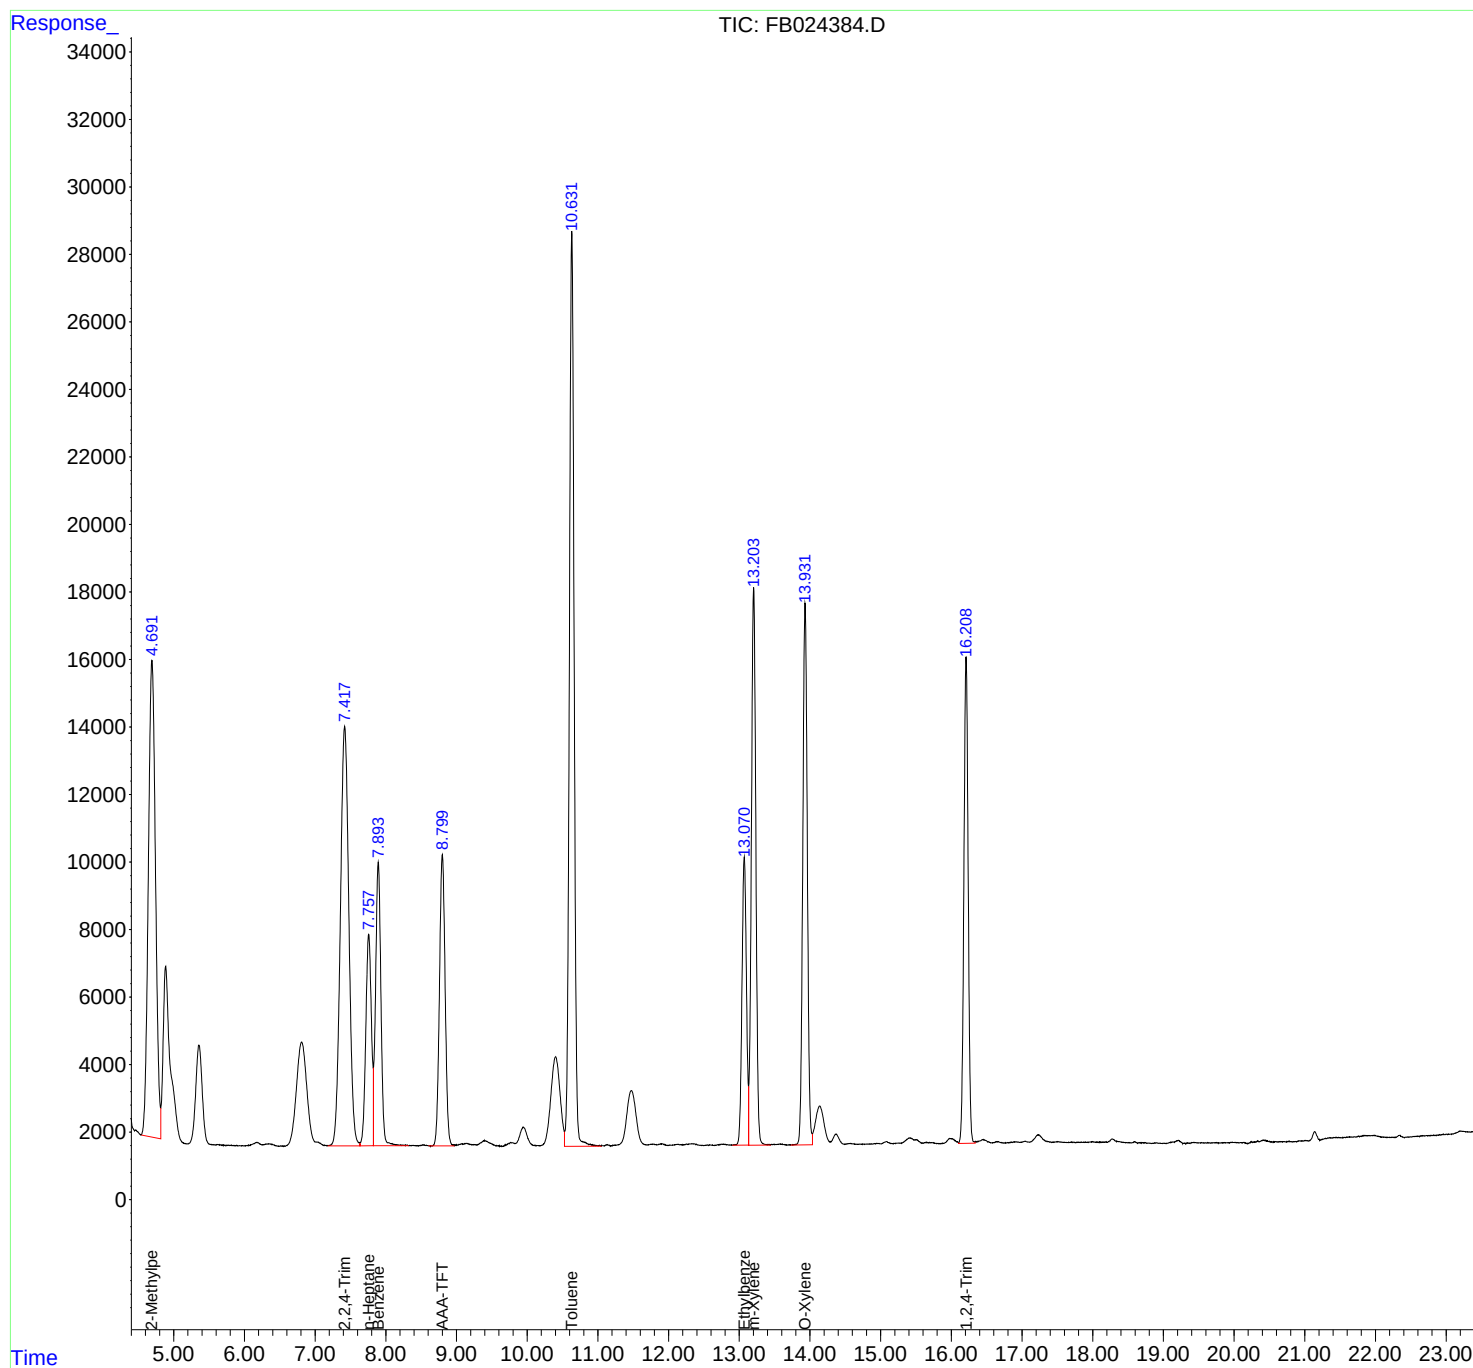

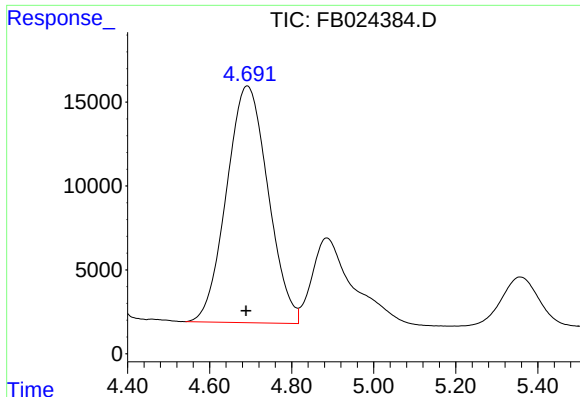


#1 2-Methylpentane

R.T.: 4.693 min
Delta R.T.: 0.004 min
Response: 992466
Conc: 33.63 ng/ml

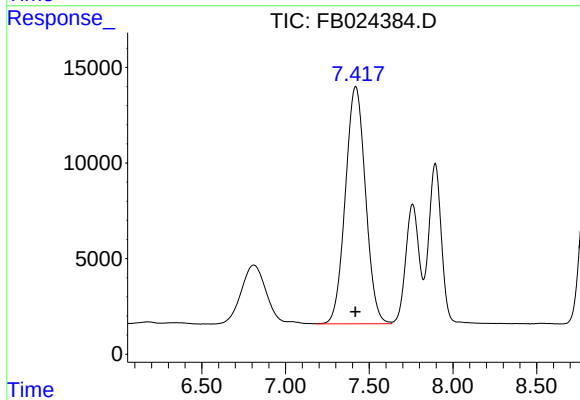


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.002 min
Response: 1036988
Conc: 33.94 ng/ml

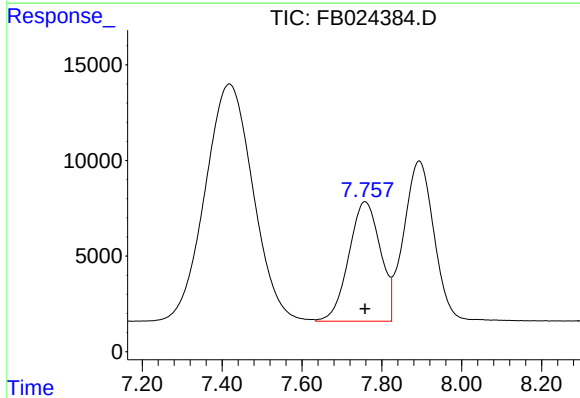


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 343781
Conc: 11.35 ng/ml

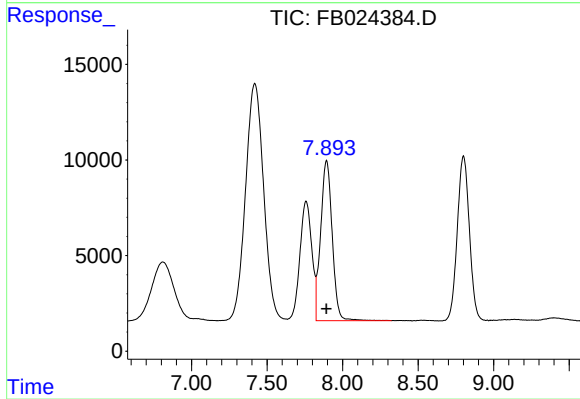


#4 Benzene

R.T.: 7.894 min
Delta R.T.: 0.001 min
Response: 445866
Conc: 11.79 ng/ml

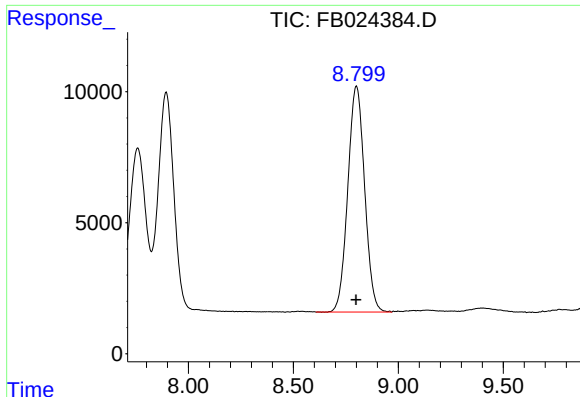


#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.001 min
Response: 479359
Conc: 21.71 ng/ml

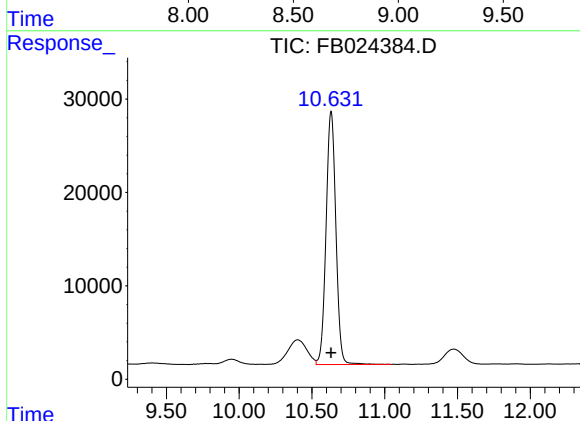


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.001 min
Response: 1265490
Conc: 34.92 ng/ml

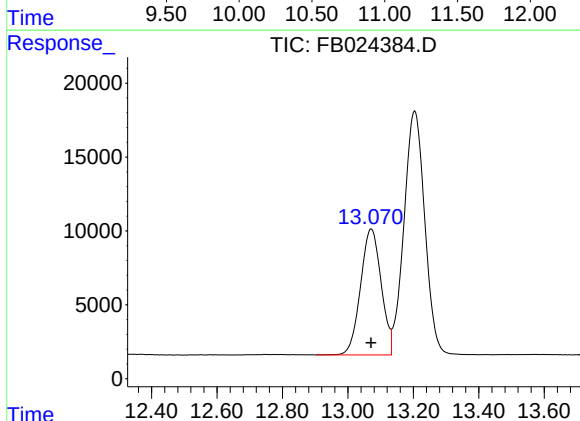


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 372892
Conc: 11.00 ng/ml

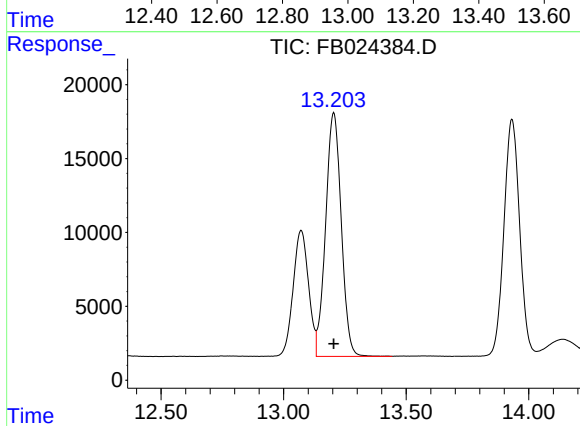


#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.000 min
Response: 730354
Conc: 22.13 ng/ml

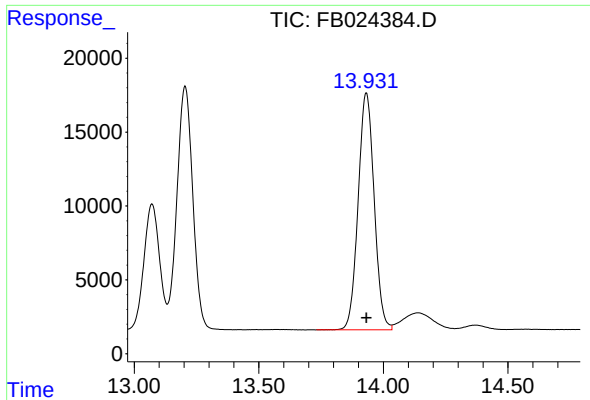

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 716141
Conc: 22.19 ng/ml

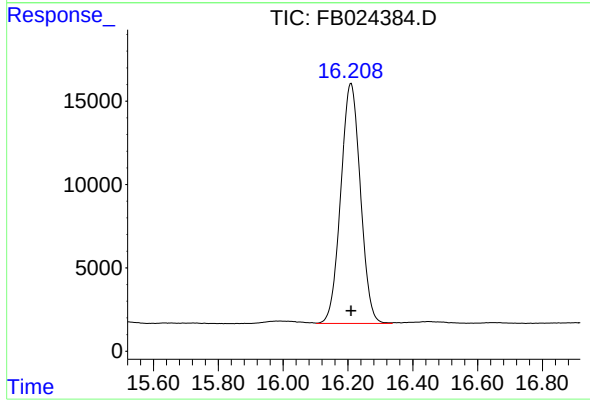

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 606473
Conc: 22.49 ng/ml