

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052623\
 Data File : FB029865.D
 Signal(s) : FID2B.CH
 Acq On : 26 May 2023 17:04
 Operator : YP/AJ
 Sample : BSF0526S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0526S2

Integration File: Calibration.e
 Quant Time: May 27 04:29:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051123.M
 Quant Title :
 QLast Update : Thu May 11 11:33:20 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.786	217285	17.843 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	452997	26.439 ng/ml
2) t 2,2,4-Trimethylpentane	7.410	502540	29.444 ng/ml
3) t n-Heptane	7.745	150421	8.470 ng/ml
4) t Benzene	7.881	187809	8.965 ng/ml
6) t Toluene	10.614	542915	26.664 ng/ml
7) t Ethylbenzene	13.051	174660	9.114 ng/ml
8) t m-Xylene	13.184	347728	18.047 ng/ml
9) t O-Xylene	13.910	343304	18.455 ng/ml
10) t 1,2,4-Trimethylbenzene	16.185	352092	18.929 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052623\
Data File : FB029865.D
Signal(s) : FID2B.CH
Acq On : 26 May 2023 17:04
Operator : YP/AJ
Sample : BSF0526S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0526S2

Integration File: Calibration.e
Quant Time: May 27 04:29:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051123.M
Quant Title :
QLast Update : Thu May 11 11:33:20 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

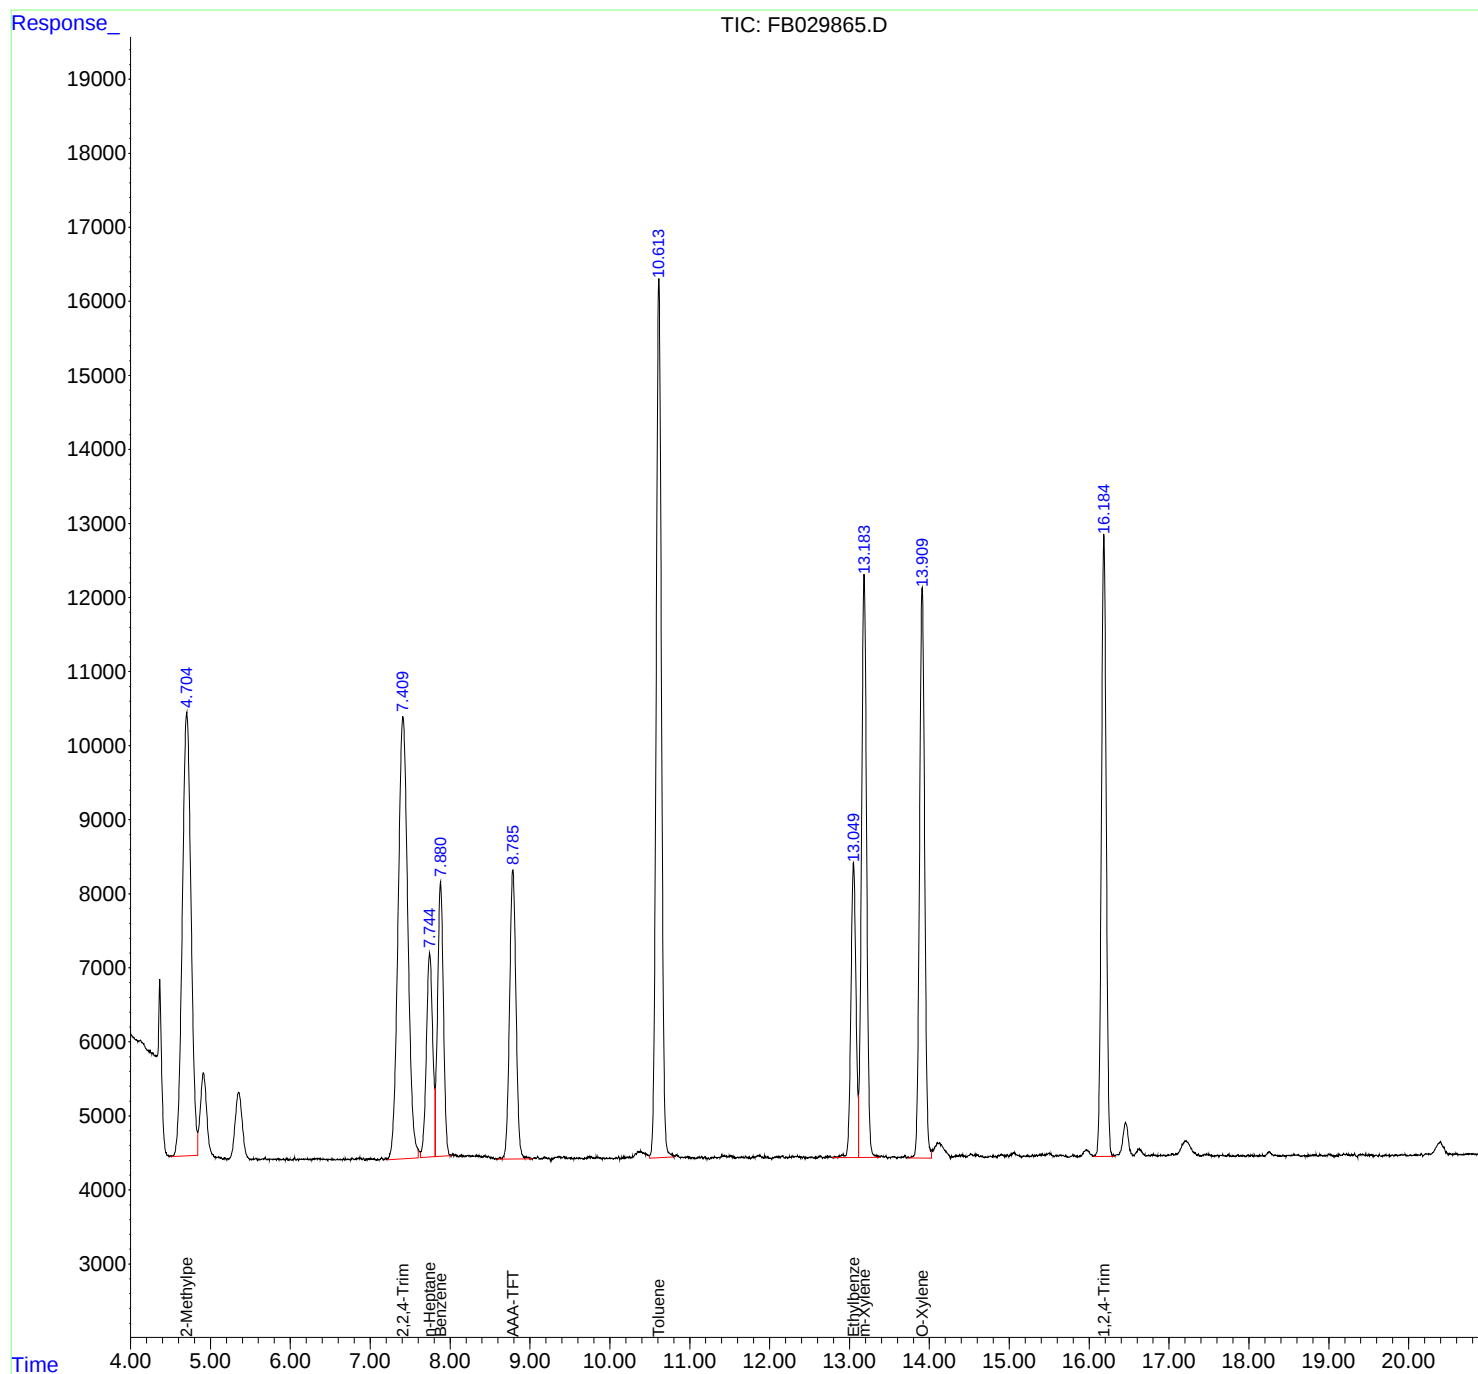


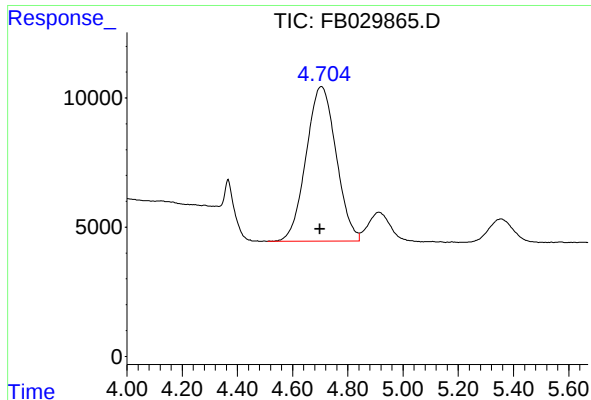

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: 0.006 min
Response: 452997
Conc: 26.44 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0526S2

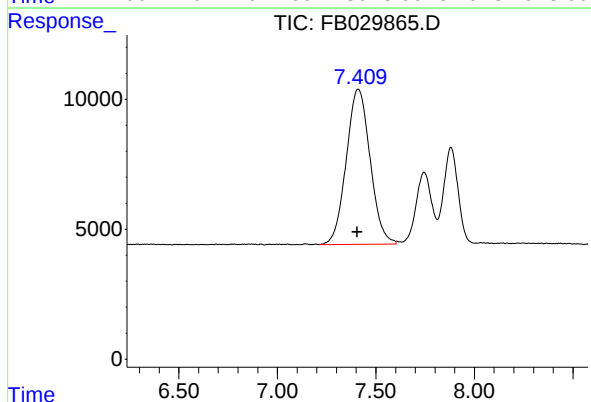


#2 2,2,4-Trimethylpentane

R.T.: 7.410 min
Delta R.T.: 0.004 min
Response: 502540
Conc: 29.44 ng/ml

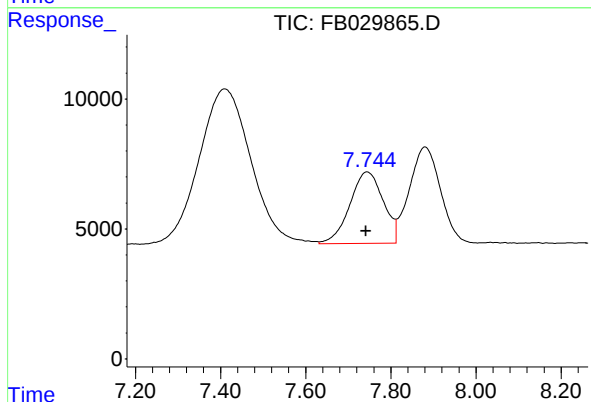


#3 n-Heptane

R.T.: 7.745 min
Delta R.T.: 0.003 min
Response: 150421
Conc: 8.47 ng/ml

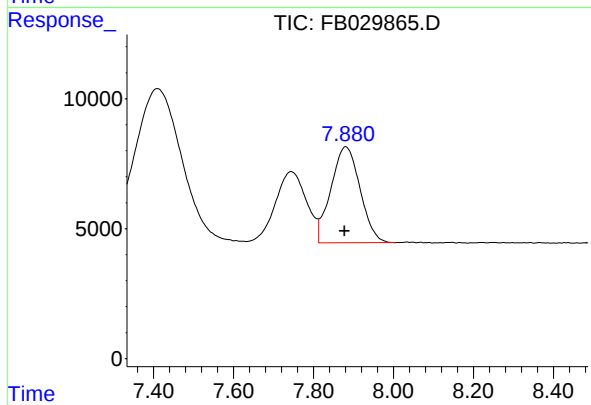

#4 Benzene


R.T.: 7.881 min
Delta R.T.: 0.003 min
Response: 187809
Conc: 8.97 ng/ml

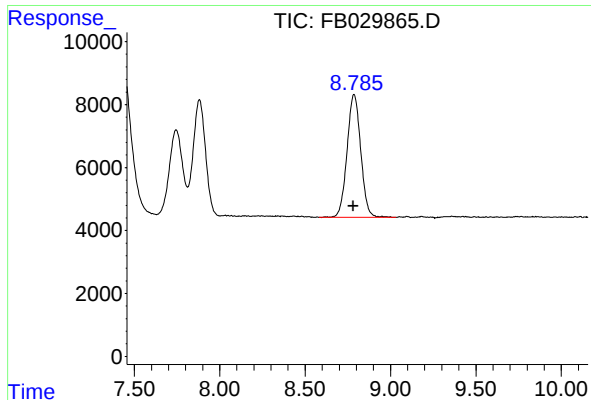

#5 AAA-TFT


R.T.: 8.786 min
Delta R.T.: 0.004 min
Response: 217285
Conc: 17.84 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0526S2

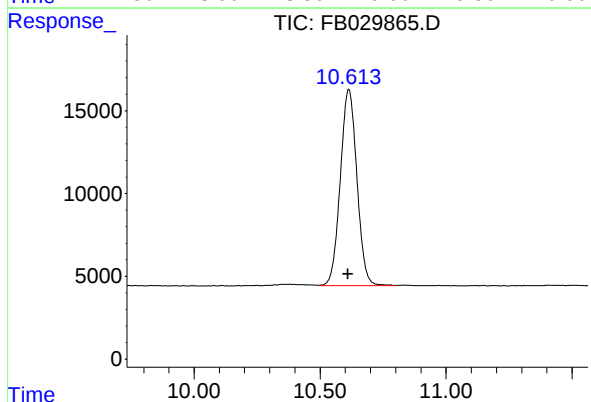


#6 Toluene

R.T.: 10.614 min
Delta R.T.: 0.004 min
Response: 542915
Conc: 26.66 ng/ml

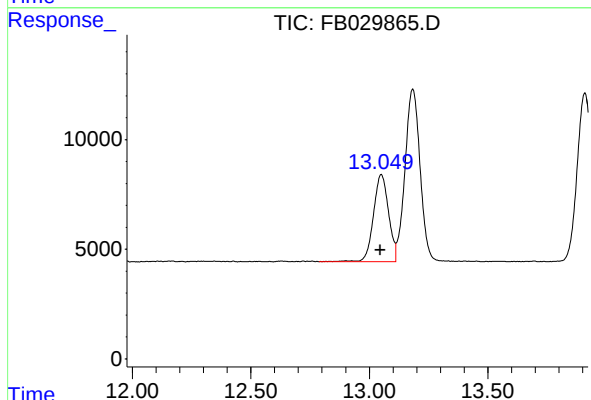


#7 Ethylbenzene

R.T.: 13.051 min
Delta R.T.: 0.005 min
Response: 174660
Conc: 9.11 ng/ml

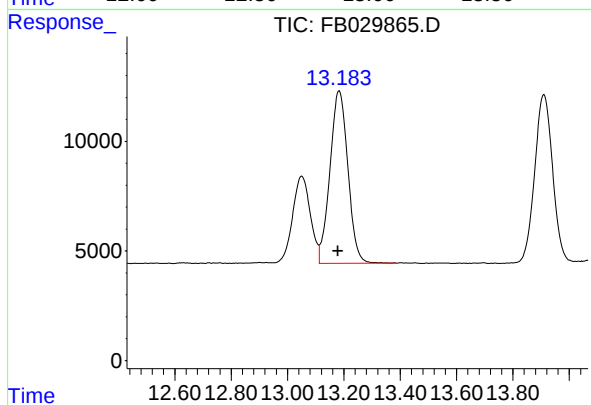

#8 m-Xylene


R.T.: 13.184 min
Delta R.T.: 0.005 min
Response: 347728
Conc: 18.05 ng/ml

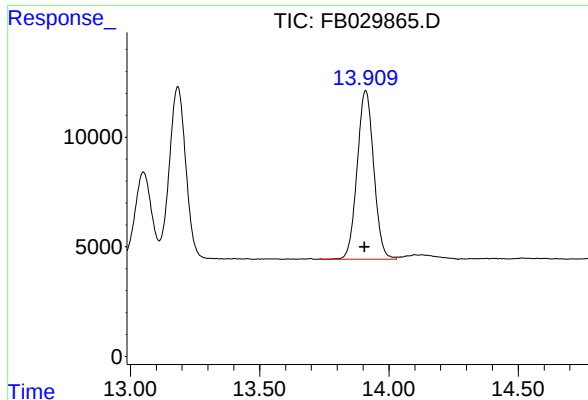

#9 O-Xylene

R.T.: 13.910 min
Delta R.T.: 0.004 min
Response: 343304
Conc: 18.46 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0526S2

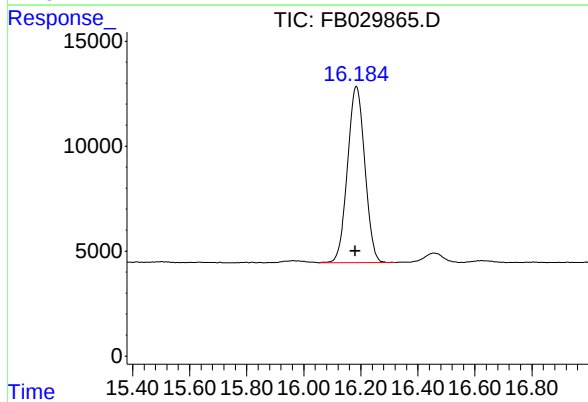

#10 1,2,4-Trimethylbenzene

R.T.: 16.185 min
Delta R.T.: 0.004 min
Response: 352092
Conc: 18.93 ng/ml