

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052820\
 Data File : FB024394.D
 Signal(s) : FID2B.CH
 Acq On : 28 May 2020 10:21
 Operator : DD/AJ
 Sample : 20 PPB GRO STD
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 1 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 29 01:19:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
 Quant Title :
 QLast Update : Mon May 11 11:14:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	478300	21.660 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	932586	31.602 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	1002215	32.806 ng/ml
3) t n-Heptane	7.756	334710	11.048 ng/ml
4) t Benzene	7.892	424386	11.226 ng/ml
6) t Toluene	10.629	1184602	32.691 ng/ml
7) t Ethylbenzene	13.069	352825	10.407 ng/ml
8) t m-Xylene	13.202	692564	20.987 ng/ml
9) t O-Xylene	13.930	685065	21.229 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	585032	21.692 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052820\
Data File : FB024394.D
Signal(s) : FID2B.CH
Acq On : 28 May 2020 10:21
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 29 01:19:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

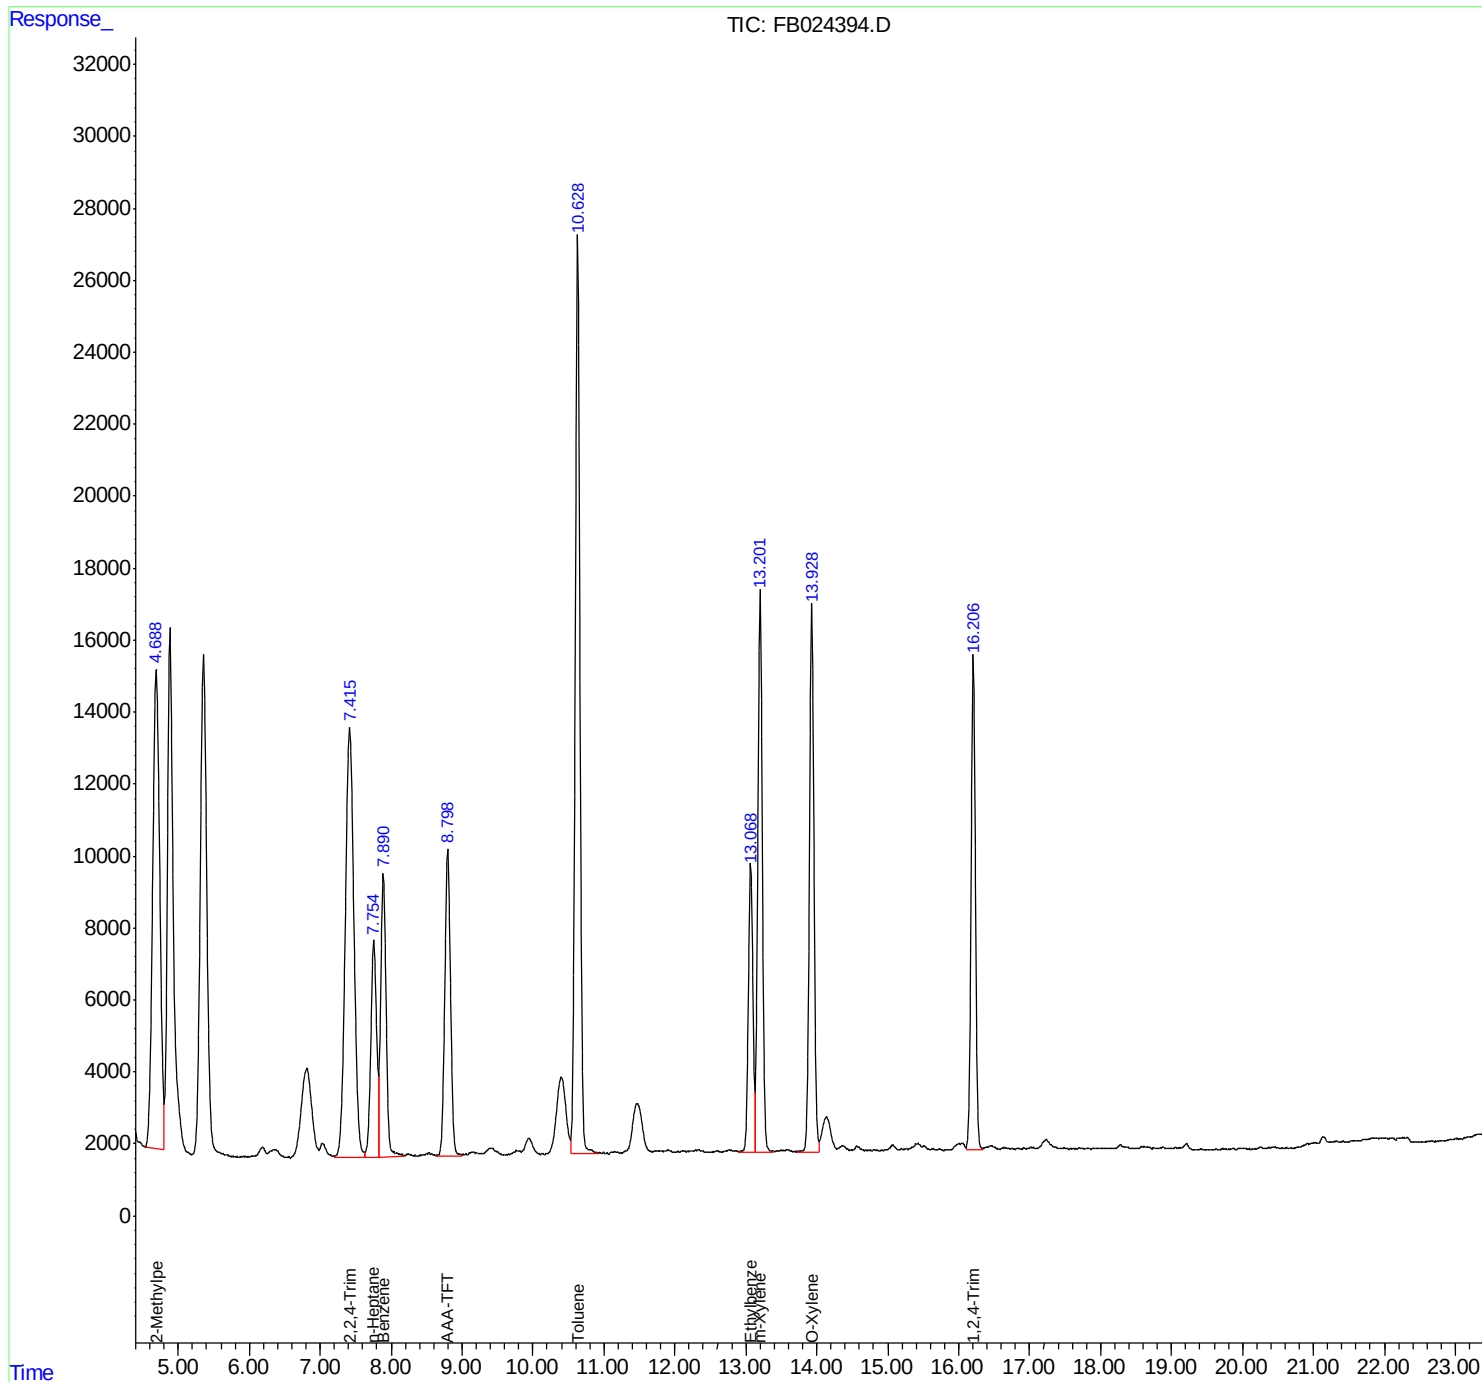

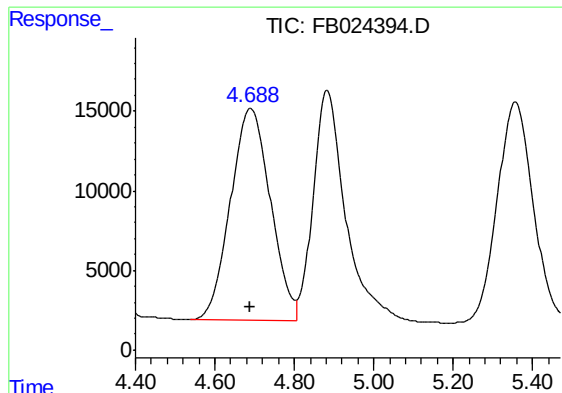


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: 0.000 min
Response: 932586
Conc: 31.60 ng/ml

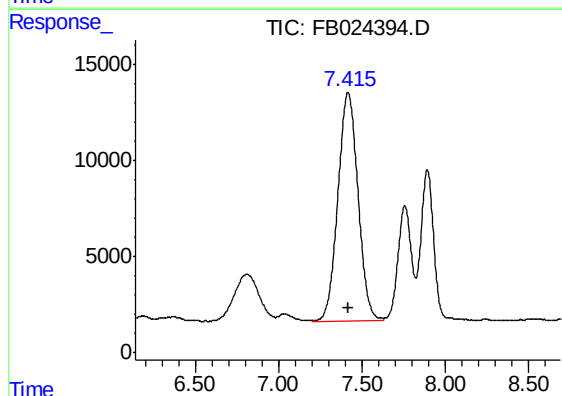


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.001 min
Response: 1002215
Conc: 32.81 ng/ml

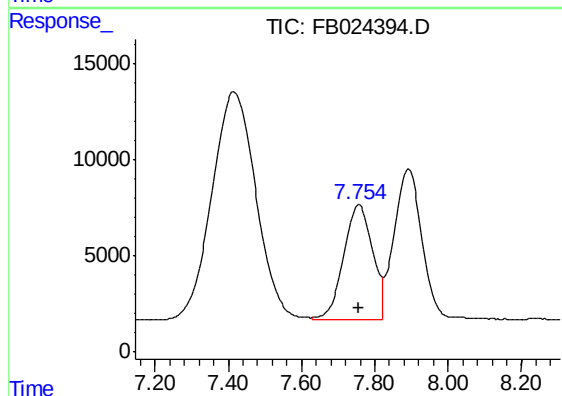


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.002 min
Response: 334710
Conc: 11.05 ng/ml

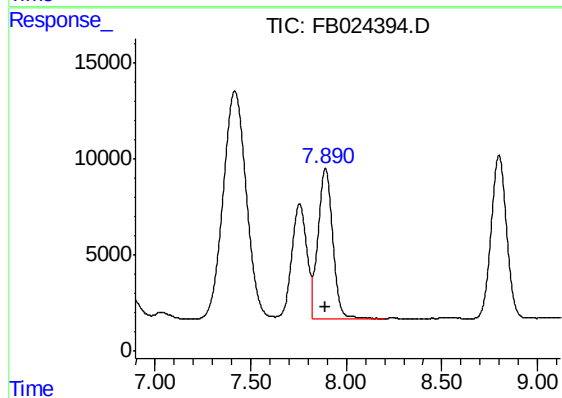


#4 Benzene

R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 424386
Conc: 11.23 ng/ml

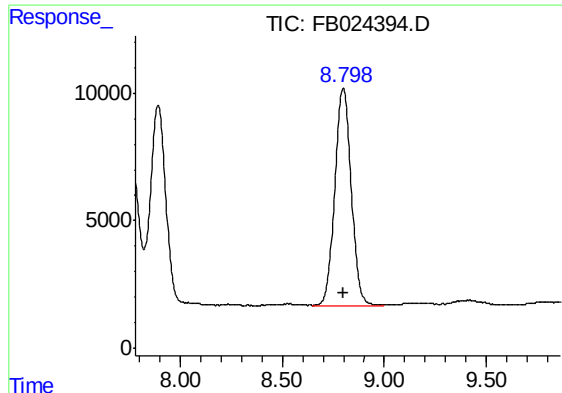


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 478300
Conc: 21.66 ng/ml

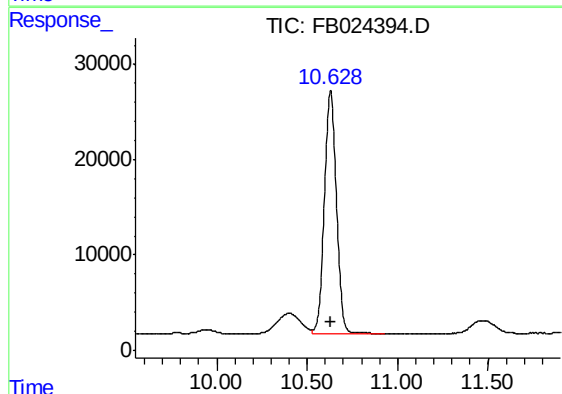


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.001 min
Response: 1184602
Conc: 32.69 ng/ml

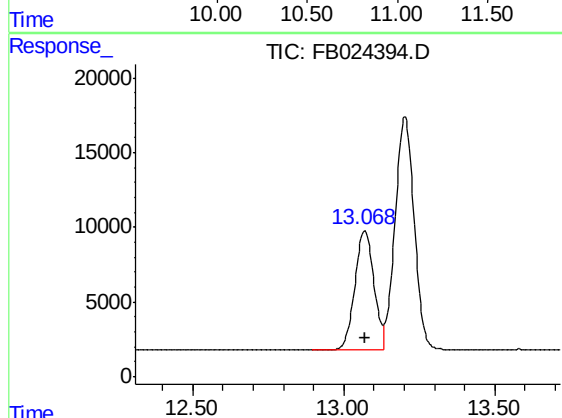


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.002 min
Response: 352825
Conc: 10.41 ng/ml

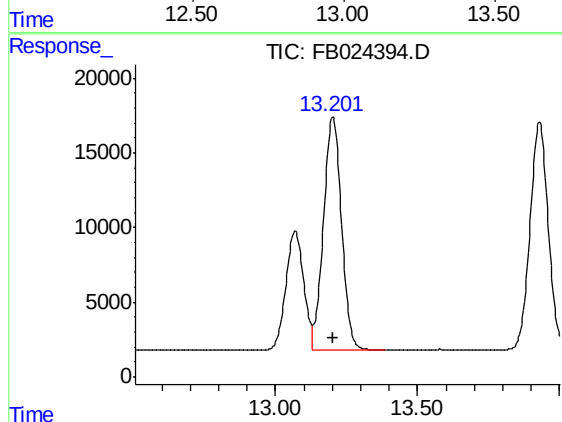


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: -0.002 min
Response: 692564
Conc: 20.99 ng/ml

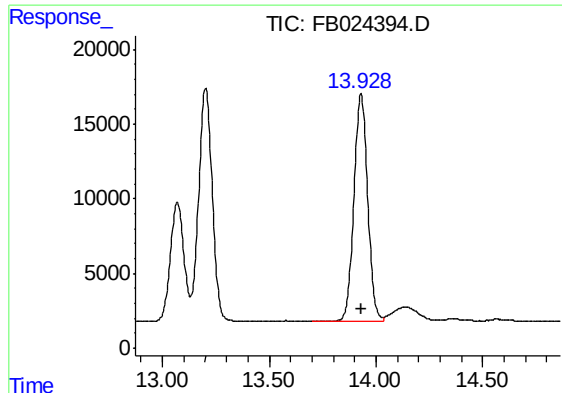

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.002 min
Response: 685065
Conc: 21.23 ng/ml

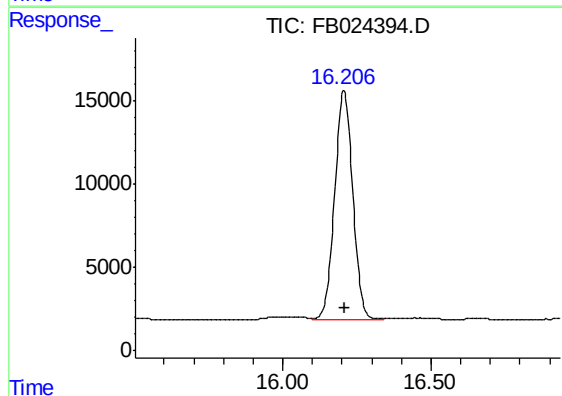

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.003 min
Response: 585032
Conc: 21.69 ng/ml