

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB052820\  
Data File : FB024402.D  
Signal(s) : FID2B.CH  
Acq On : 28 May 2020 14:38  
Operator : DD/AJ  
Sample : L2790-05  
Misc : 5.01g/5.00ml DI WATER  
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: May 29 01:21:13 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB051120.M  
Quant Title :  
QLast Update : Mon May 11 11:14:42 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| 5) s AAA-TFT                | 8.806  | 467343   | 21.164 ng/ml |
| Target Compounds            |        |          |              |
| 1) t 2-Methylpentane        | 4.690  | 920      | 0.031 ng/ml  |
| 6) t Toluene                | 10.619 | 1286     | 0.035 ng/ml  |
| 8) t m-Xylene               | 13.217 | 886      | 0.027 ng/ml  |
| 9) t O-Xylene               | 13.944 | 1346     | 0.042 ng/ml  |
| -----                       |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB052820\  
Data File : FB024402.D  
Signal(s) : FID2B.CH  
Acq On : 28 May 2020 14:38  
Operator : DD/AJ  
Sample : L2790-05  
Misc : 5.01g/5.00ml DI WATER  
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: May 29 01:21:13 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB051120.M  
Quant Title :  
QLast Update : Mon May 11 11:14:42 2020  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

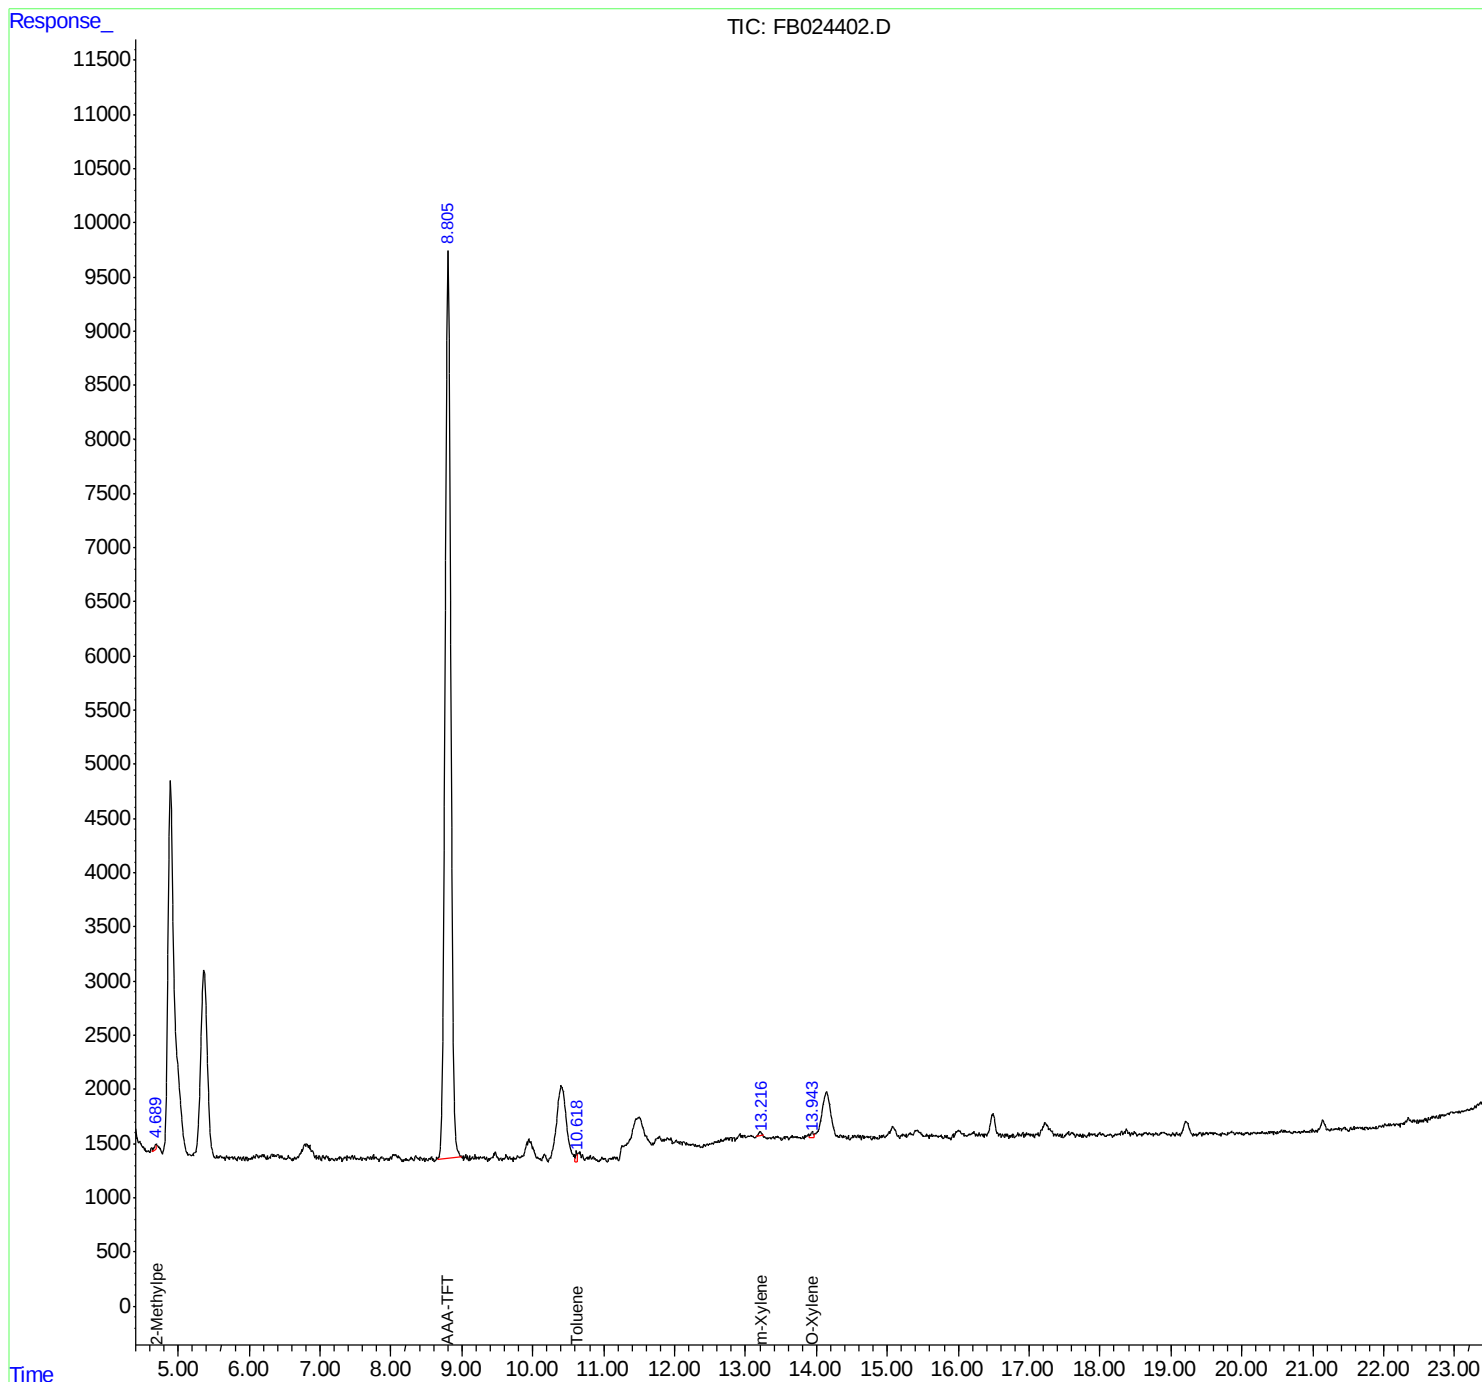

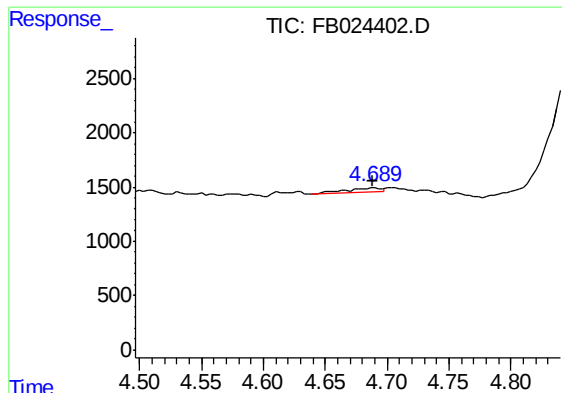


#1 2-Methylpentane

R.T.: 4.690 min  
Delta R.T.: 0.001 min  
Response: 920  
Conc: 0.03 ng/ml

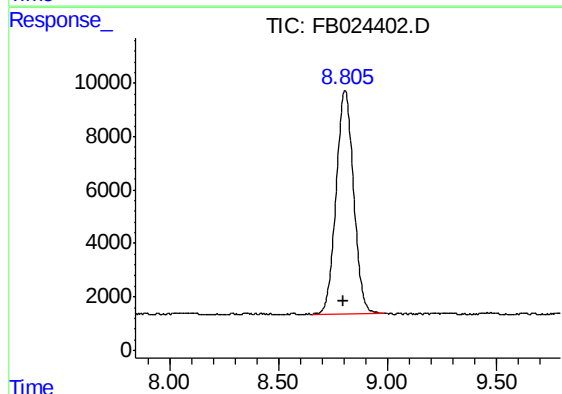


#5 AAA-TFT

R.T.: 8.806 min  
Delta R.T.: 0.007 min  
Response: 467343  
Conc: 21.16 ng/ml

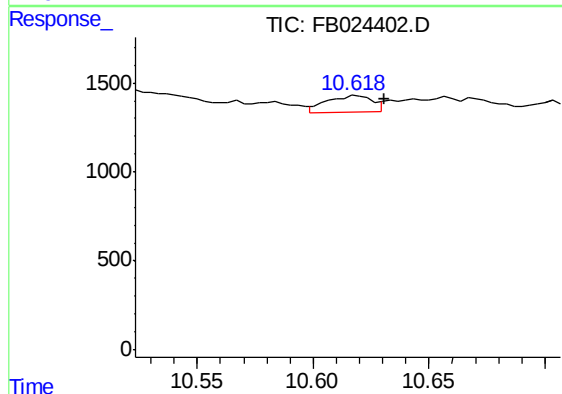


#6 Toluene

R.T.: 10.619 min  
Delta R.T.: -0.012 min  
Response: 1286  
Conc: 0.04 ng/ml

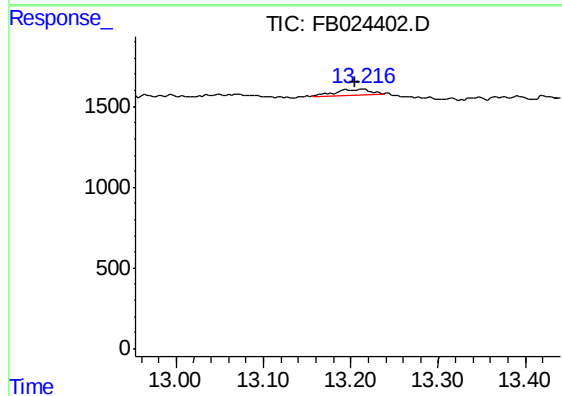

#8 m-Xylene

R.T.: 13.217 min  
Delta R.T.: 0.012 min  
Response: 886  
Conc: 0.03 ng/ml

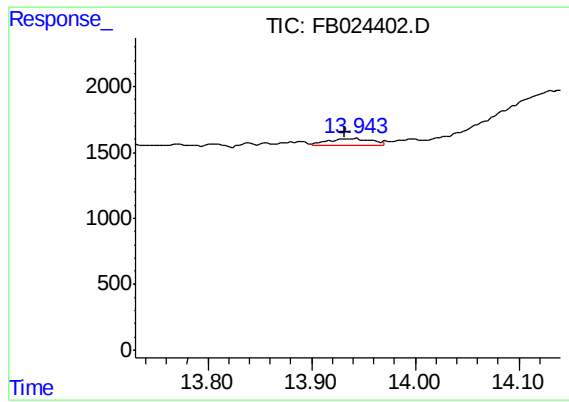

#9 O-Xylene

R.T.: 13.944 min  
Delta R.T.: 0.011 min  
Response: 1346  
Conc: 0.04 ng/ml