

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052824\
 Data File : FB030766.D
 Signal(s) : FID2B.CH
 Acq On : 28 May 2024 14:36
 Operator : YP/AJ
 Sample : P2611-01MS 50X
 Misc : 5.07G/5.00 ML MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 AU-06-052424MS

Integration File: Calibration.e
 Quant Time: May 29 06:14:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB050824.M
 Quant Title :
 QLast Update : Wed May 08 14:36:01 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.787	253206	18.349 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.697	504555	28.799 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	531158	29.558 ng/ml
3) t n-Heptane	7.744	198383	9.950 ng/ml
4) t Benzene	7.881	248978	10.993 ng/ml
6) t Toluene	10.615	718232	32.267 ng/ml
7) t Ethylbenzene	13.052	220005	10.661 ng/ml
8) t m-Xylene	13.185	436545	20.957 ng/ml
9) t O-Xylene	13.912	417008	21.845 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	375976	19.879 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052824\
Data File : FB030766.D
Signal(s) : FID2B.CH
Acq On : 28 May 2024 14:36
Operator : YP/AJ
Sample : P2611-01MS 50X
Misc : 5.07G/5.00 ML MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
AU-06-052424MS

Integration File: Calibration.e
Quant Time: May 29 06:14:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB050824.M
Quant Title :
QLast Update : Wed May 08 14:36:01 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

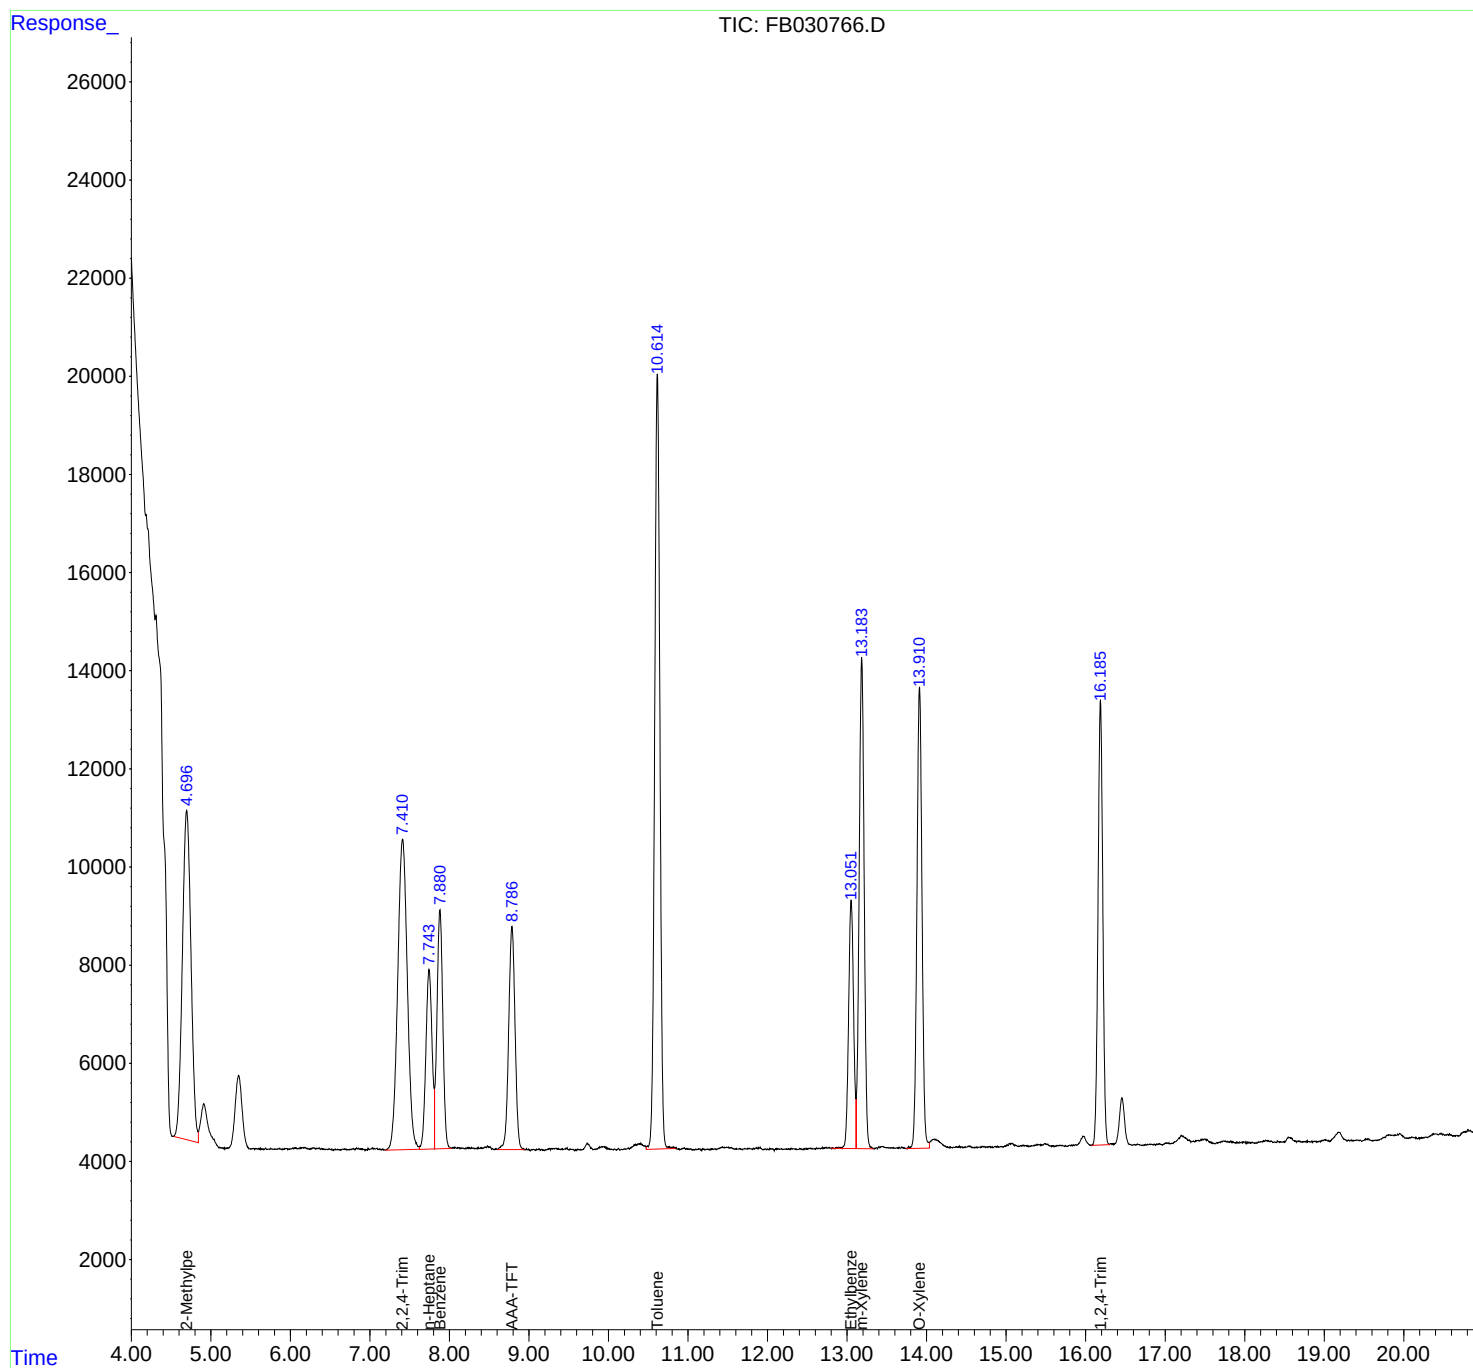


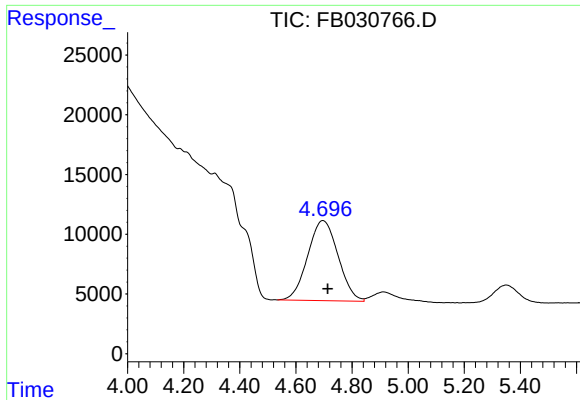

#1 2-Methylpentane


R.T.: 4.697 min
Delta R.T.: -0.016 min
Response: 504555
Conc: 28.80 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-052424MS

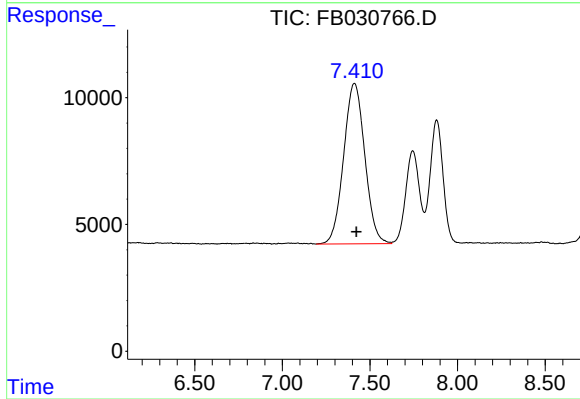


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.010 min
Response: 531158
Conc: 29.56 ng/ml

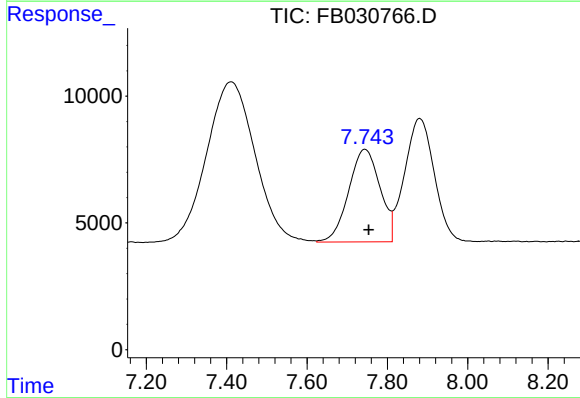


#3 n-Heptane

R.T.: 7.744 min
Delta R.T.: -0.009 min
Response: 198383
Conc: 9.95 ng/ml

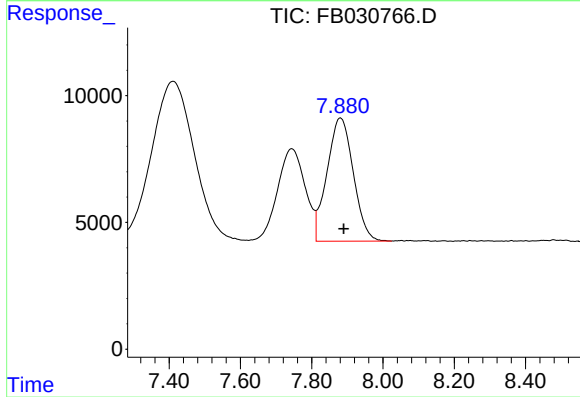

#4 Benzene


R.T.: 7.881 min
Delta R.T.: -0.009 min
Response: 248978
Conc: 10.99 ng/ml

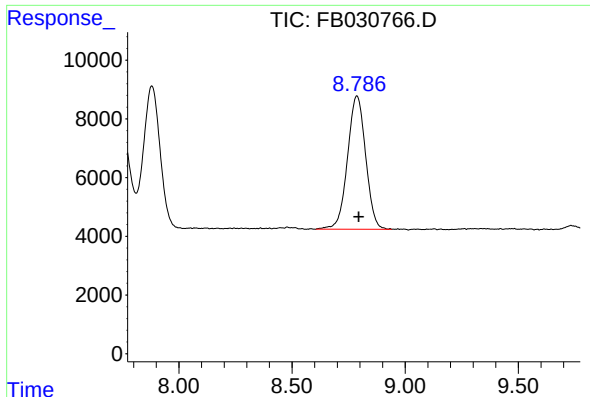

#5 AAA-TFT


R.T.: 8.787 min
Delta R.T.: -0.008 min
Response: 253206
Conc: 18.35 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-052424MS

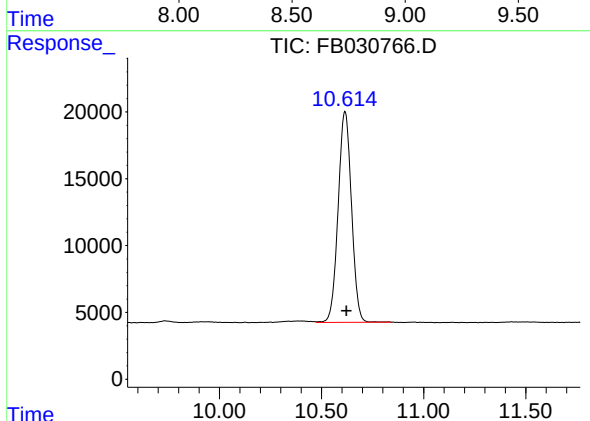


#6 Toluene

R.T.: 10.615 min
Delta R.T.: -0.008 min
Response: 718232
Conc: 32.27 ng/ml

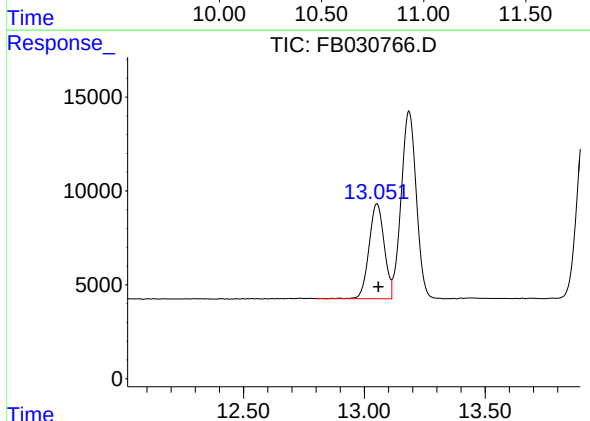


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: -0.007 min
Response: 220005
Conc: 10.66 ng/ml

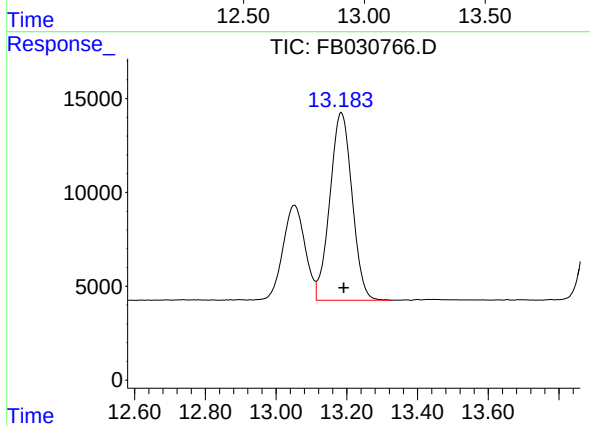

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: -0.007 min
Response: 436545
Conc: 20.96 ng/ml

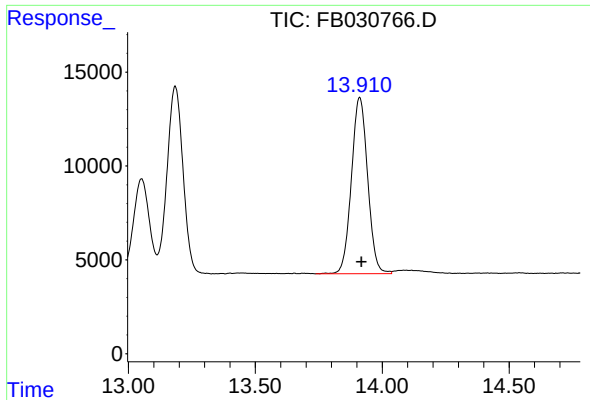

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.007 min
Response: 417008
Conc: 21.85 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-052424MS

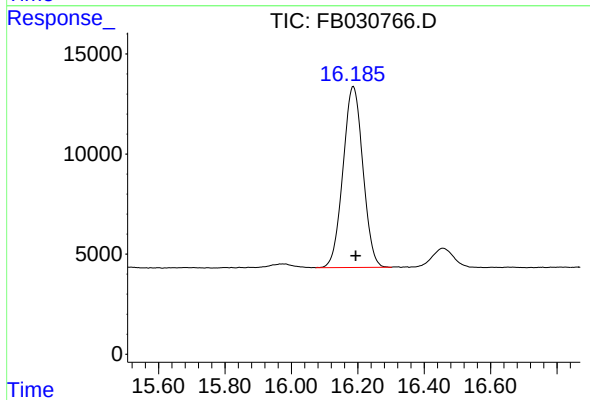

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: -0.007 min
Response: 375976
Conc: 19.88 ng/ml