

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052824\
 Data File : FB030767.D
 Signal(s) : FID2B.CH
 Acq On : 28 May 2024 15:15
 Operator : YP/AJ
 Sample : P2611-01MSD 50X
 Misc : 5.03G/5.00 ML MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 AU-06-052424MSD

Integration File: Calibration.e
 Quant Time: May 29 06:14:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB050824.M
 Quant Title :
 QLast Update : Wed May 08 14:36:01 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.787	252195	18.275 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.699	498463	28.451 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	530503	29.522 ng/ml
3) t n-Heptane	7.744	193496	9.705 ng/ml
4) t Benzene	7.882	244555	10.798 ng/ml
6) t Toluene	10.615	694543	31.202 ng/ml
7) t Ethylbenzene	13.052	214602	10.399 ng/ml
8) t m-Xylene	13.185	426937	20.496 ng/ml
9) t O-Xylene	13.912	406966	21.319 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	362990	19.192 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052824\
Data File : FB030767.D
Signal(s) : FID2B.CH
Acq On : 28 May 2024 15:15
Operator : YP/AJ
Sample : P2611-01MSD 50X
Misc : 5.03G/5.00 ML MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
AU-06-052424MSD

Integration File: Calibration.e
Quant Time: May 29 06:14:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB050824.M
Quant Title :
QLast Update : Wed May 08 14:36:01 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

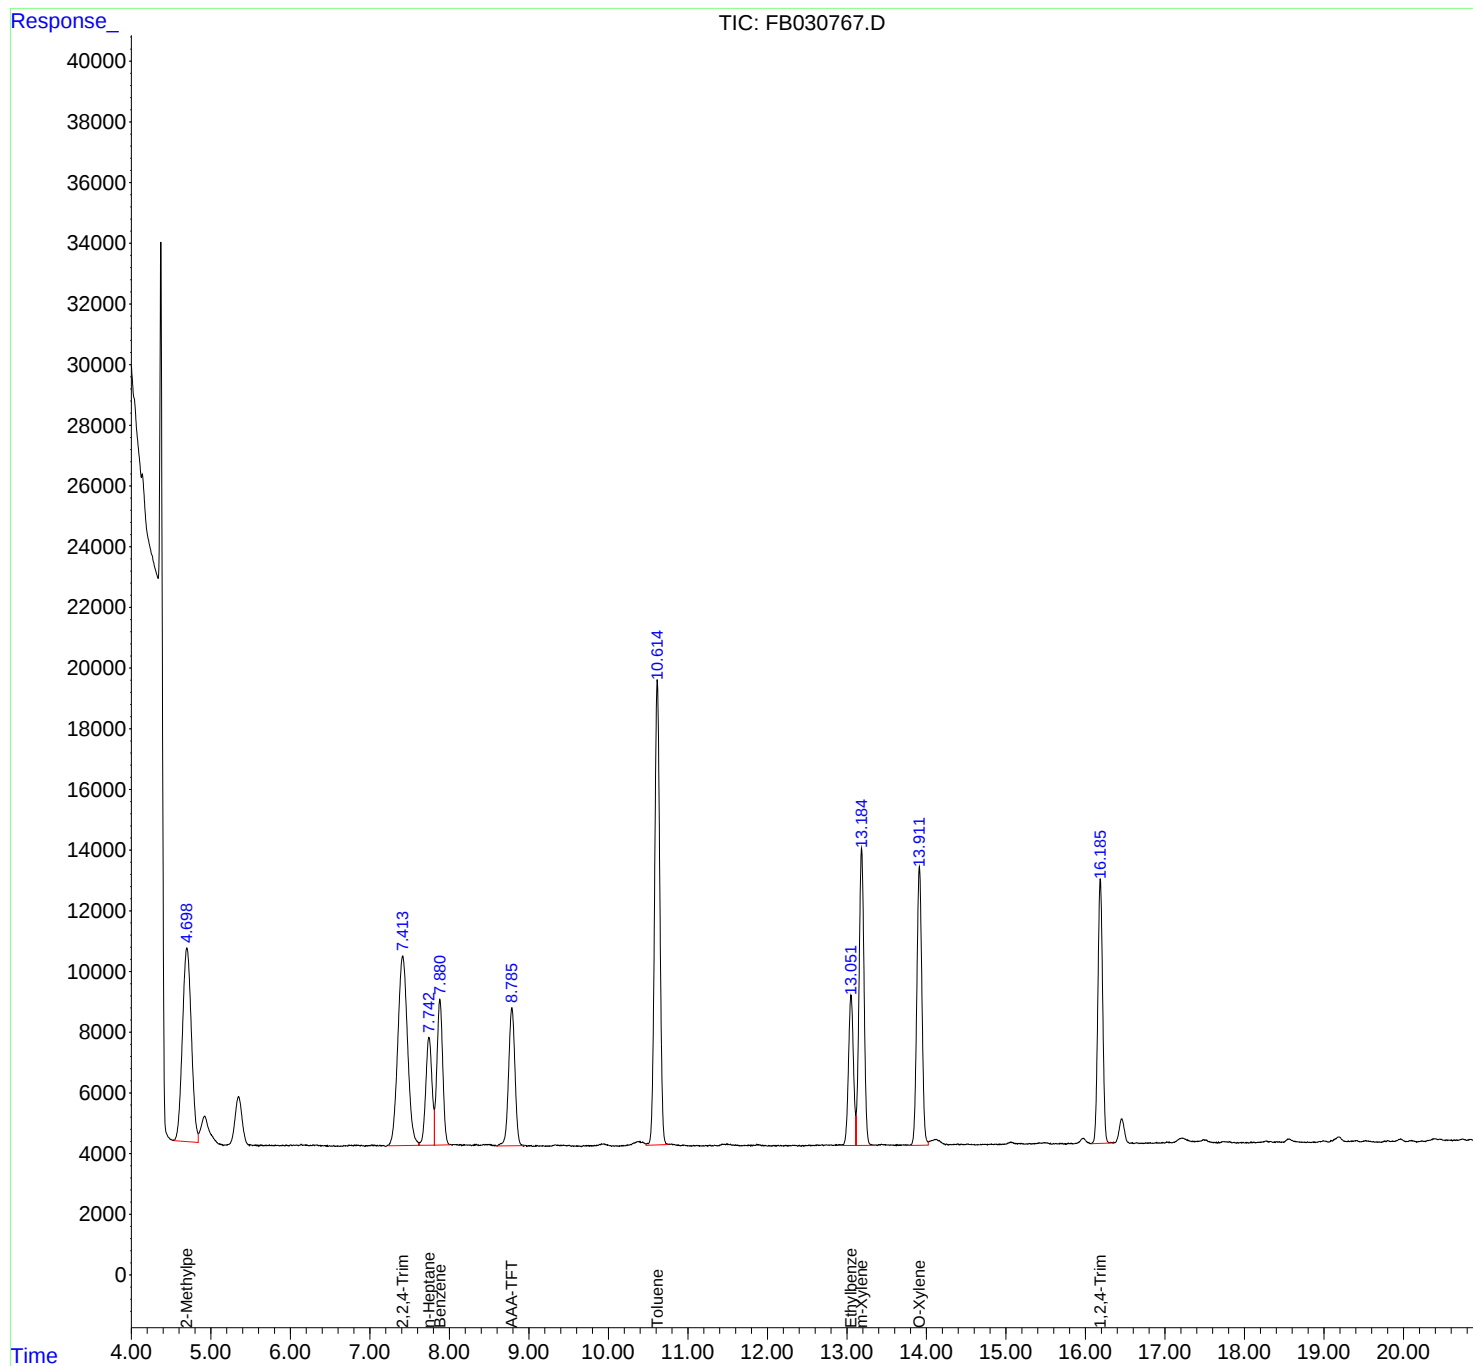


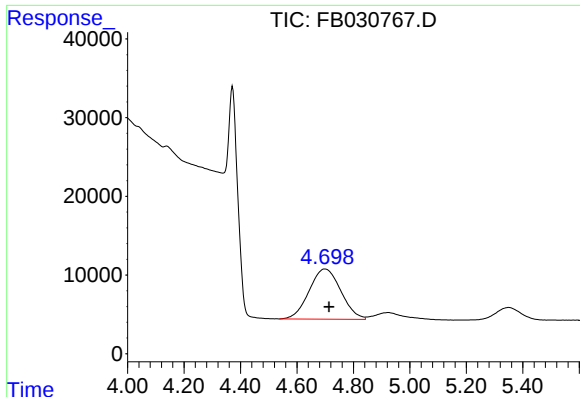

#1 2-Methylpentane


R.T.: 4.699 min
Delta R.T.: -0.014 min
Response: 498463
Conc: 28.45 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-052424MSD

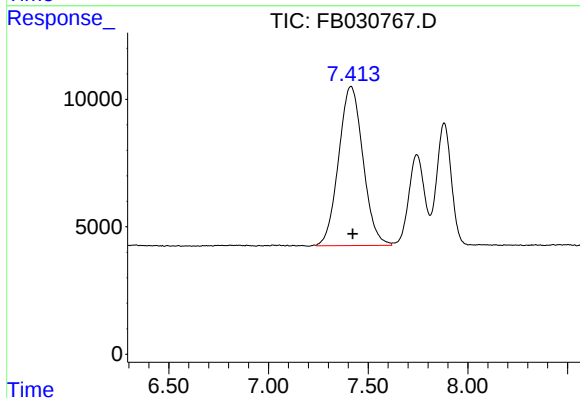


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.007 min
Response: 530503
Conc: 29.52 ng/ml

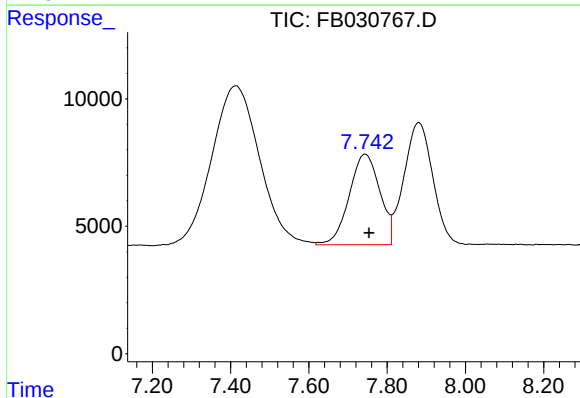


#3 n-Heptane

R.T.: 7.744 min
Delta R.T.: -0.010 min
Response: 193496
Conc: 9.70 ng/ml

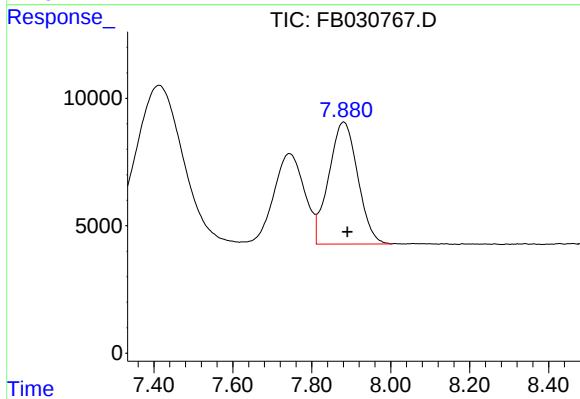

#4 Benzene


R.T.: 7.882 min
Delta R.T.: -0.009 min
Response: 244555
Conc: 10.80 ng/ml

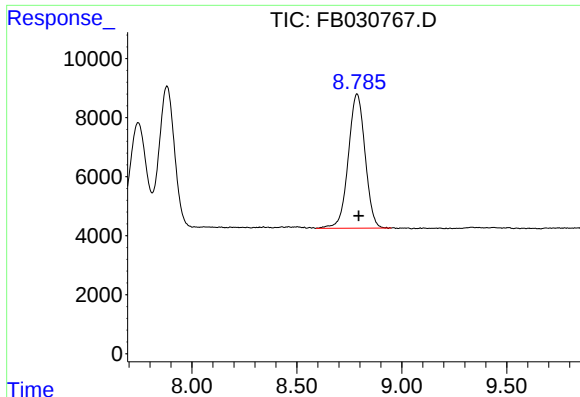

#5 AAA-TFT


R.T.: 8.787 min
Delta R.T.: -0.008 min
Response: 252195
Conc: 18.28 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-052424MSD

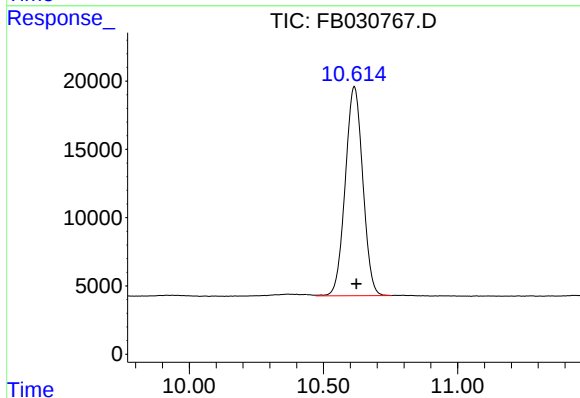


#6 Toluene

R.T.: 10.615 min
Delta R.T.: -0.007 min
Response: 694543
Conc: 31.20 ng/ml

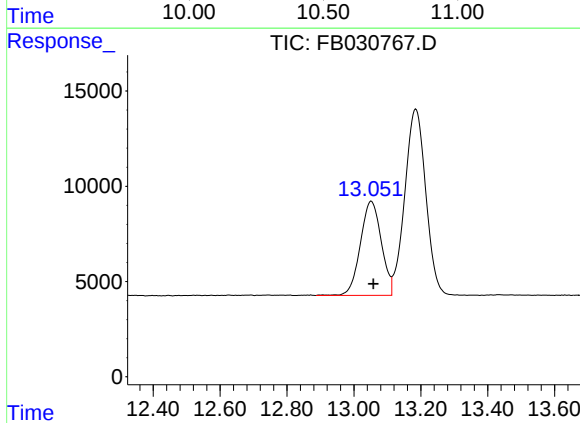


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: -0.007 min
Response: 214602
Conc: 10.40 ng/ml

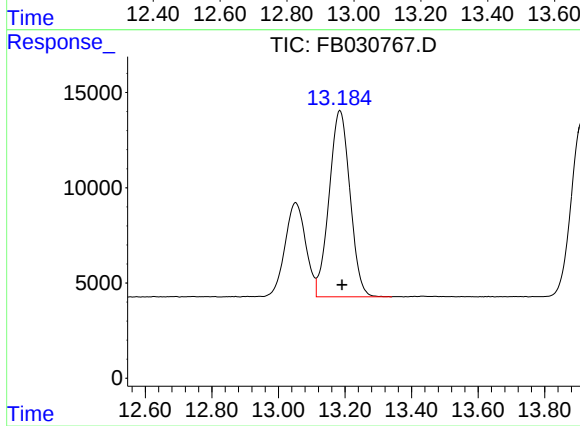

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: -0.007 min
Response: 426937
Conc: 20.50 ng/ml

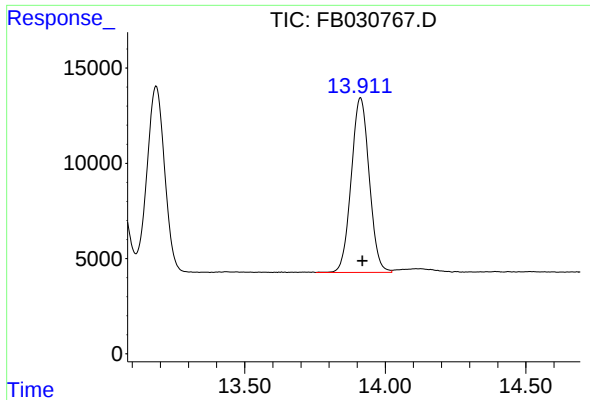

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.006 min
Response: 406966
Conc: 21.32 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-052424MSD

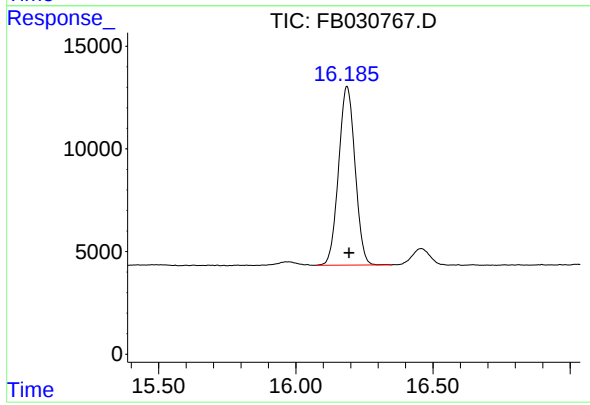

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: -0.007 min
Response: 362990
Conc: 19.19 ng/ml