

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052824\
 Data File : FB030768.D
 Signal(s) : FID2B.CH
 Acq On : 28 May 2024 15:54
 Operator : YP/AJ
 Sample : BSF0528S2
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0528S2

Integration File: Calibration.e
 Quant Time: May 29 06:14:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB050824.M
 Quant Title :
 QLast Update : Wed May 08 14:36:01 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	261022	18.915 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	574179	32.773 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	612906	34.107 ng/ml
3) t n-Heptane	7.747	211834	10.624 ng/ml
4) t Benzene	7.885	247741	10.938 ng/ml
6) t Toluene	10.618	715977	32.165 ng/ml
7) t Ethylbenzene	13.054	222571	10.785 ng/ml
8) t m-Xylene	13.187	444214	21.325 ng/ml
9) t O-Xylene	13.914	431065	22.582 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	418180	22.110 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB052824\
Data File : FB030768.D
Signal(s) : FID2B.CH
Acq On : 28 May 2024 15:54
Operator : YP/AJ
Sample : BSF0528S2
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0528S2

Integration File: Calibration.e
Quant Time: May 29 06:14:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB050824.M
Quant Title :
QLast Update : Wed May 08 14:36:01 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

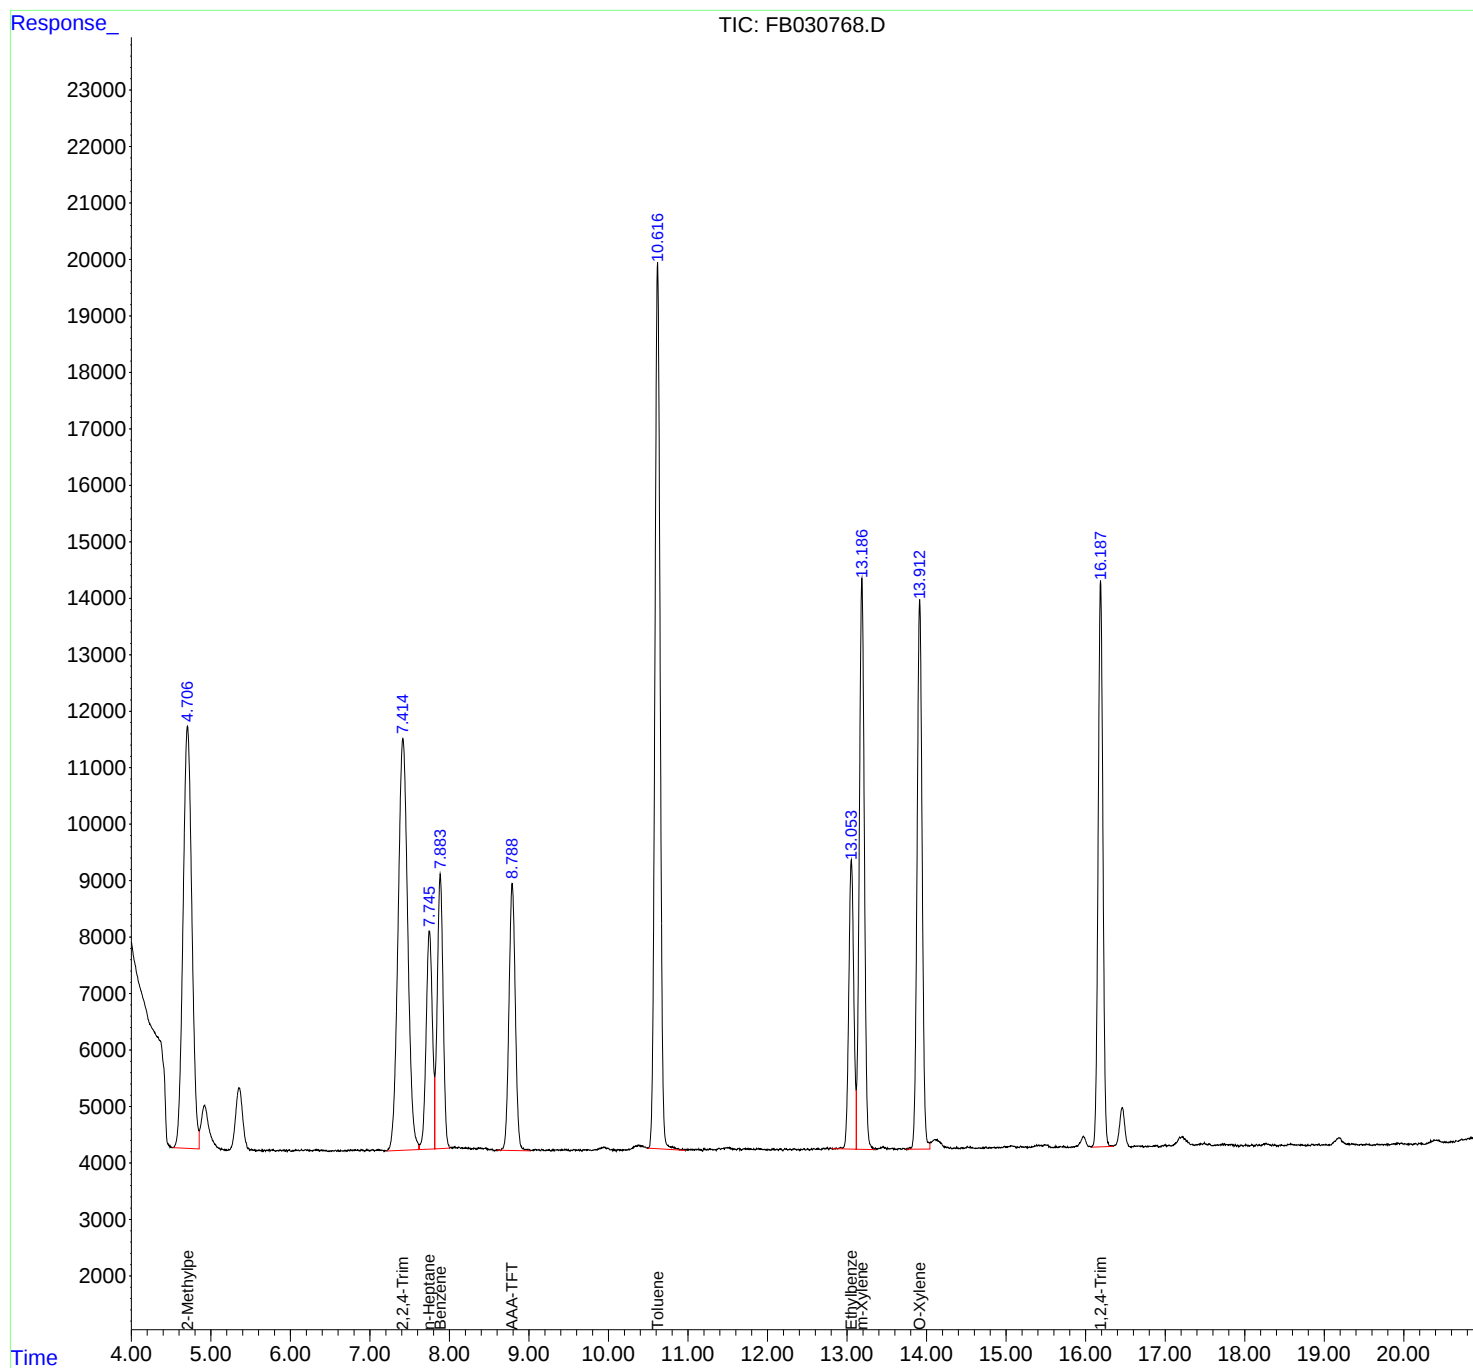


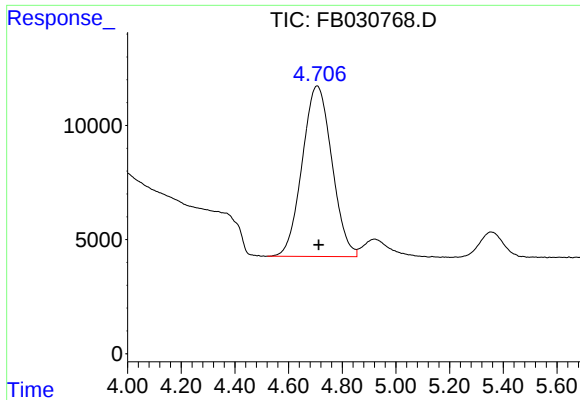

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: -0.006 min
Response: 574179
Conc: 32.77 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0528S2

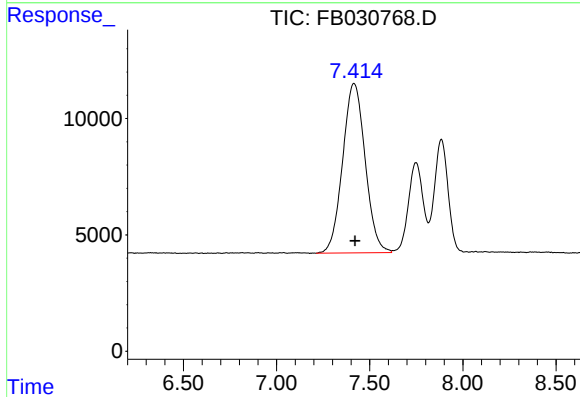


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.007 min
Response: 612906
Conc: 34.11 ng/ml

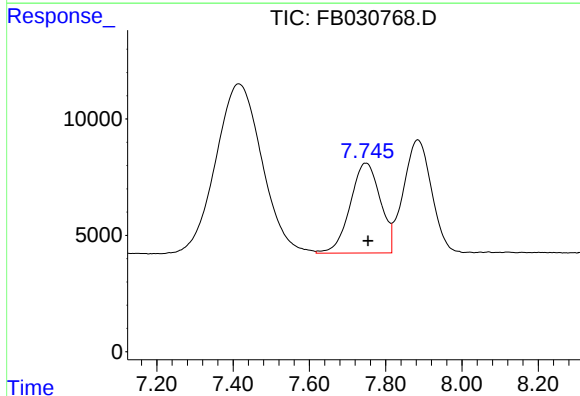


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.006 min
Response: 211834
Conc: 10.62 ng/ml

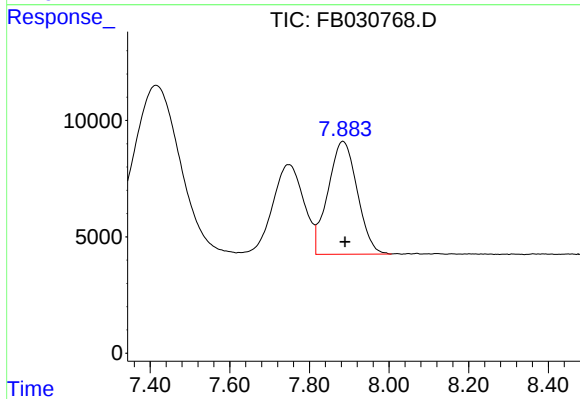

#4 Benzene


R.T.: 7.885 min
Delta R.T.: -0.005 min
Response: 247741
Conc: 10.94 ng/ml

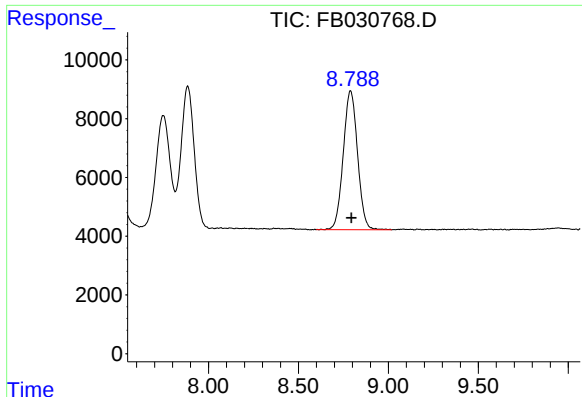

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: -0.005 min
Response: 261022
Conc: 18.91 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0528S2

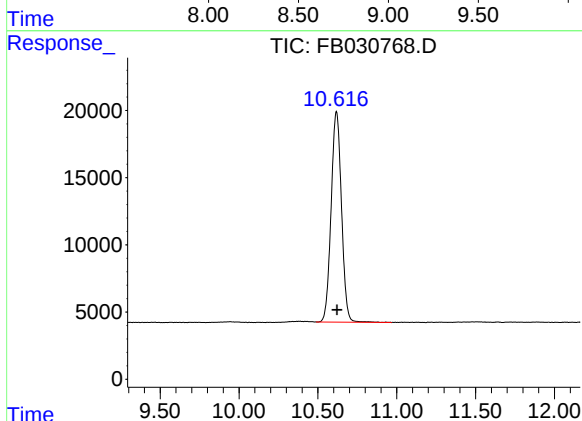


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.005 min
Response: 715977
Conc: 32.17 ng/ml

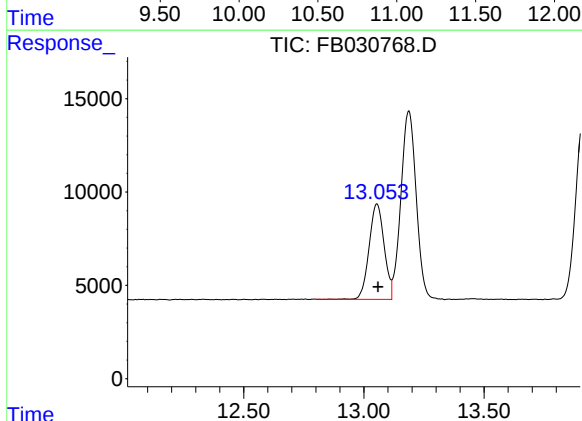


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.004 min
Response: 222571
Conc: 10.79 ng/ml

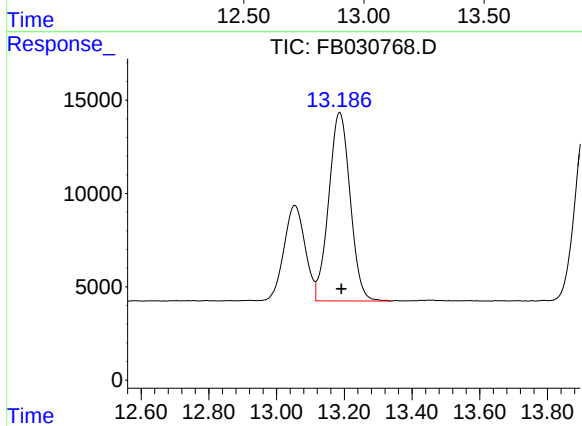

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: -0.005 min
Response: 444214
Conc: 21.33 ng/ml

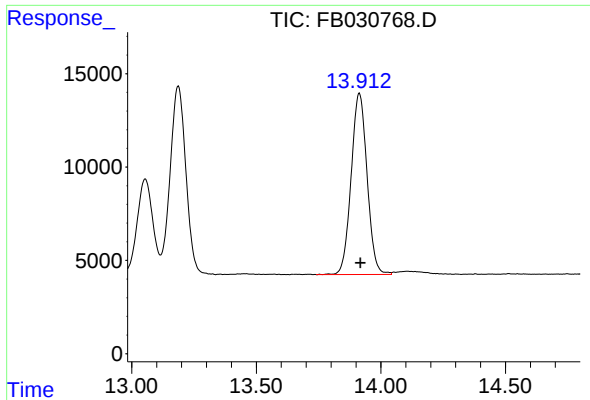

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: -0.005 min
Response: 431065
Conc: 22.58 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0528S2

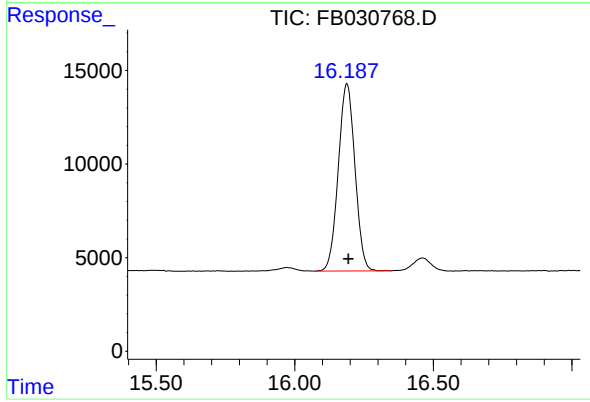

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.005 min
Response: 418180
Conc: 22.11 ng/ml