

Data Path : P:\HPCHEM1\FID_B\Data\FB052918\
Data File : FB015820.D
Signal(s) : FID2B.CH
Acq On : 29 May 2018 18:35
Operator : MJ/SJ
Sample : J3130-20
Misc : 5.00g/5.00mL DI Water
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 30 04:19:59 2018
Quant Method : P:\HPCHEM1\FID_B\Method\FB052418.M
Quant Title :
QLast Update : Thu May 24 11:17:17 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.120	187611	21.642 ng/ml
Target Compounds			
6) t Toluene	10.967	4758	0.315 ng/ml
8) t m-Xylene	13.549	5987	0.334 ng/ml
9) t O-Xylene	14.335	9896	0.526 ng/ml
10) t 1,2,4-Trimethylbenzene	16.572	6170	0.291 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_B\Data\FB052918\
Data File : FB015820.D
Signal(s) : FID2B.CH
Acq On : 29 May 2018 18:35
Operator : MJ/SJ
Sample : J3130-20
Misc : 5.00g/5.00mL DI Water
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 30 04:19:59 2018
Quant Method : P:\HPCHEM1\FID_B\Method\FB052418.M
Quant Title :
QLast Update : Thu May 24 11:17:17 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

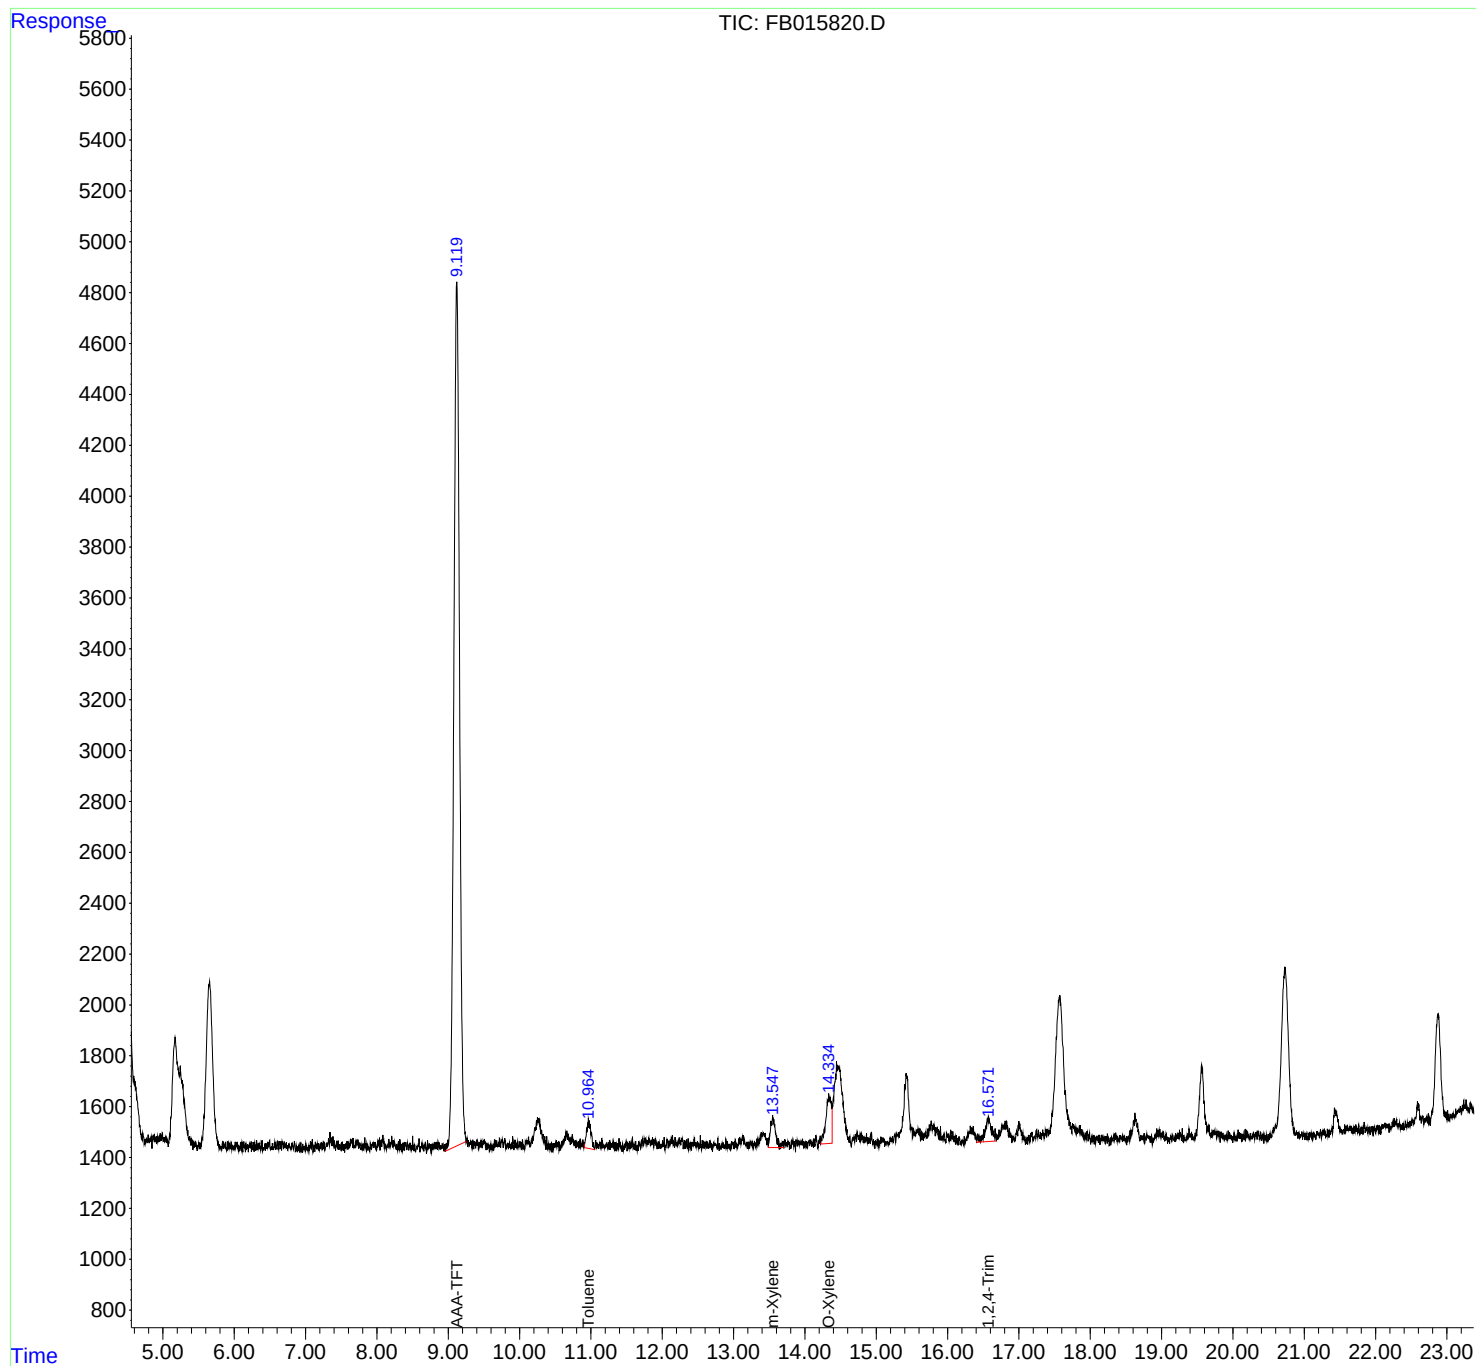


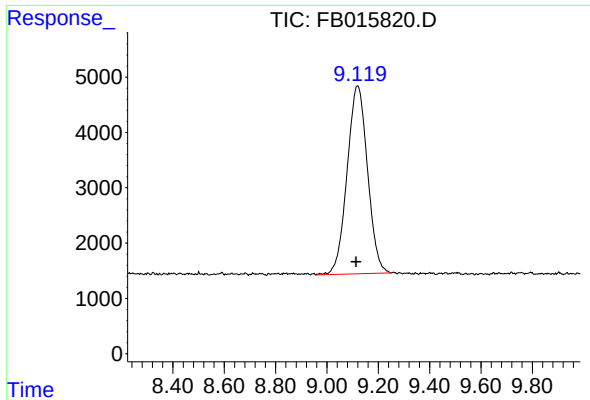

#5 AAA-TFT


R.T.: 9.120 min
Delta R.T.: 0.007 min
Response: 187611
Conc: 21.64 ng/ml

Instrument :
FID_B
ClientSampleId :

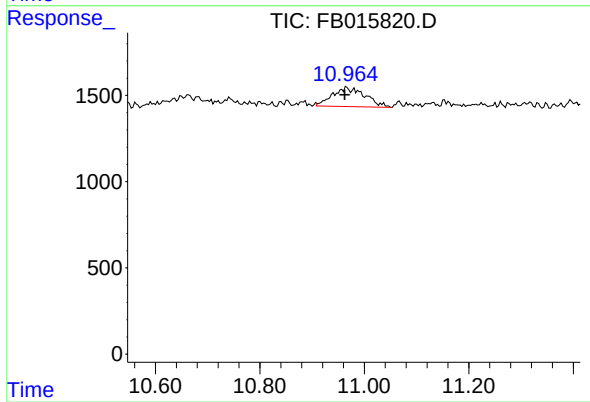


#6 Toluene

R.T.: 10.967 min
Delta R.T.: 0.005 min
Response: 4758
Conc: 0.32 ng/ml

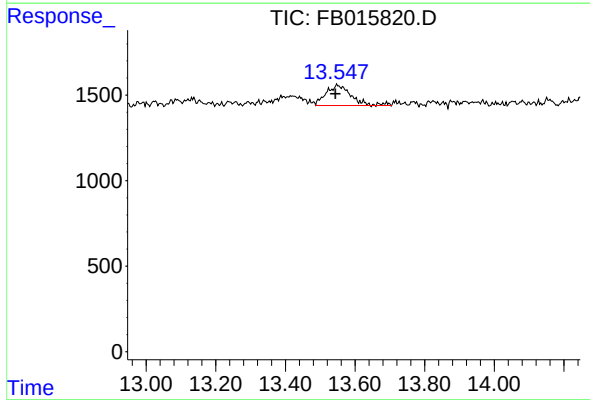


#8 m-Xylene

R.T.: 13.549 min
Delta R.T.: 0.006 min
Response: 5987
Conc: 0.33 ng/ml

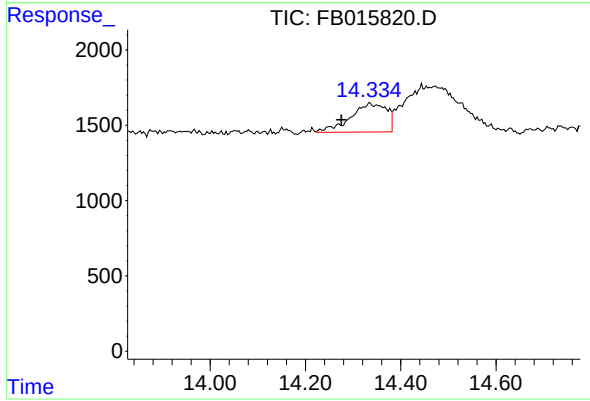

#9 O-Xylene

R.T.: 14.335 min
Delta R.T.: 0.060 min
Response: 9896
Conc: 0.53 ng/ml

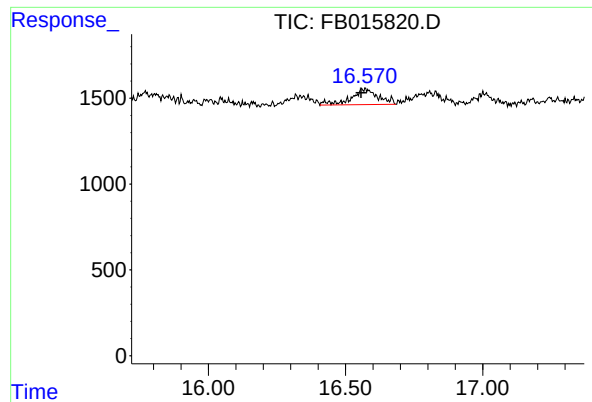

#10 1,2,4-Trimethylbenzene

R.T.: 16.572 min
Delta R.T.: 0.015 min
Response: 6170
Conc: 0.29 ng/ml

Instrument :
FID_B
ClientSampleId :