

Data Path : P:\HPCHEM1\FID_B\Data\FB052918\
Data File : FB015821.D
Signal(s) : FID2B.CH
Acq On : 29 May 2018 19:06
Operator : MJ/SJ
Sample : J3138-01
Misc : 5.01g/5.00mL DI Water
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 30 04:20:10 2018
Quant Method : P:\HPCHEM1\FID_B\Method\FB052418.M
Quant Title :
QLast Update : Thu May 24 11:17:17 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.121	116437	13.432 ng/ml
Target Compounds			
7) t Ethylbenzene	13.413	13273	0.805 ng/ml
8) t m-Xylene	13.543	8360	0.467 ng/ml
9) t O-Xylene	14.292	11986	0.637 ng/ml
10) t 1,2,4-Trimethylbenzene	16.567	9808	0.463 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_B\Data\FB052918\
Data File : FB015821.D
Signal(s) : FID2B.CH
Acq On : 29 May 2018 19:06
Operator : MJ/SJ
Sample : J3138-01
Misc : 5.01g/5.00mL DI Water
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 30 04:20:10 2018
Quant Method : P:\HPCHEM1\FID_B\Method\FB052418.M
Quant Title :
QLast Update : Thu May 24 11:17:17 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

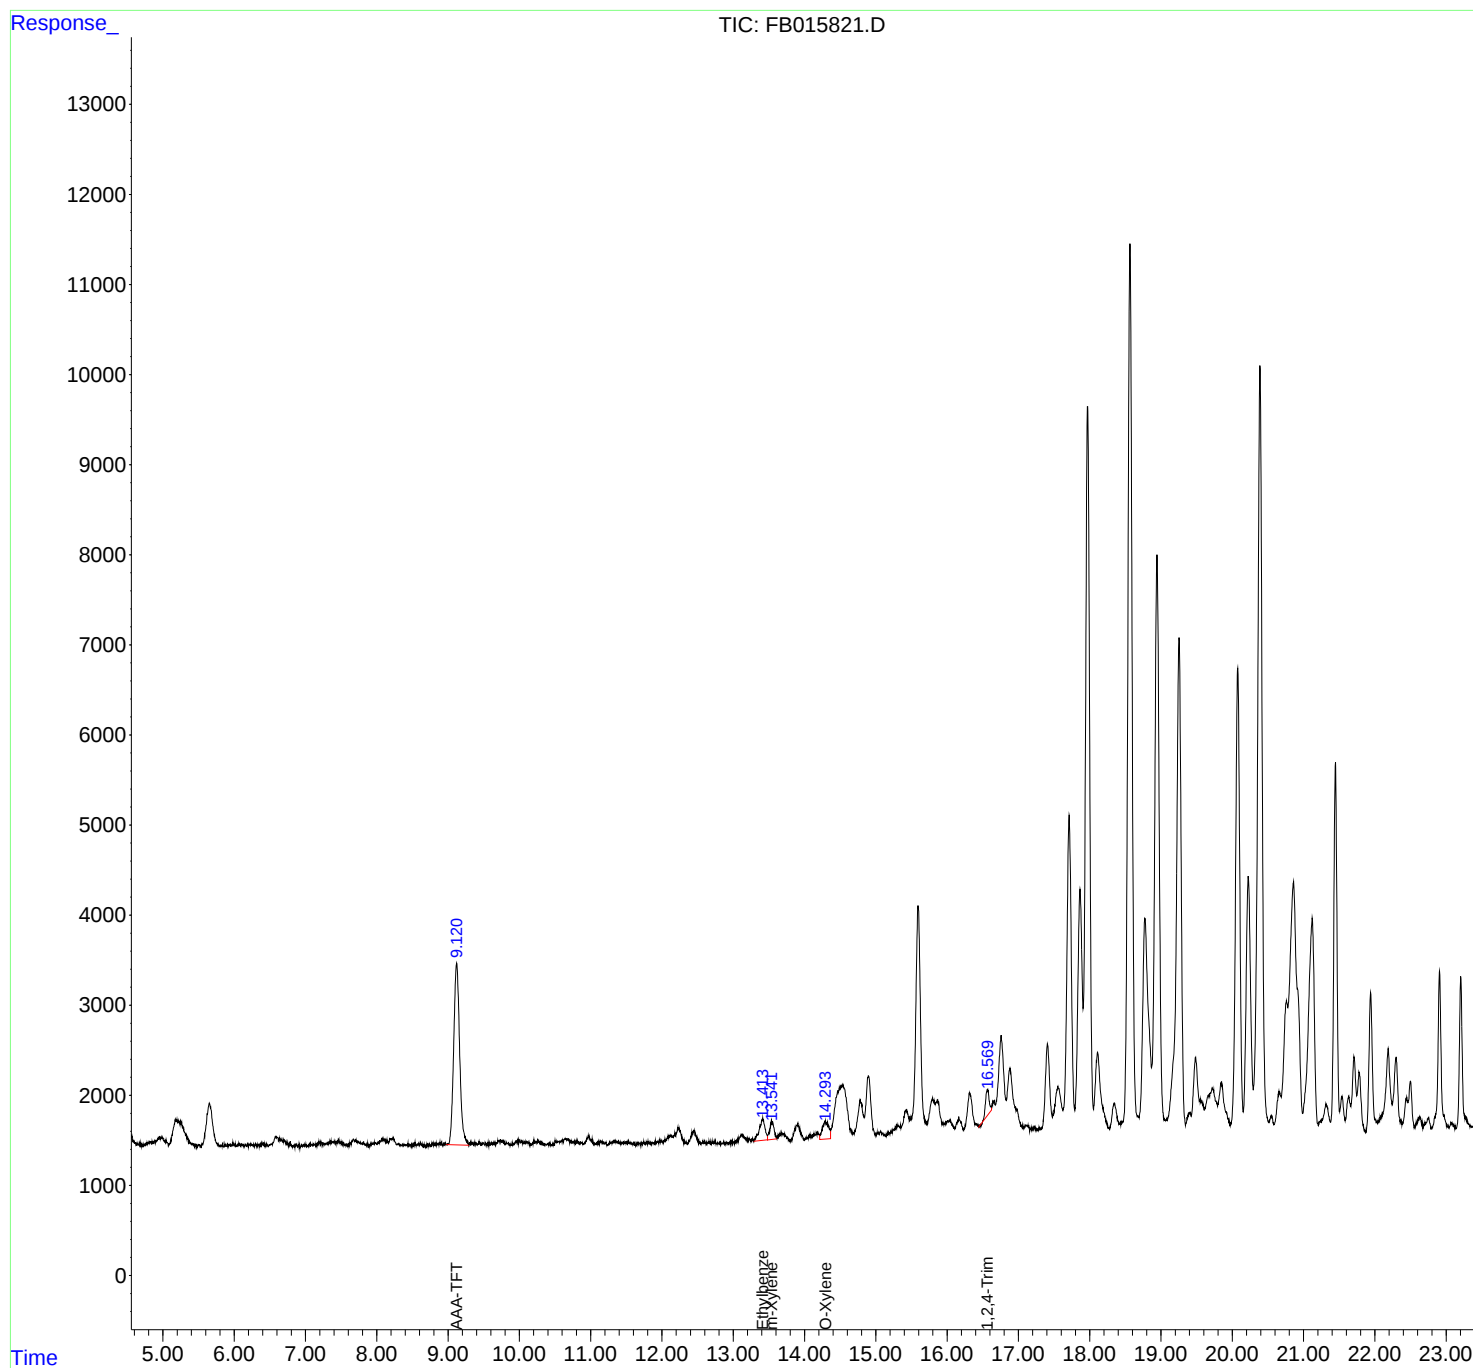


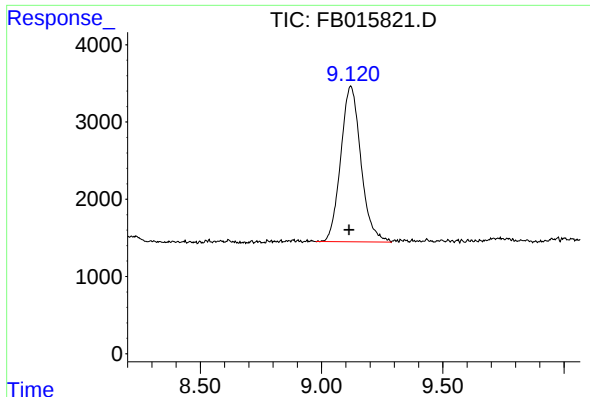

#5 AAA-TFT


R.T.: 9.121 min
Delta R.T.: 0.008 min
Response: 116437
Conc: 13.43 ng/ml

Instrument :
FID_B
ClientSampleId :

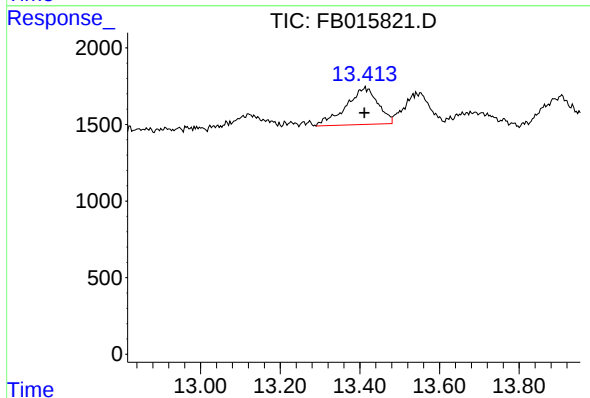


#7 Ethylbenzene

R.T.: 13.413 min
Delta R.T.: 0.002 min
Response: 13273
Conc: 0.80 ng/ml

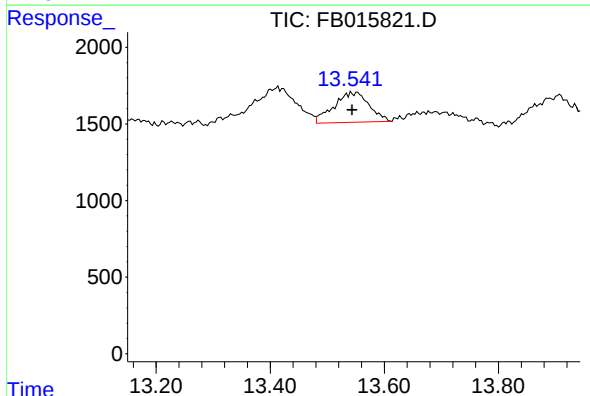


#8 m-Xylene

R.T.: 13.543 min
Delta R.T.: 0.000 min
Response: 8360
Conc: 0.47 ng/ml

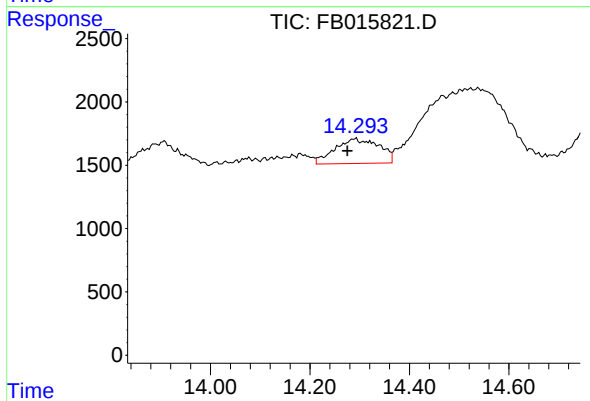

#9 O-Xylene

R.T.: 14.292 min
Delta R.T.: 0.017 min
Response: 11986
Conc: 0.64 ng/ml

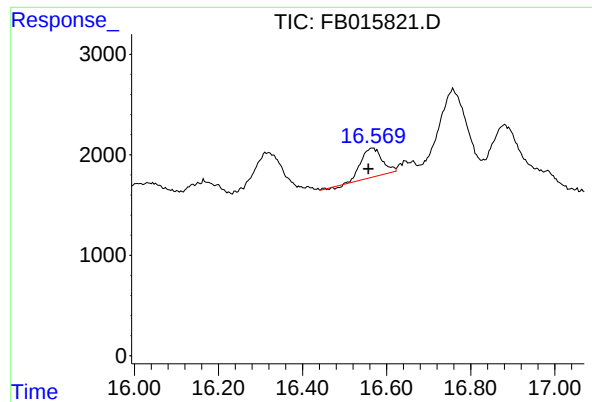

#10 1,2,4-Trimethylbenzene

R.T.: 16.567 min
Delta R.T.: 0.010 min
Response: 9808
Conc: 0.46 ng/ml

Instrument :
FID_B
ClientSampleId :