

Data Path : P:\HPCHEM1\FID\_B\Data\FB052918\  
Data File : FB015824.D  
Signal(s) : FID2B.CH  
Acq On : 29 May 2018 21:10  
Operator : MJ/SJ  
Sample : J3166-01  
Misc : 5.01g/5.00mL DI Water  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: May 30 11:09:35 2018  
Quant Method : P:\HPCHEM1\FID\_B\Method\FB052418.M  
Quant Title :  
QLast Update : Thu May 24 11:17:17 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| 5) s AAA-TFT                | 9.119  | 177407   | 20.465 ng/ml |
| Target Compounds            |        |          |              |
| 6) t Toluene                | 10.975 | 3328     | 0.221 ng/ml  |
| 8) t m-Xylene               | 13.554 | 5388     | 0.301 ng/ml  |
| 9) t O-Xylene               | 14.335 | 7726     | 0.411 ng/ml  |
| -----                       |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID\_B\Data\FB052918\  
Data File : FB015824.D  
Signal(s) : FID2B.CH  
Acq On : 29 May 2018 21:10  
Operator : MJ/SJ  
Sample : J3166-01  
Misc : 5.01g/5.00mL DI Water  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: May 30 11:09:35 2018  
Quant Method : P:\HPCHEM1\FID\_B\Method\FB052418.M  
Quant Title :  
QLast Update : Thu May 24 11:17:17 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

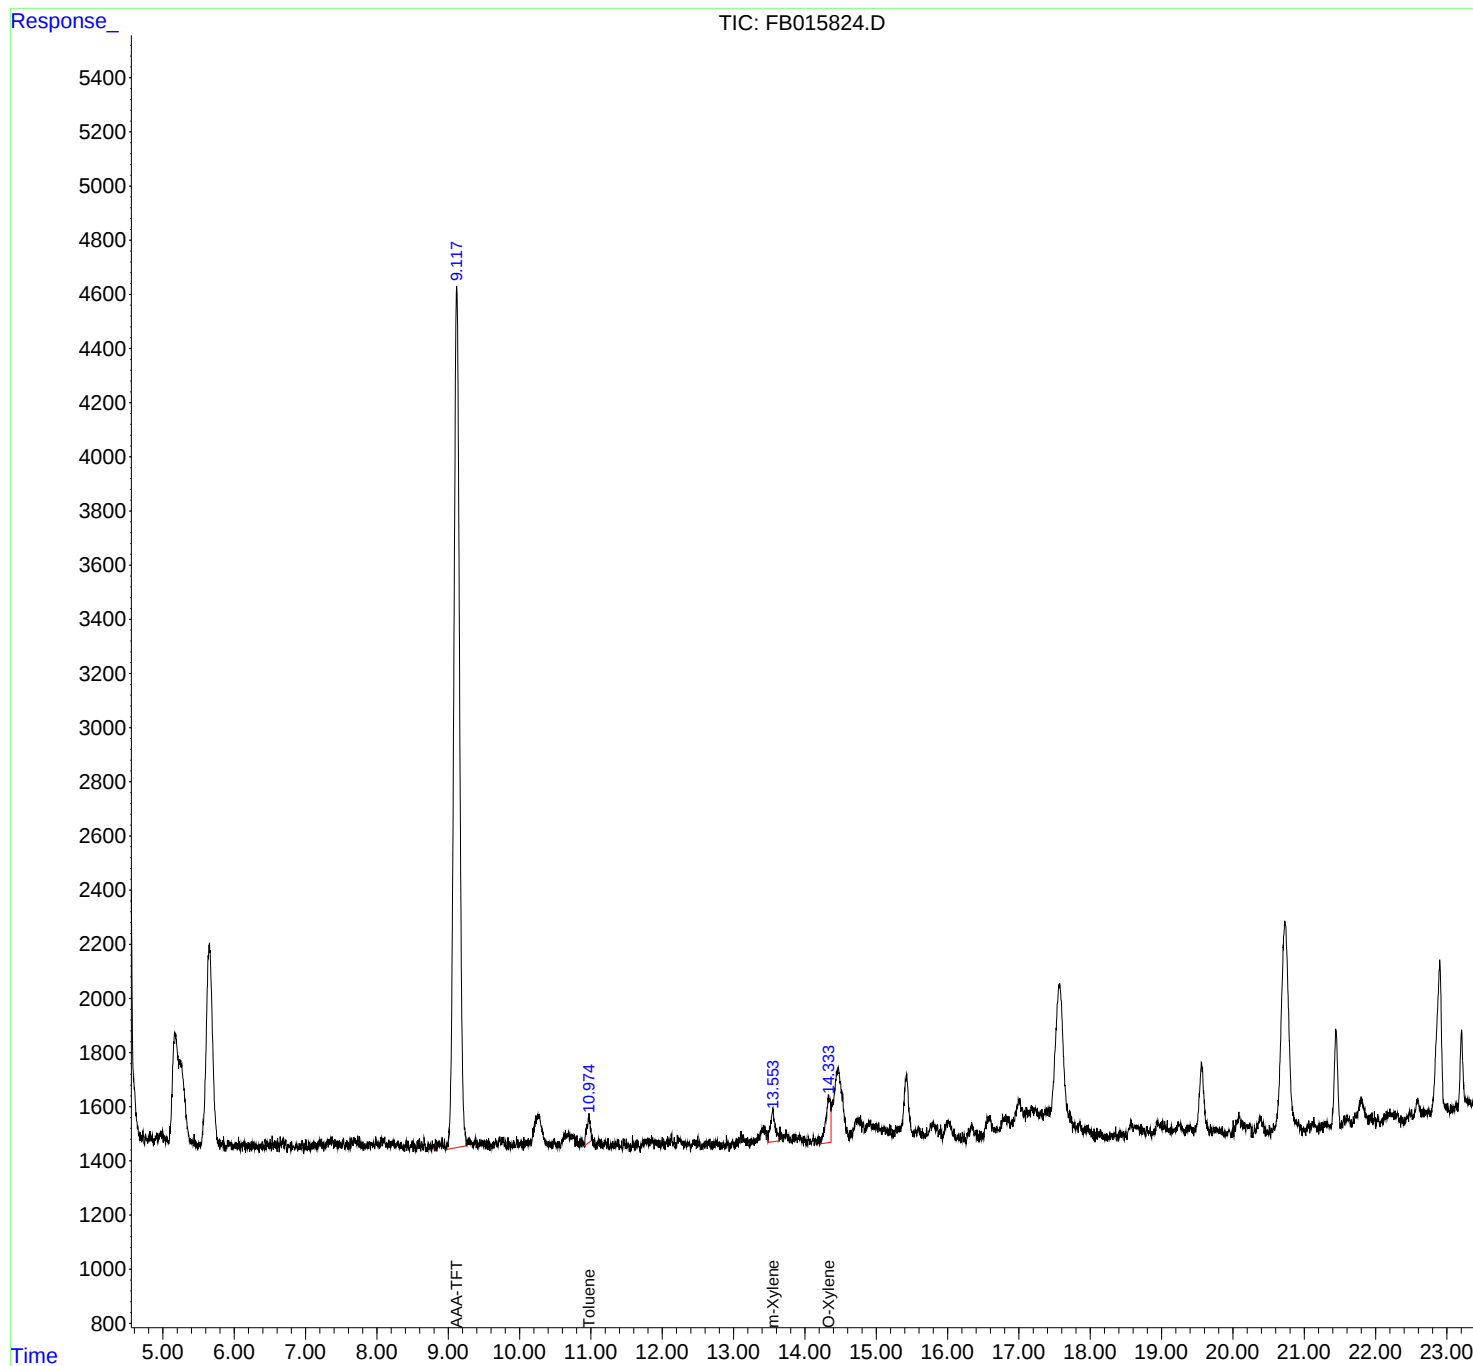


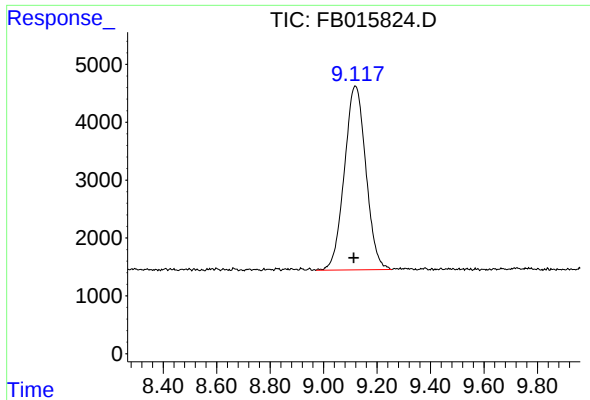

#5 AAA-TFT


R.T.: 9.119 min  
Delta R.T.: 0.006 min  
Response: 177407  
Conc: 20.46 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

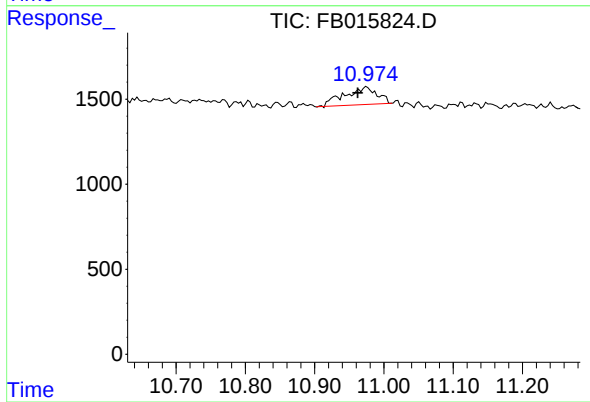


#6 Toluene

R.T.: 10.975 min  
Delta R.T.: 0.013 min  
Response: 3328  
Conc: 0.22 ng/ml

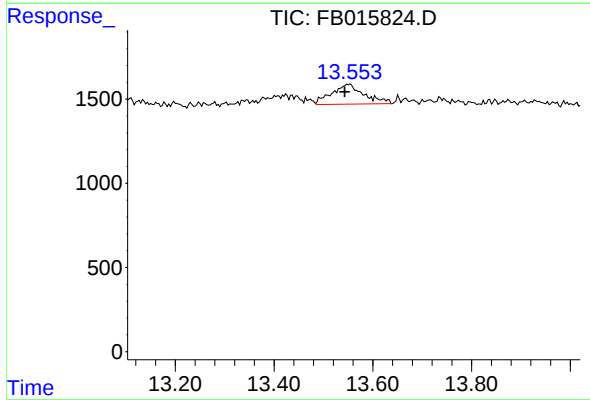

#8 m-Xylene

R.T.: 13.554 min  
Delta R.T.: 0.010 min  
Response: 5388  
Conc: 0.30 ng/ml

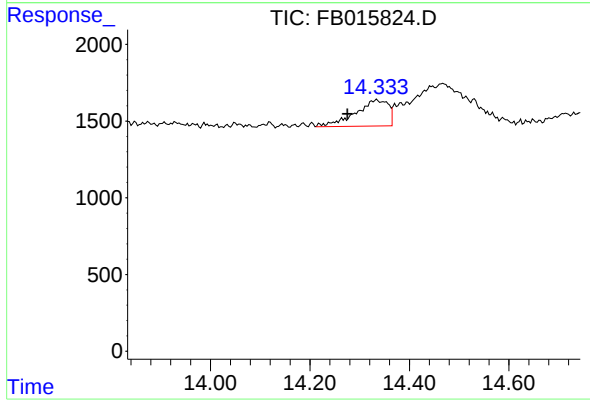

#9 O-Xylene

R.T.: 14.335 min  
Delta R.T.: 0.059 min  
Response: 7726  
Conc: 0.41 ng/ml