

Data Path : P:\HPCHEM1\FID_B\Data\FB052918\
 Data File : FB015831.D
 Signal(s) : FID2B.CH
 Acq On : 30 May 2018 1:17
 Operator : MJ/SJ
 Sample : J3177-01
 Misc : 5.01g/5.00mL DI Water
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: May 30 09:20:57 2018
 Quant Method : P:\HPCHEM1\FID_B\Method\FB052418.M
 Quant Title :
 QLast Update : Thu May 24 11:17:17 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.116	159497	18.399 ng/ml
Target Compounds			
6) t Toluene	10.978	4676	0.310 ng/ml
8) t m-Xylene	13.552	5045	0.282 ng/ml
9) t O-Xylene	14.323	10776	0.573 ng/ml
10) t 1,2,4-Trimethylbenzene	16.561	1183	0.056 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_B\Data\FB052918\
Data File : FB015831.D
Signal(s) : FID2B.CH
Acq On : 30 May 2018 1:17
Operator : MJ/SJ
Sample : J3177-01
Misc : 5.01g/5.00mL DI Water
ALS Vial : 28 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 30 09:20:57 2018
Quant Method : P:\HPCHEM1\FID_B\Method\FB052418.M
Quant Title :
QLast Update : Thu May 24 11:17:17 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

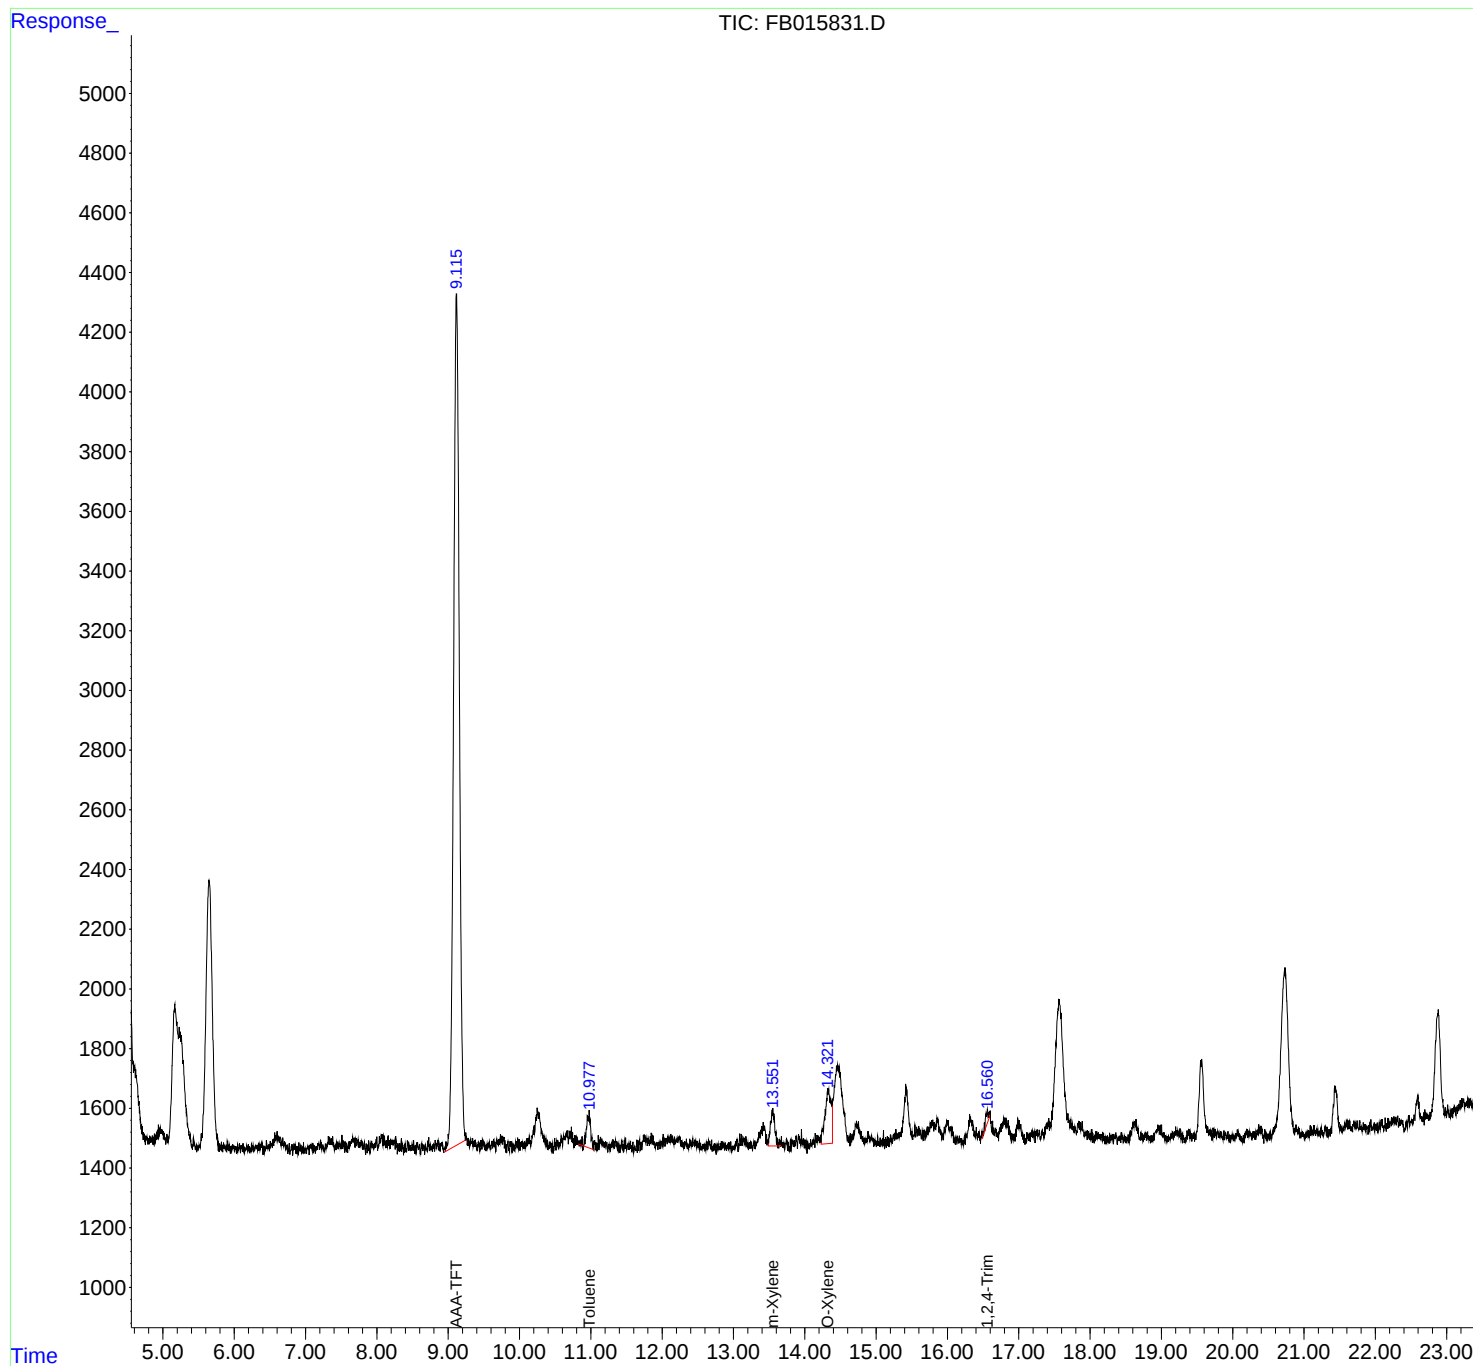


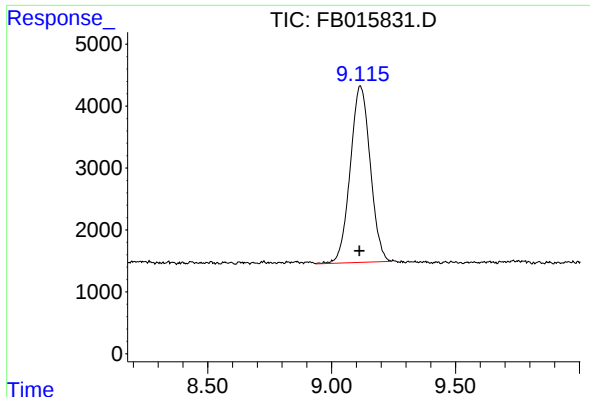

#5 AAA-TFT


R.T.: 9.116 min
Delta R.T.: 0.003 min
Response: 159497
Conc: 18.40 ng/ml

Instrument :
FID_B
ClientSampleId :

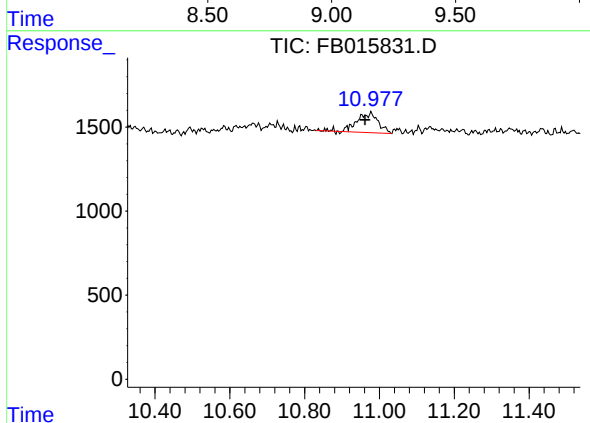


#6 Toluene

R.T.: 10.978 min
Delta R.T.: 0.016 min
Response: 4676
Conc: 0.31 ng/ml

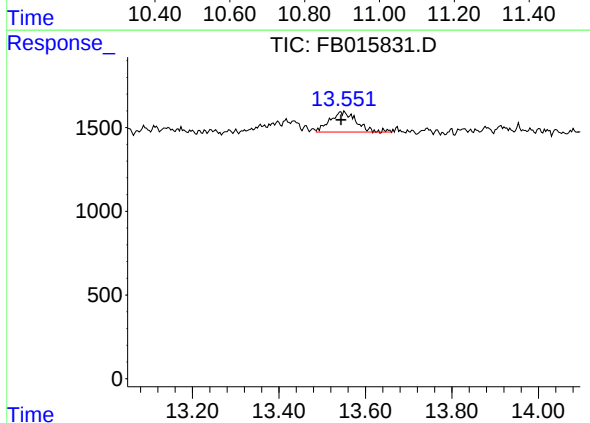


#8 m-Xylene

R.T.: 13.552 min
Delta R.T.: 0.009 min
Response: 5045
Conc: 0.28 ng/ml

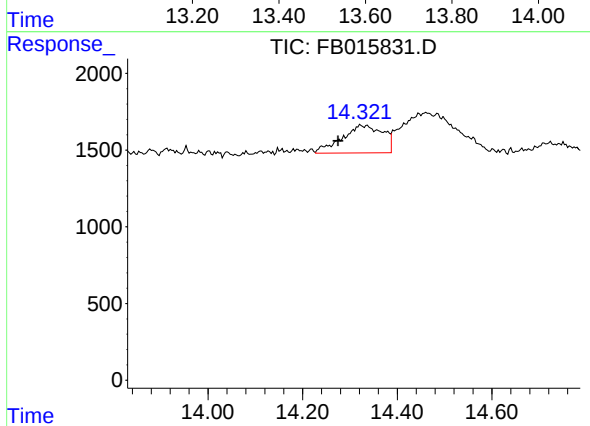

#9 O-Xylene

R.T.: 14.323 min
Delta R.T.: 0.047 min
Response: 10776
Conc: 0.57 ng/ml

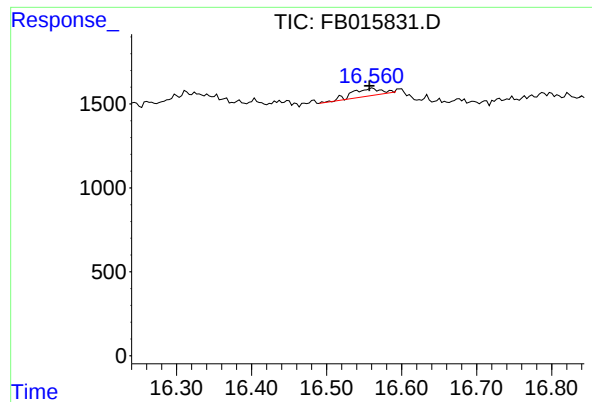

#10 1,2,4-Trimethylbenzene

R.T.: 16.561 min
Delta R.T.: 0.004 min
Response: 1183
Conc: 0.06 ng/ml

Instrument :
FID_B
ClientSampleId :