

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB053019\
 Data File : FB021237.D
 Signal(s) : FID2B.CH
 Acq On : 30 May 2019 9:47
 Operator : MJ/SJ
 Sample : BSF0530S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 31 01:00:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.994	329310	22.335 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.856	1258799	33.484 ng/ml
2) t	2,2,4-Trimethylpentane	7.610	1176126	34.440 ng/ml
3) t	n-Heptane	7.950	371291	11.389 ng/ml
4) t	Benzene	8.086	395924	11.471 ng/ml
6) t	Toluene	10.839	783608	33.060 ng/ml
7) t	Ethylbenzene	13.289	245374	10.501 ng/ml
8) t	m-Xylene	13.423	524317	21.006 ng/ml
9) t	O-Xylene	14.153	543291	20.826 ng/ml
10) t	1,2,4-Trimethylbenzene	16.438	547785	20.397 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB053019\
Data File : FB021237.D
Signal(s) : FID2B.CH
Acq On : 30 May 2019 9:47
Operator : MJ/SJ
Sample : BSF0530S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 31 01:00:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

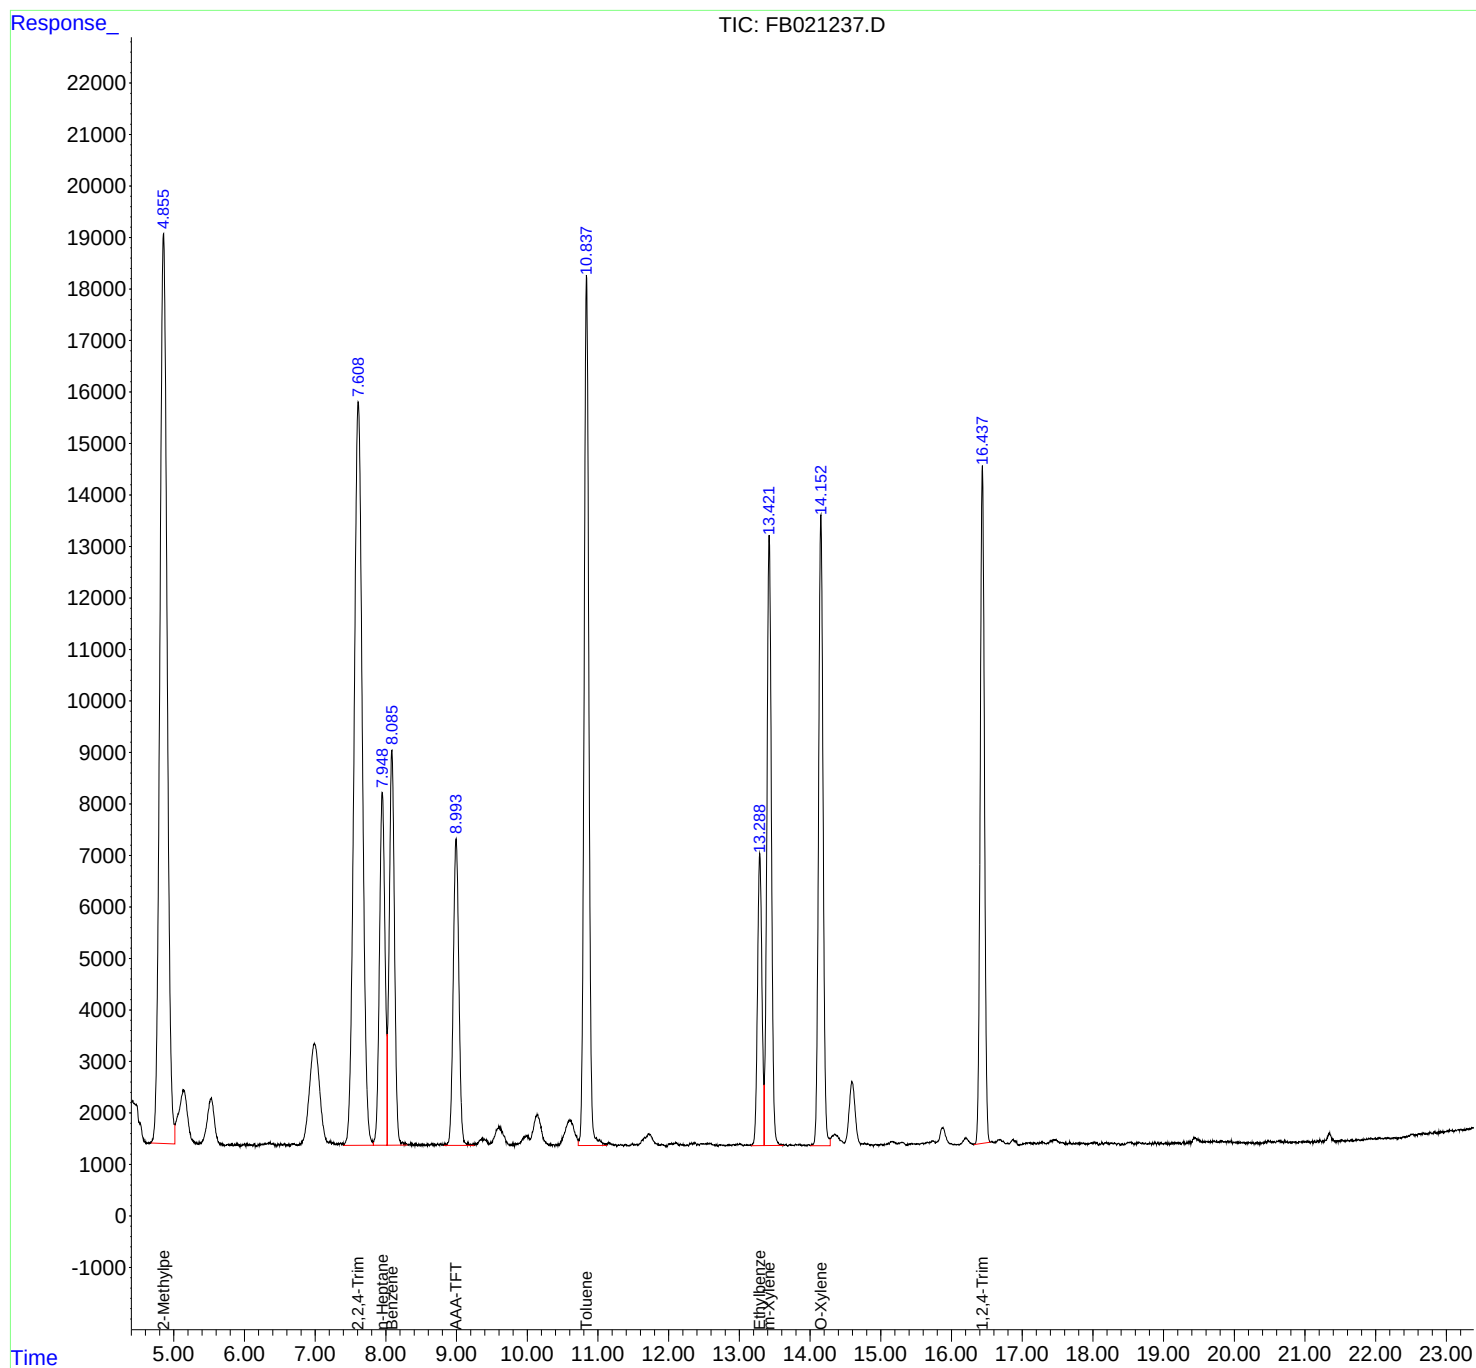

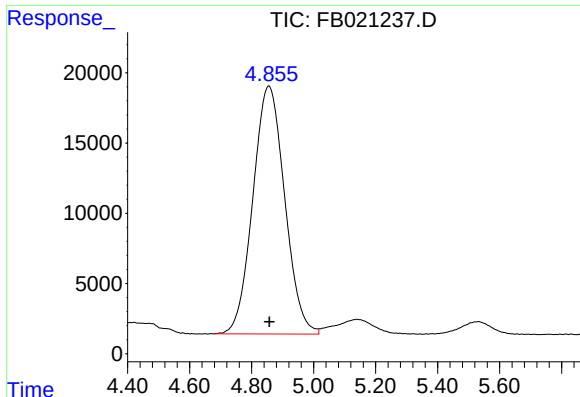


#1 2-Methylpentane

R.T.: 4.856 min
Delta R.T.: -0.002 min
Response: 1258799
Conc: 33.48 ng/ml

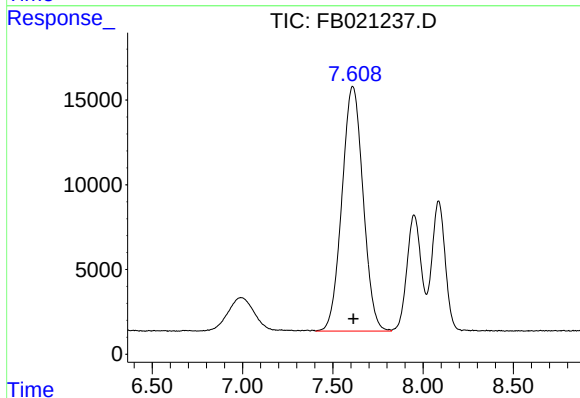


#2 2,2,4-Trimethylpentane

R.T.: 7.610 min
Delta R.T.: -0.004 min
Response: 1176126
Conc: 34.44 ng/ml

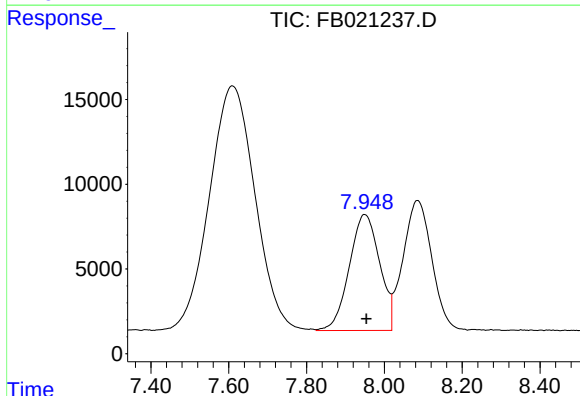


#3 n-Heptane

R.T.: 7.950 min
Delta R.T.: -0.004 min
Response: 371291
Conc: 11.39 ng/ml

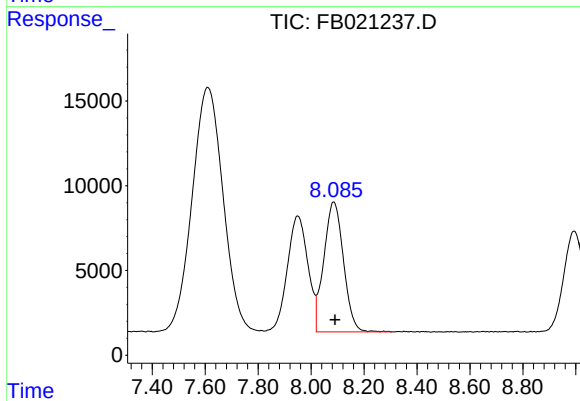


#4 Benzene

R.T.: 8.086 min
Delta R.T.: -0.004 min
Response: 395924
Conc: 11.47 ng/ml

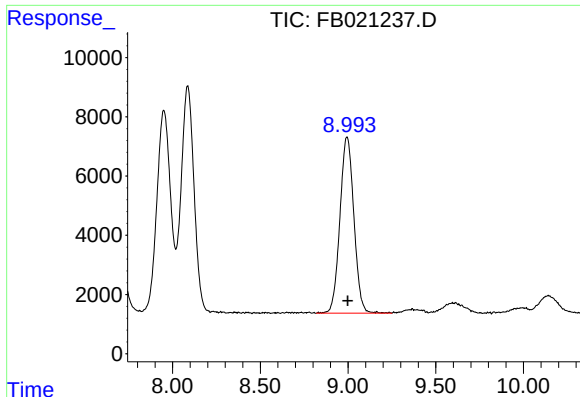


#5 AAA-TFT

R.T.: 8.994 min
Delta R.T.: -0.004 min
Response: 329310
Conc: 22.33 ng/ml

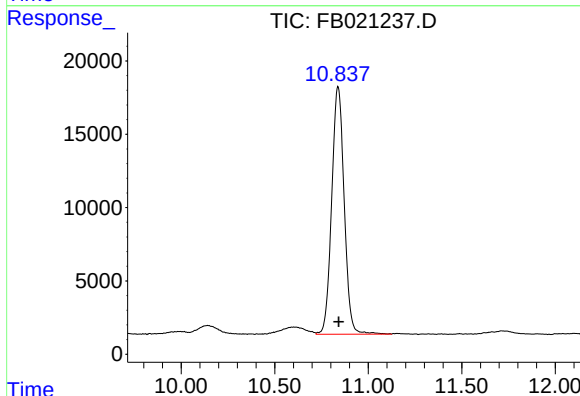


#6 Toluene

R.T.: 10.839 min
Delta R.T.: -0.004 min
Response: 783608
Conc: 33.06 ng/ml

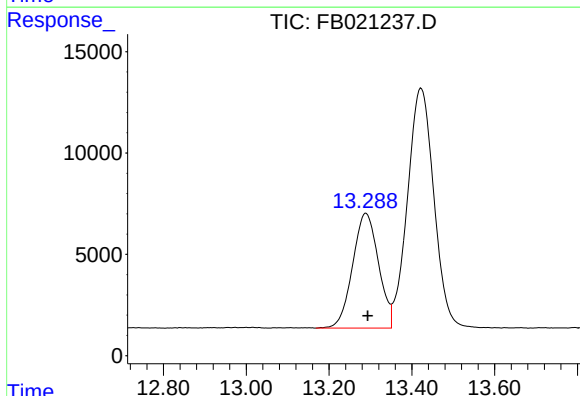


#7 Ethylbenzene

R.T.: 13.289 min
Delta R.T.: -0.004 min
Response: 245374
Conc: 10.50 ng/ml

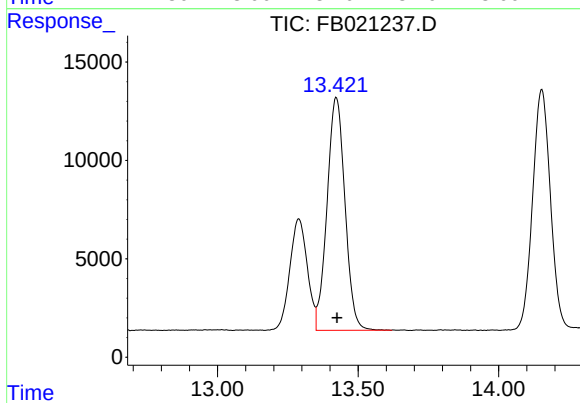

#8 m-Xylene

R.T.: 13.423 min
Delta R.T.: -0.003 min
Response: 524317
Conc: 21.01 ng/ml

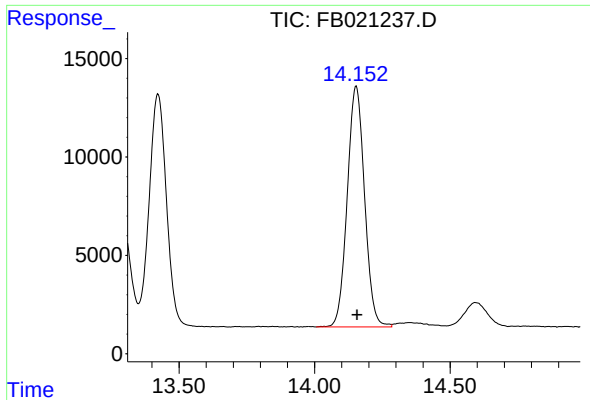


#9 O-Xylene

R.T.: 14.153 min

Delta R.T.: -0.003 min

Response: 543291

Conc: 20.83 ng/ml

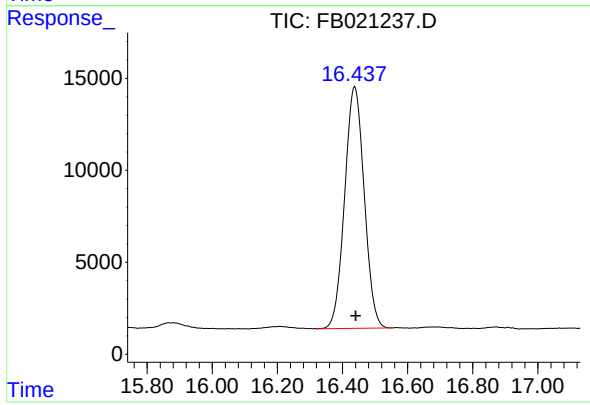

#10 1,2,4-Trimethylbenzene

R.T.: 16.438 min

Delta R.T.: -0.003 min

Response: 547785

Conc: 20.40 ng/ml