

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB053023\
 Data File : FB029896.D
 Signal(s) : FID2B.CH
 Acq On : 30 May 2023 20:21
 Operator : YP/AJ
 Sample : BSF0530S3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: May 31 03:34:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051123.M
 Quant Title :
 QLast Update : Thu May 11 11:33:20 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.786	253215	20.793 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	501936	29.295 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	528948	30.991 ng/ml
3) t n-Heptane	7.745	173451	9.767 ng/ml
4) t Benzene	7.881	215042	10.265 ng/ml
6) t Toluene	10.614	618165	30.359 ng/ml
7) t Ethylbenzene	13.050	197843	10.323 ng/ml
8) t m-Xylene	13.182	393053	20.400 ng/ml
9) t O-Xylene	13.909	380184	20.438 ng/ml
10) t 1,2,4-Trimethylbenzene	16.184	380643	20.463 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB053023\
Data File : FB029896.D
Signal(s) : FID2B.CH
Acq On : 30 May 2023 20:21
Operator : YP/AJ
Sample : BSF0530S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 31 03:34:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051123.M
Quant Title :
QLast Update : Thu May 11 11:33:20 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

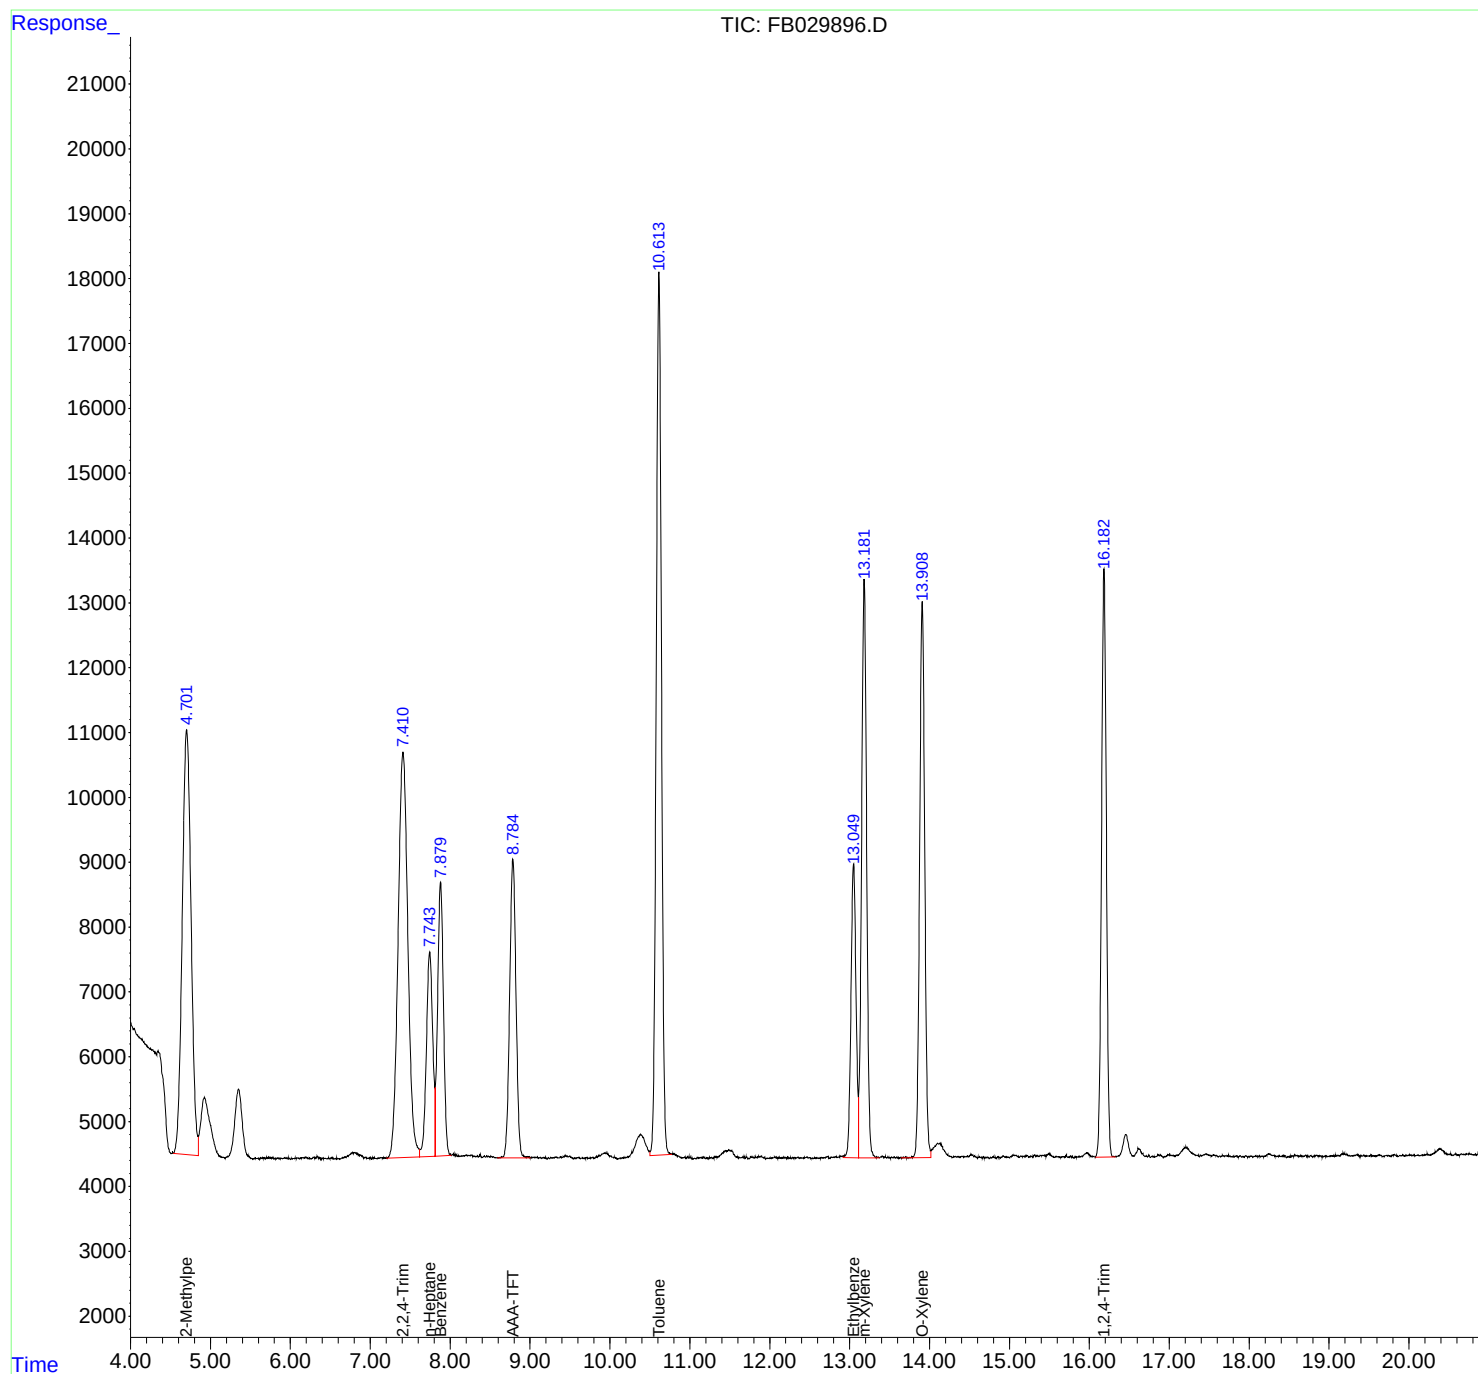


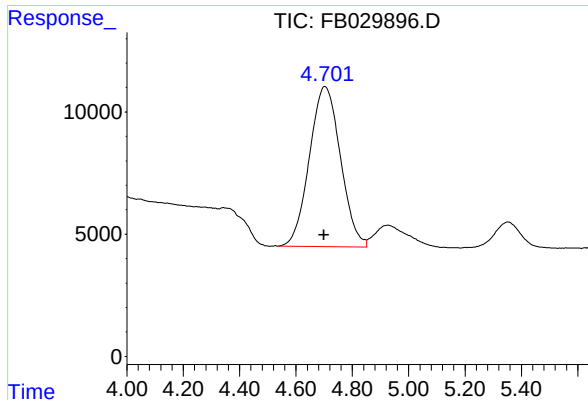

#1 2-Methylpentane


R.T.: 4.702 min
Delta R.T.: 0.003 min
Response: 501936
Conc: 29.29 ng/ml

Instrument :
FID_B
ClientSampleId :

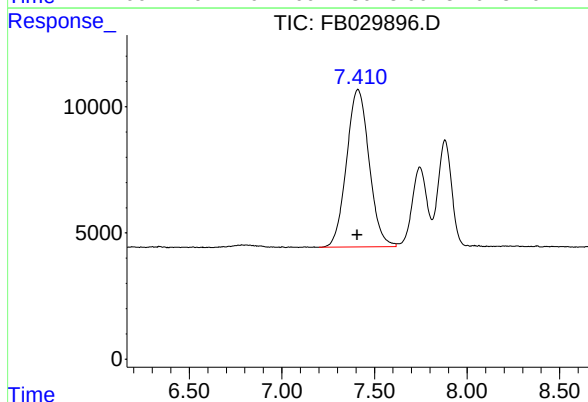


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: 0.005 min
Response: 528948
Conc: 30.99 ng/ml

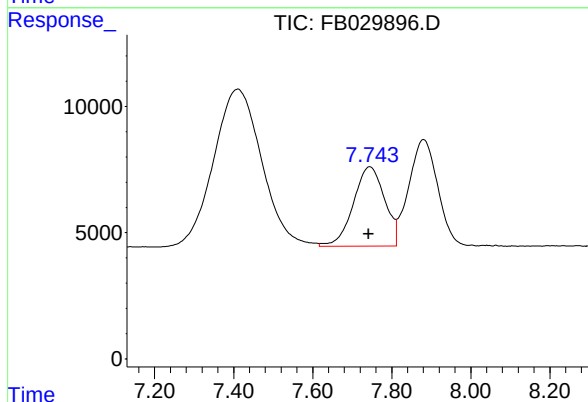


#3 n-Heptane

R.T.: 7.745 min
Delta R.T.: 0.003 min
Response: 173451
Conc: 9.77 ng/ml

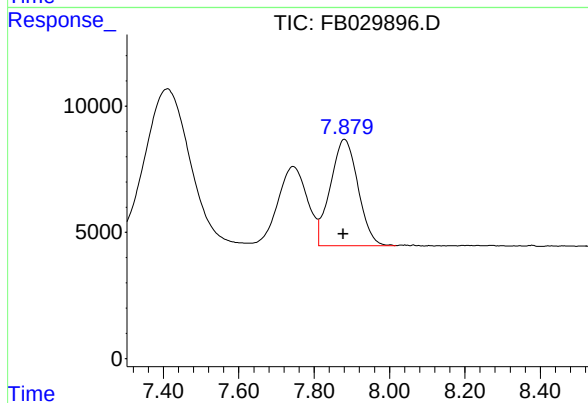

#4 Benzene


R.T.: 7.881 min
Delta R.T.: 0.003 min
Response: 215042
Conc: 10.27 ng/ml

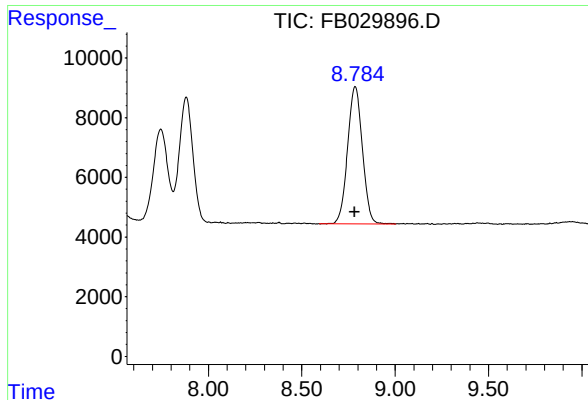

#5 AAA-TFT


R.T.: 8.786 min
Delta R.T.: 0.003 min
Response: 253215
Conc: 20.79 ng/ml

Instrument :
FID_B
ClientSampleId :

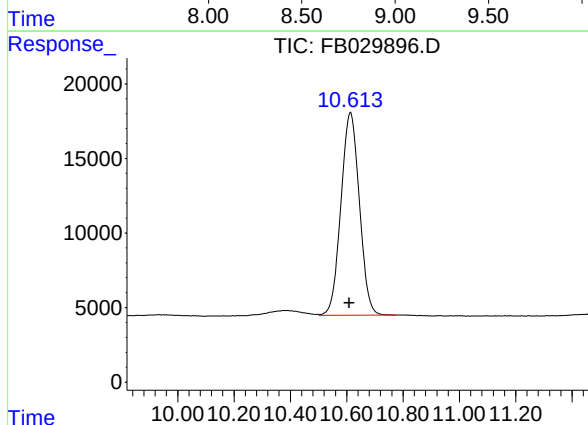


#6 Toluene

R.T.: 10.614 min
Delta R.T.: 0.004 min
Response: 618165
Conc: 30.36 ng/ml

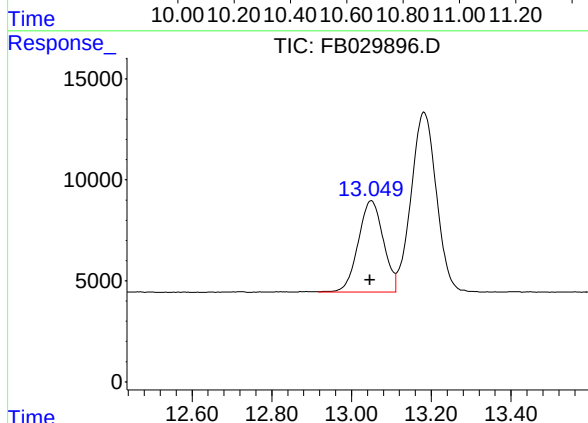


#7 Ethylbenzene

R.T.: 13.050 min
Delta R.T.: 0.004 min
Response: 197843
Conc: 10.32 ng/ml

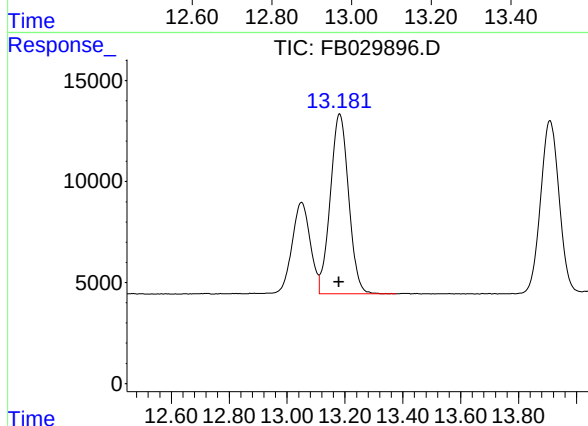

#8 m-Xylene


R.T.: 13.182 min
Delta R.T.: 0.003 min
Response: 393053
Conc: 20.40 ng/ml

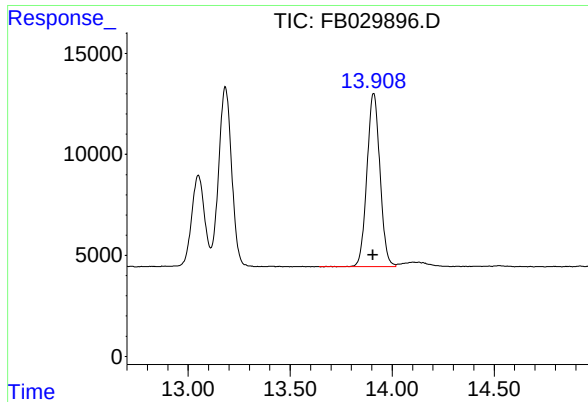

#9 O-Xylene

R.T.: 13.909 min
Delta R.T.: 0.003 min
Response: 380184
Conc: 20.44 ng/ml

Instrument :
FID_B
ClientSampleId :

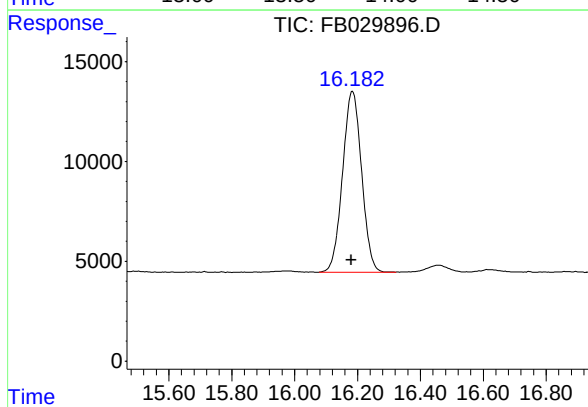

#10 1,2,4-Trimethylbenzene

R.T.: 16.184 min
Delta R.T.: 0.003 min
Response: 380643
Conc: 20.46 ng/ml