

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB053023\
 Data File : FB029882.D
 Signal(s) : FID2B.CH
 Acq On : 30 May 2023 10:59
 Operator : YP/AJ
 Sample : BSF0530S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0530S1

Integration File: Calibration.e
 Quant Time: May 31 03:33:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051123.M
 Quant Title :
 QLast Update : Thu May 11 11:33:20 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.783	231254	18.990 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.699	410773	23.974 ng/ml
2) t 2,2,4-Trimethylpentane	7.405	402246	23.568 ng/ml
3) t n-Heptane	7.742	143790	8.097 ng/ml
4) t Benzene	7.878	171747	8.199 ng/ml
6) t Toluene	10.610	513663	25.227 ng/ml
7) t Ethylbenzene	13.046	160739	8.387 ng/ml
8) t m-Xylene	13.179	318701	16.541 ng/ml
9) t O-Xylene	13.906	306122	16.456 ng/ml
10) t 1,2,4-Trimethylbenzene	16.181	301901	16.230 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB053023\
Data File : FB029882.D
Signal(s) : FID2B.CH
Acq On : 30 May 2023 10:59
Operator : YP/AJ
Sample : BSF0530S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0530S1

Integration File: Calibration.e
Quant Time: May 31 03:33:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051123.M
Quant Title :
QLast Update : Thu May 11 11:33:20 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

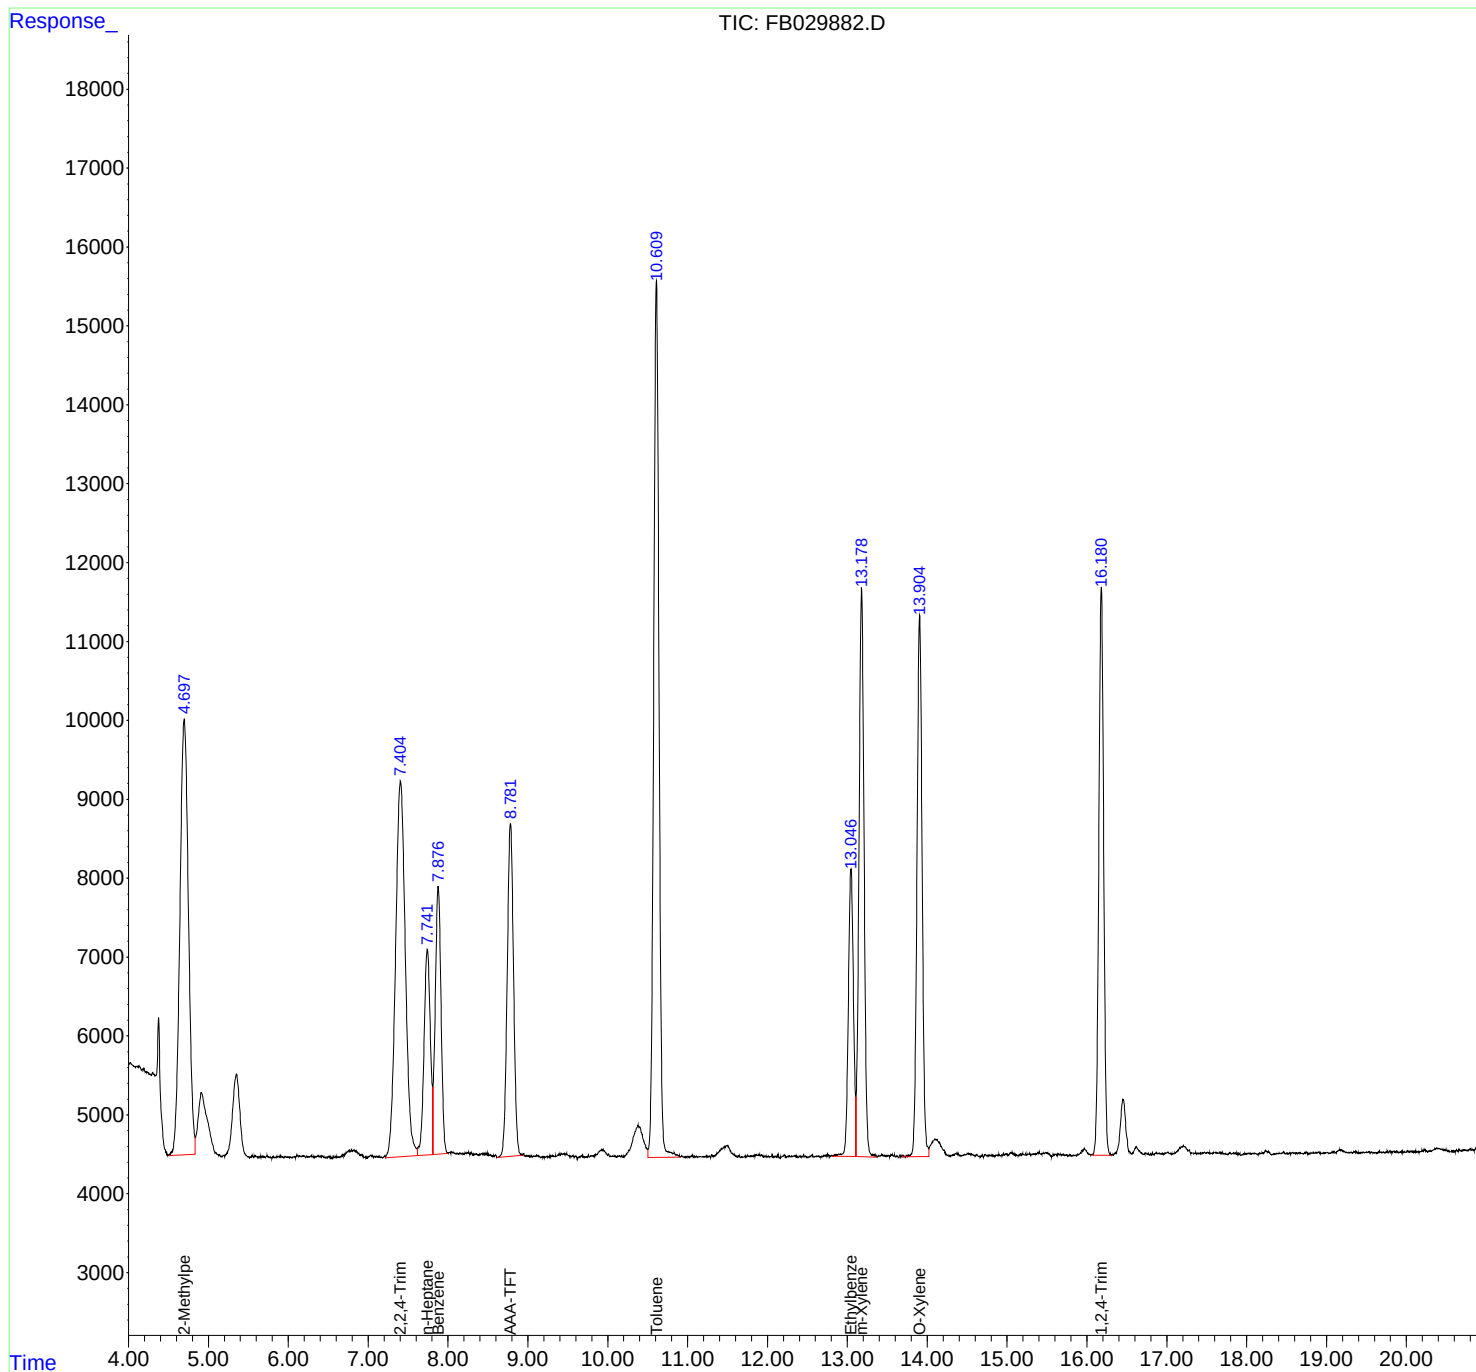


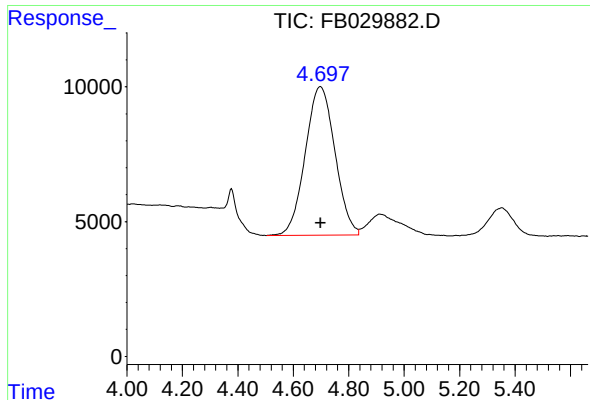

#1 2-Methylpentane


R.T.: 4.699 min
Delta R.T.: 0.000 min
Response: 410773
Conc: 23.97 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0530S1

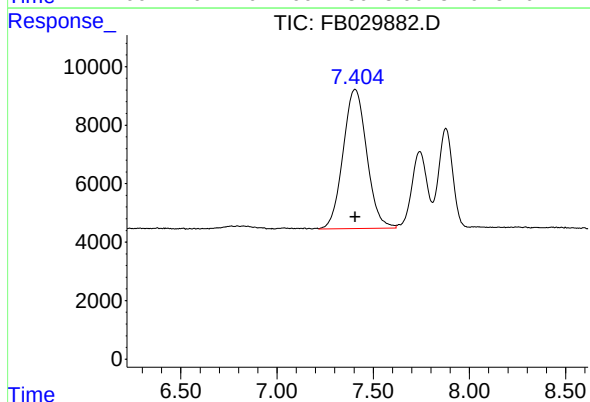


#2 2,2,4-Trimethylpentane

R.T.: 7.405 min
Delta R.T.: -0.001 min
Response: 402246
Conc: 23.57 ng/ml

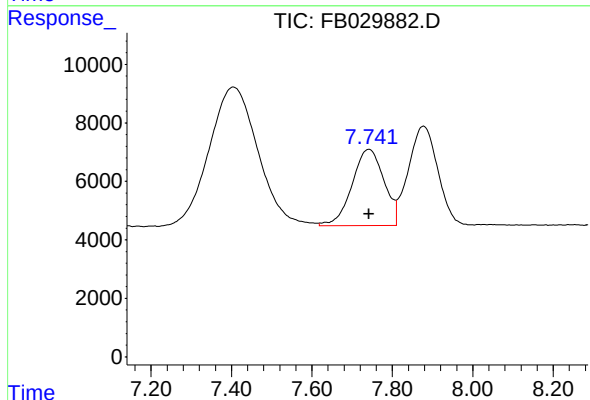


#3 n-Heptane

R.T.: 7.742 min
Delta R.T.: 0.000 min
Response: 143790
Conc: 8.10 ng/ml

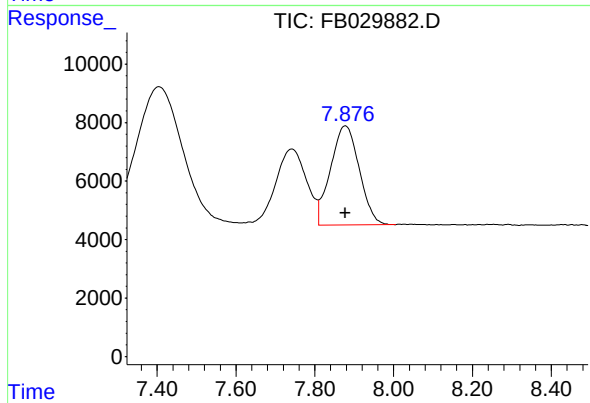

#4 Benzene


R.T.: 7.878 min
Delta R.T.: 0.000 min
Response: 171747
Conc: 8.20 ng/ml

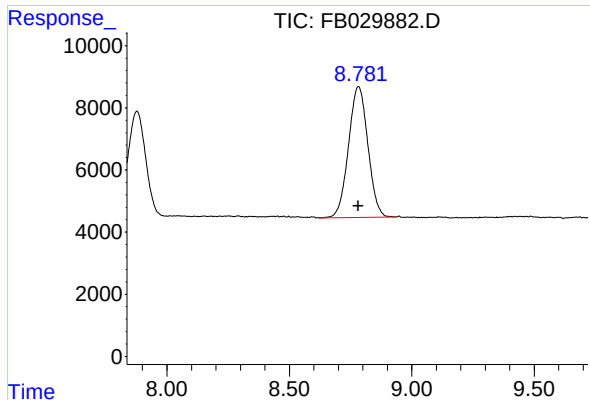

#5 AAA-TFT


R.T.: 8.783 min
Delta R.T.: 0.000 min
Response: 231254
Conc: 18.99 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0530S1

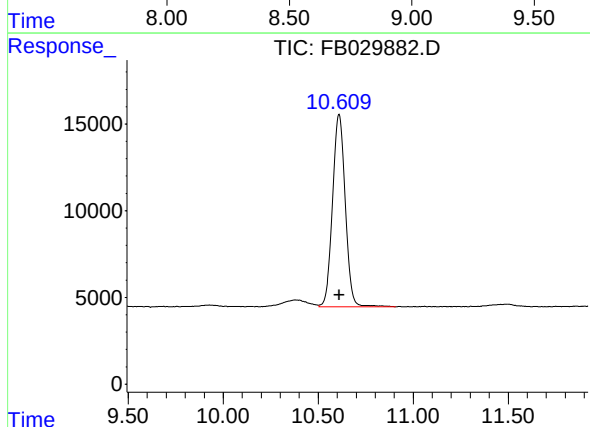


#6 Toluene

R.T.: 10.610 min
Delta R.T.: 0.000 min
Response: 513663
Conc: 25.23 ng/ml

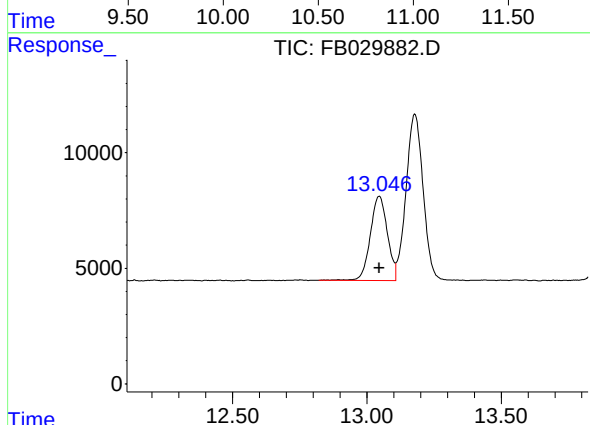


#7 Ethylbenzene

R.T.: 13.046 min
Delta R.T.: 0.000 min
Response: 160739
Conc: 8.39 ng/ml

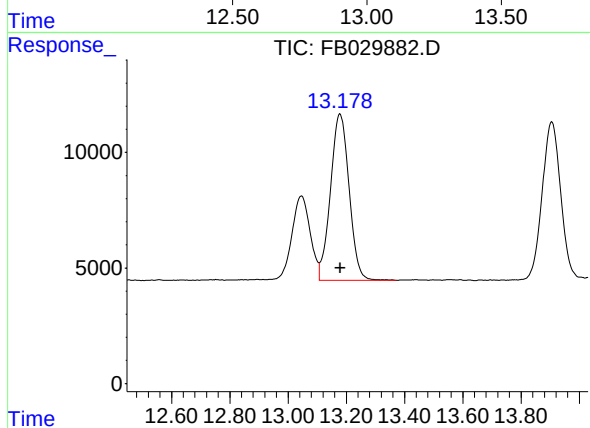

#8 m-Xylene


R.T.: 13.179 min
Delta R.T.: 0.000 min
Response: 318701
Conc: 16.54 ng/ml

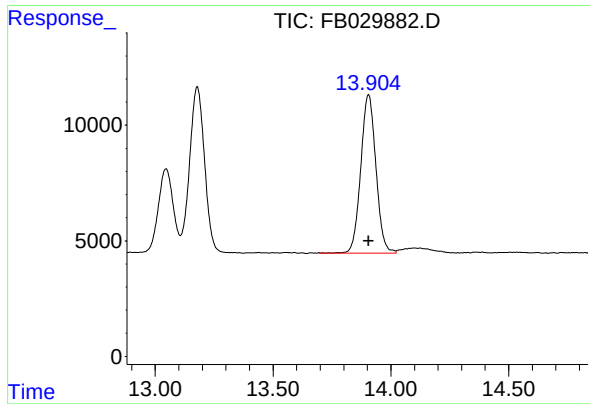

#9 O-Xylene

R.T.: 13.906 min
Delta R.T.: 0.000 min
Response: 306122
Conc: 16.46 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0530S1

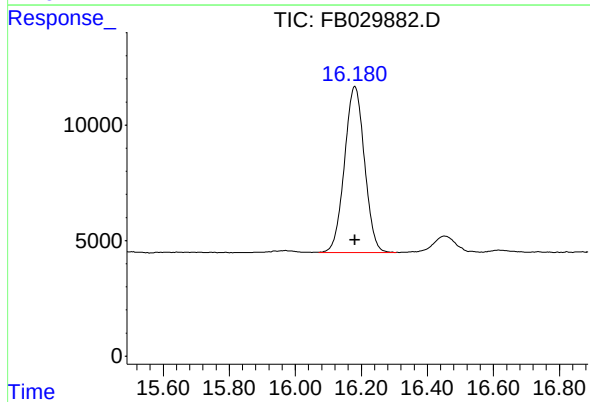

#10 1,2,4-Trimethylbenzene

R.T.: 16.181 min
Delta R.T.: 0.000 min
Response: 301901
Conc: 16.23 ng/ml