

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB053119\
 Data File : FB021259.D
 Signal(s) : FID2B.CH
 Acq On : 31 May 2019 9:21
 Operator : MJ/SJ
 Sample : BSF0531S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 31 23:59:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.995	310339	21.048 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.856	1169151	31.100 ng/ml
2) t 2,2,4-Trimethylpentane	7.611	1030628	30.179 ng/ml
3) t n-Heptane	7.951	327995	10.061 ng/ml
4) t Benzene	8.087	366458	10.617 ng/ml
6) t Toluene	10.840	752351	31.742 ng/ml
7) t Ethylbenzene	13.290	251195	10.750 ng/ml
8) t m-Xylene	13.423	535576	21.457 ng/ml
9) t O-Xylene	14.154	546075	20.933 ng/ml
10) t 1,2,4-Trimethylbenzene	16.439	553883	20.624 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB053119\
Data File : FB021259.D
Signal(s) : FID2B.CH
Acq On : 31 May 2019 9:21
Operator : MJ/SJ
Sample : BSF0531S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1


Integration File: Calibration.e
Quant Time: May 31 23:59:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

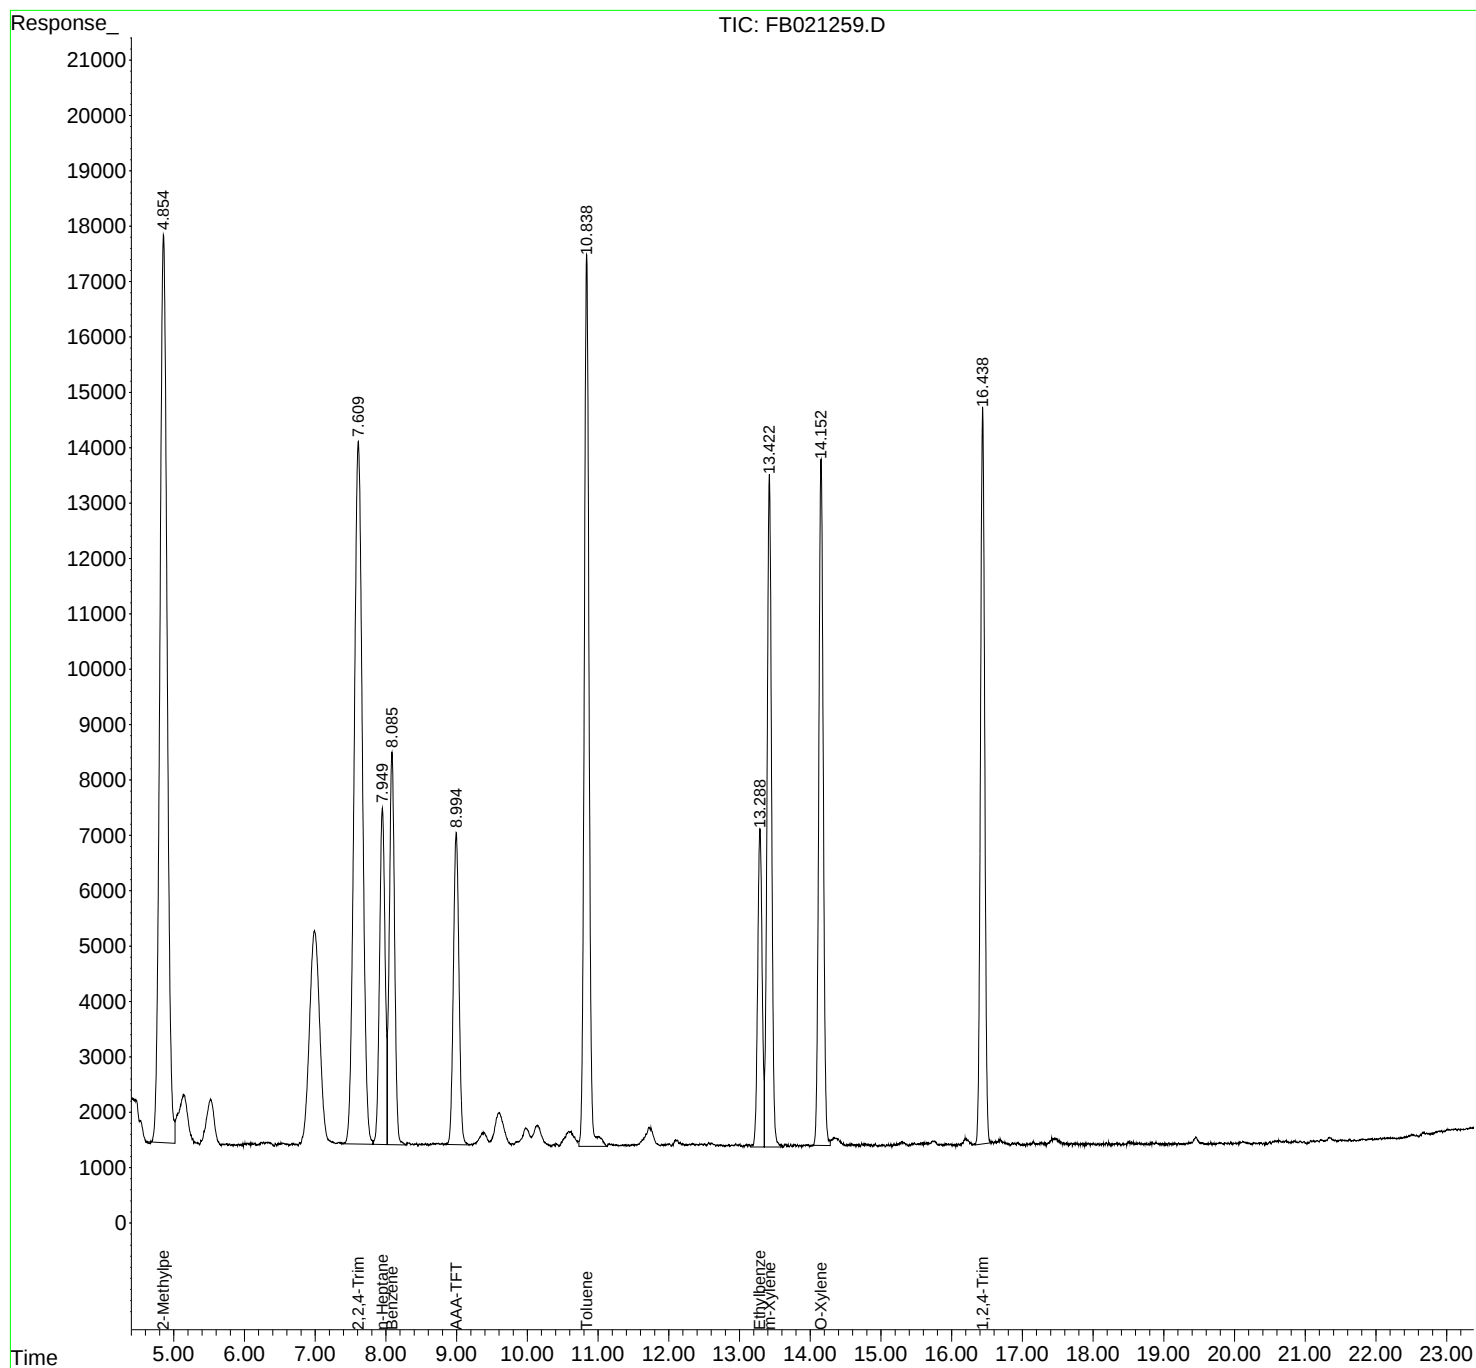


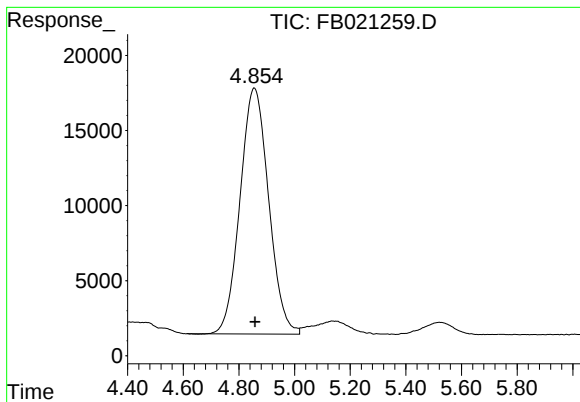


#1 2-Methylpentane
 R.T.: 4.856 min
 Delta R.T.: -0.002 min
 Response: 1169151
 Conc: 31.10 ng/ml

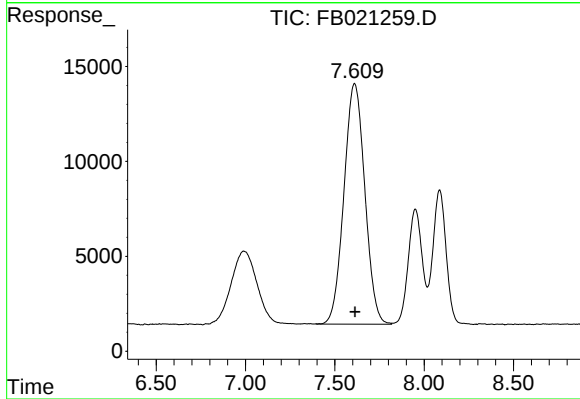


#2 2,2,4-Trimethylpentane
 R.T.: 7.611 min
 Delta R.T.: -0.003 min
 Response: 1030628
 Conc: 30.18 ng/ml

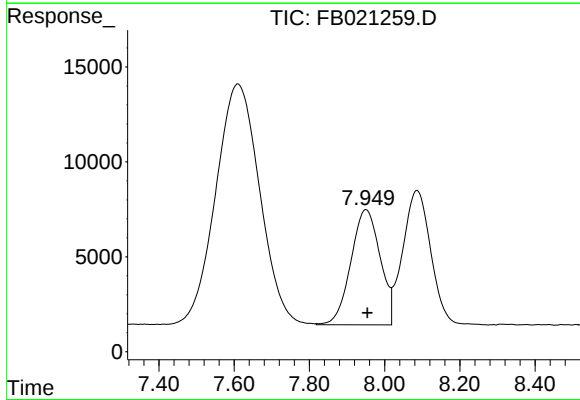

#3 n-Heptane
 R.T.: 7.951 min
 Delta R.T.: -0.003 min
 Response: 327995
 Conc: 10.06 ng/ml

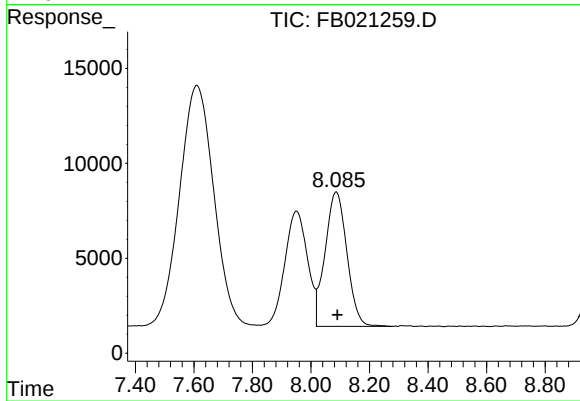


#4 Benzene
 R.T.: 8.087 min
 Delta R.T.: -0.003 min
 Response: 366458
 Conc: 10.62 ng/ml

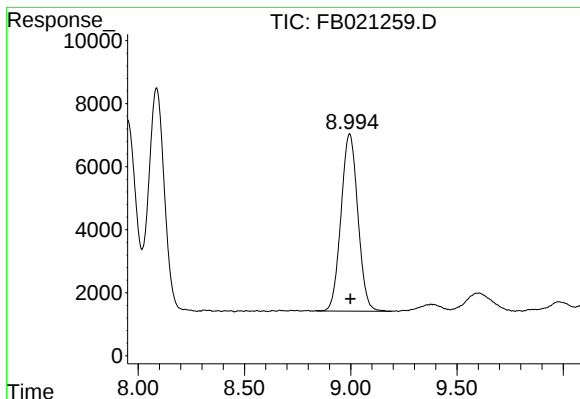


#5 AAA-TFT

R.T.: 8.995 min
Delta R.T.: -0.003 min
Response: 310339
Conc: 21.05 ng/ml

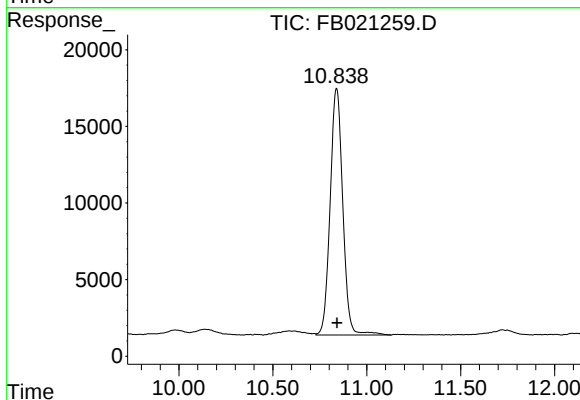


#6 Toluene

R.T.: 10.840 min
Delta R.T.: -0.003 min
Response: 752351
Conc: 31.74 ng/ml

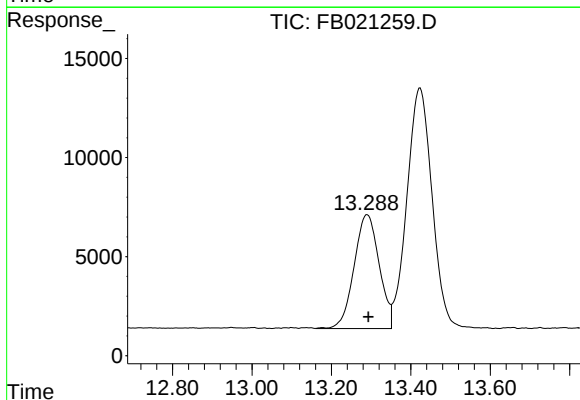


#7 Ethylbenzene

R.T.: 13.290 min
Delta R.T.: -0.003 min
Response: 251195
Conc: 10.75 ng/ml

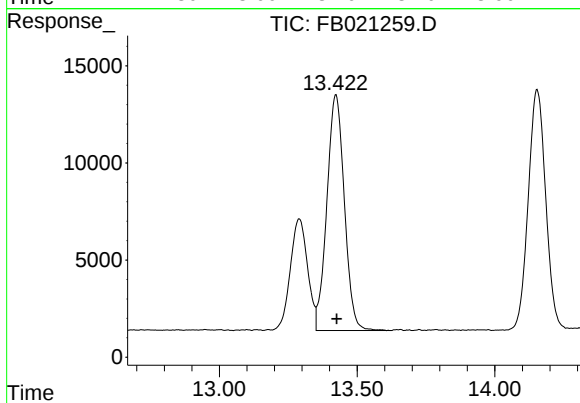


#8 m-Xylene

R.T.: 13.423 min
Delta R.T.: -0.003 min
Response: 535576
Conc: 21.46 ng/ml

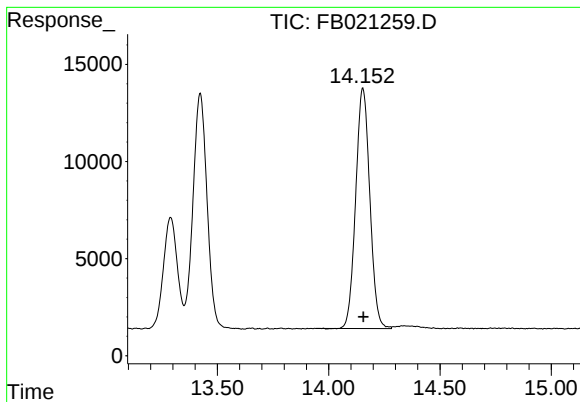

#9 O-Xylene

R.T.: 14.154 min
Delta R.T.: -0.003 min
Response: 546075
Conc: 20.93 ng/ml

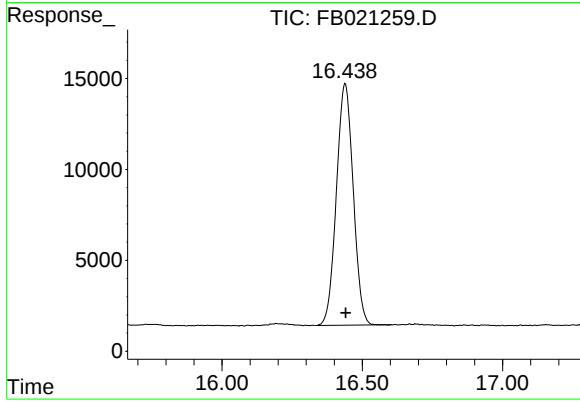

#10 1,2,4-Trimethylbenzene

R.T.: 16.439 min
Delta R.T.: -0.002 min
Response: 553883
Conc: 20.62 ng/ml