

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB053122\
 Data File : FB027326.D
 Signal(s) : FID2B.CH
 Acq On : 31 May 2022 11:55
 Operator : AJ/MA
 Sample : I.BLK
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 01 03:54:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
 Quant Title :
 QLast Update : Tue May 10 13:42:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	268584	25.586 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.427	9768	0.605 ng/ml
3) t n-Heptane	7.779	26300	1.609 ng/ml
4) t Benzene	7.863	1566	0.084 ng/ml
6) t Toluene	10.623	139664	7.867 ng/ml
7) t Ethylbenzene	13.058	64959	3.934 ng/ml
8) t m-Xylene	13.190	157314	9.561 ng/ml
9) t O-Xylene	13.923	87241	5.319 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	229449	13.743 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB053122\
Data File : FB027326.D
Signal(s) : FID2B.CH
Acq On : 31 May 2022 11:55
Operator : AJ/MA
Sample : I.BLK
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 01 03:54:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
Quant Title :
QLast Update : Tue May 10 13:42:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

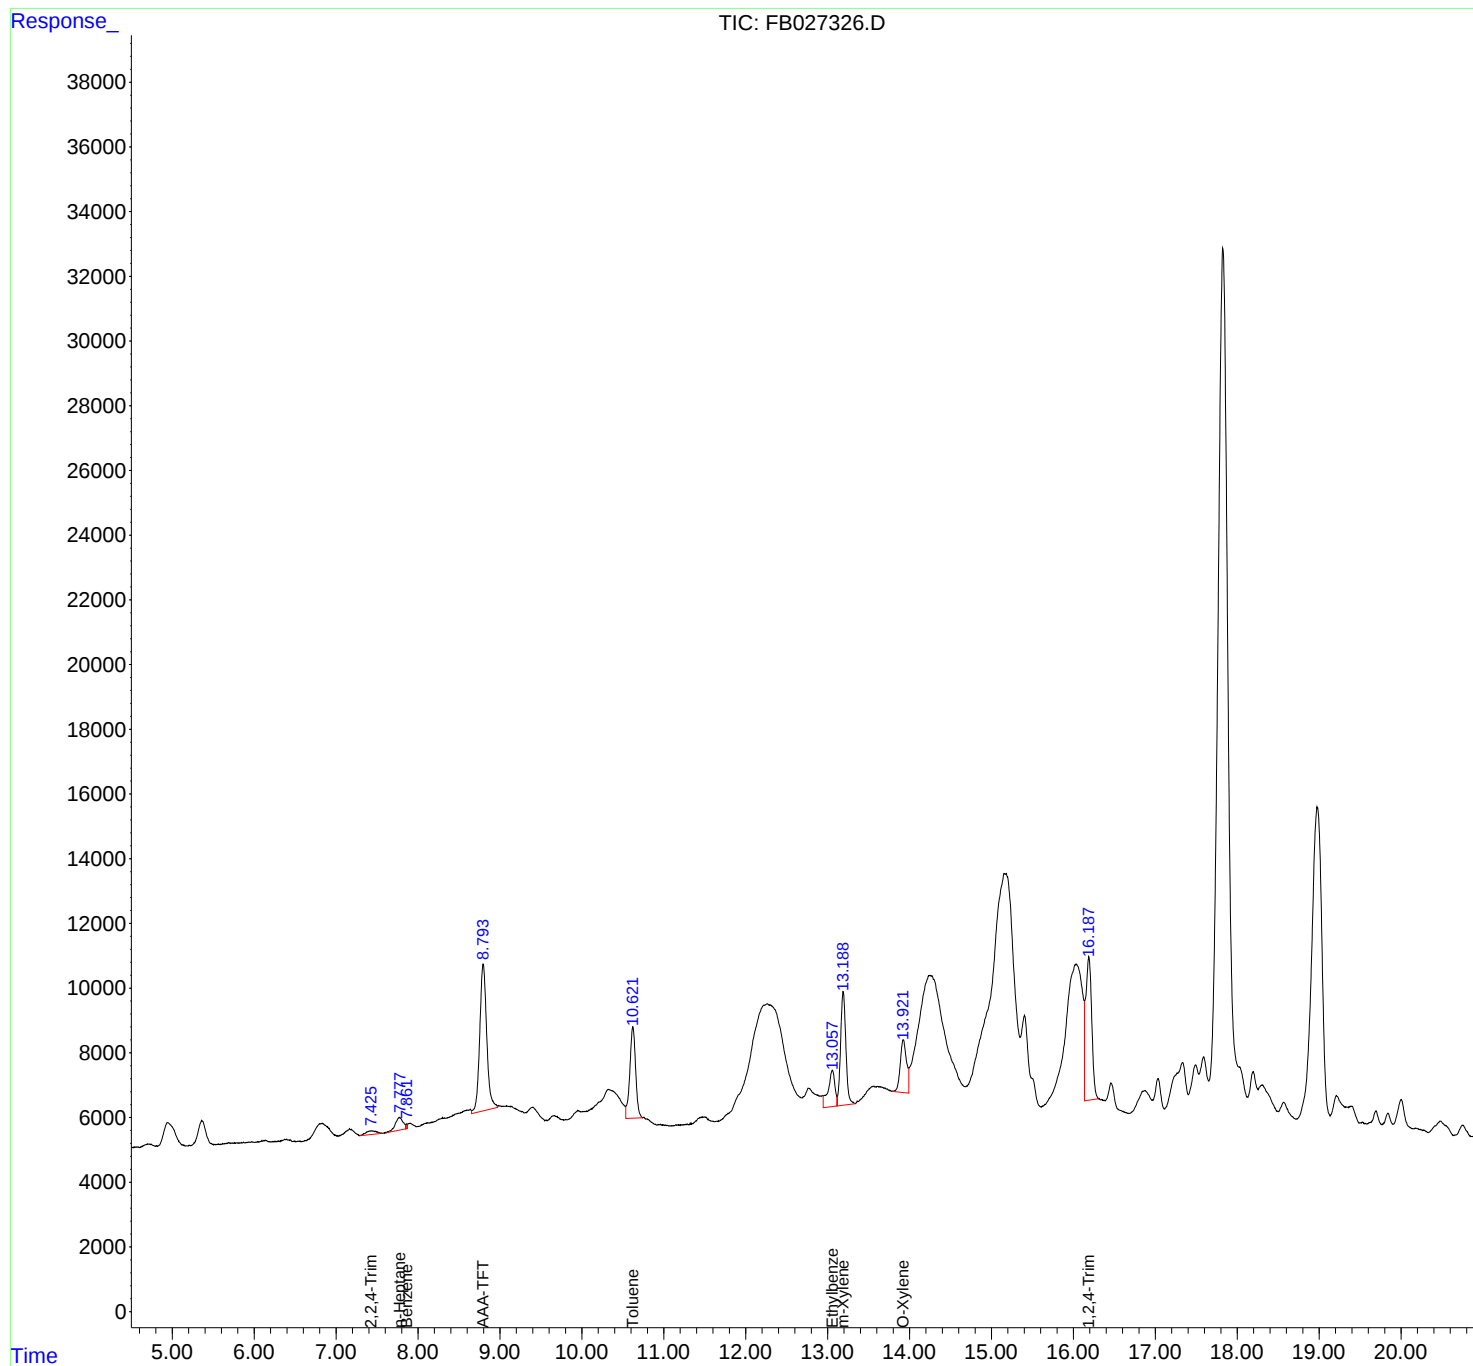


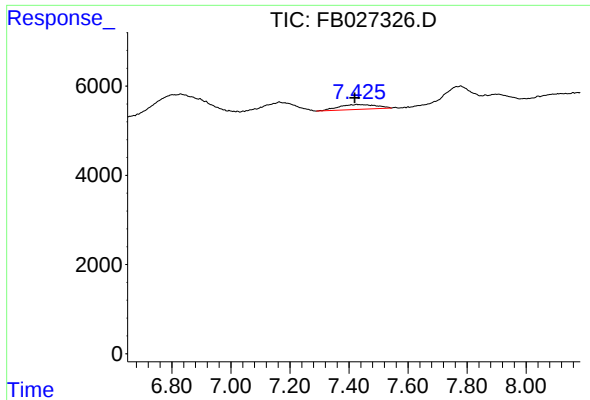

#2 2,2,4-Trimethylpentane


R.T.: 7.427 min
Delta R.T.: 0.007 min
Response: 9768
Conc: 0.61 ng/ml

Instrument :
FID_B
ClientSampleId :

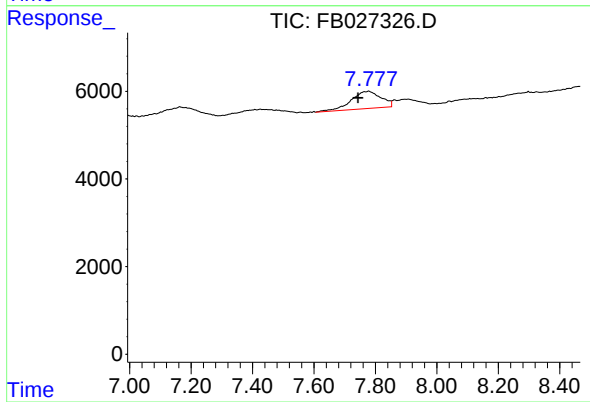


#3 n-Heptane

R.T.: 7.779 min
Delta R.T.: 0.036 min
Response: 26300
Conc: 1.61 ng/ml

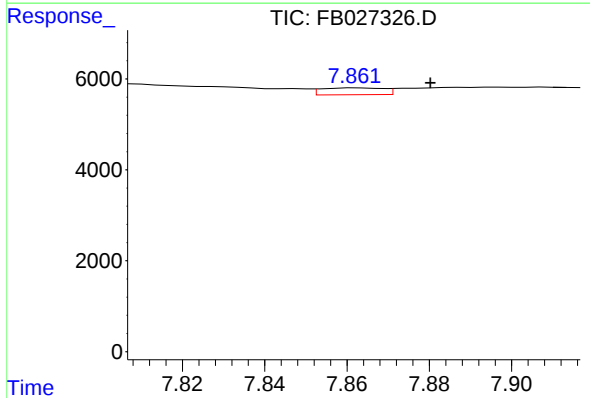


#4 Benzene

R.T.: 7.863 min
Delta R.T.: -0.017 min
Response: 1566
Conc: 0.08 ng/ml

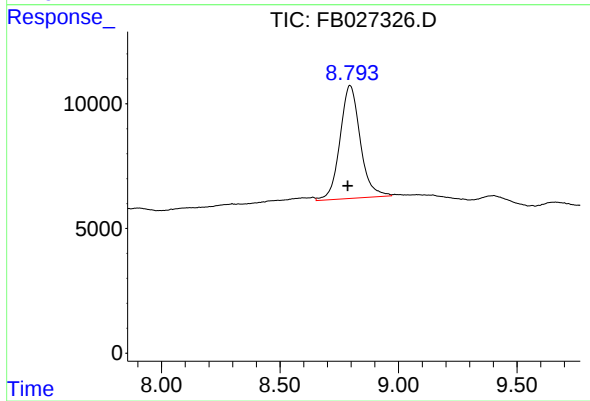

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.010 min
Response: 268584
Conc: 25.59 ng/ml

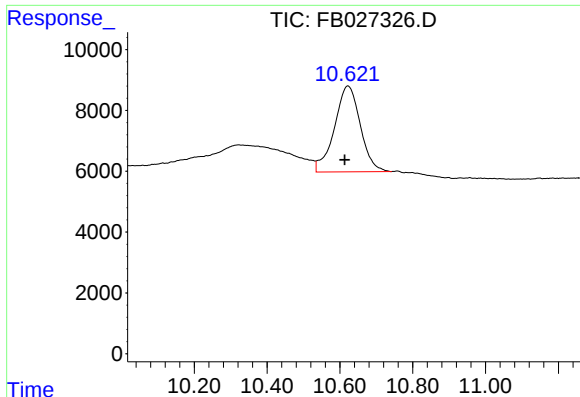

#6 Toluene


R.T.: 10.623 min
Delta R.T.: 0.010 min
Response: 139664
Conc: 7.87 ng/ml

Instrument :
FID_B
ClientSampleId :

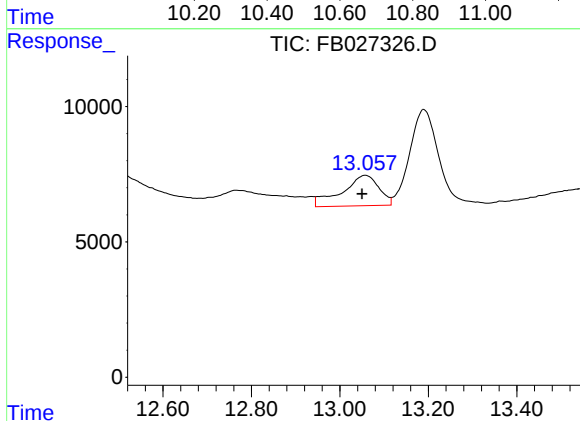


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.008 min
Response: 64959
Conc: 3.93 ng/ml

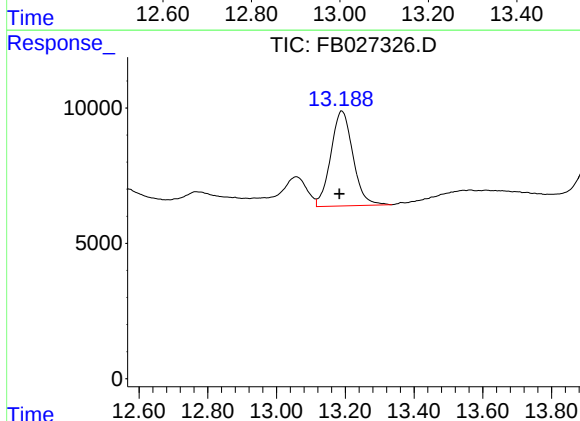


#8 m-Xylene

R.T.: 13.190 min
Delta R.T.: 0.007 min
Response: 157314
Conc: 9.56 ng/ml

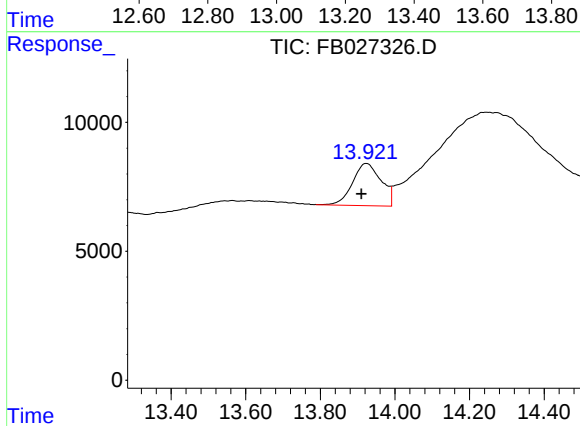

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: 0.013 min
Response: 87241
Conc: 5.32 ng/ml

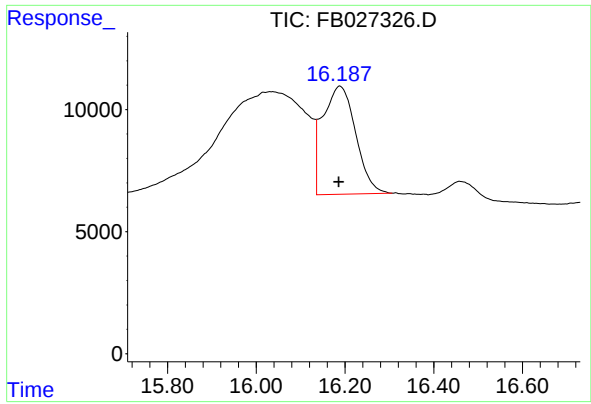

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: 0.003 min
Response: 229449
Conc: 13.74 ng/ml

Instrument :
FID_B
ClientSampleId :