

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB053122\
 Data File : FB027327.D
 Signal(s) : FID2B.CH
 Acq On : 31 May 2022 12:32
 Operator : AJ/MA
 Sample : I.BLK
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 01 03:54:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
 Quant Title :
 QLast Update : Tue May 10 13:42:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	220203	20.977 ng/ml
Target Compounds			
3) t n-Heptane	7.768	3624	0.222 ng/ml
6) t Toluene	10.626	33664	1.896 ng/ml
7) t Ethylbenzene	13.060	9985	0.605 ng/ml
8) t m-Xylene	13.192	38697	2.352 ng/ml
9) t O-Xylene	13.927	9626	0.587 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	26895	1.611 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB053122\
Data File : FB027327.D
Signal(s) : FID2B.CH
Acq On : 31 May 2022 12:32
Operator : AJ/MA
Sample : I.BLK
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 01 03:54:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
Quant Title :
QLast Update : Tue May 10 13:42:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

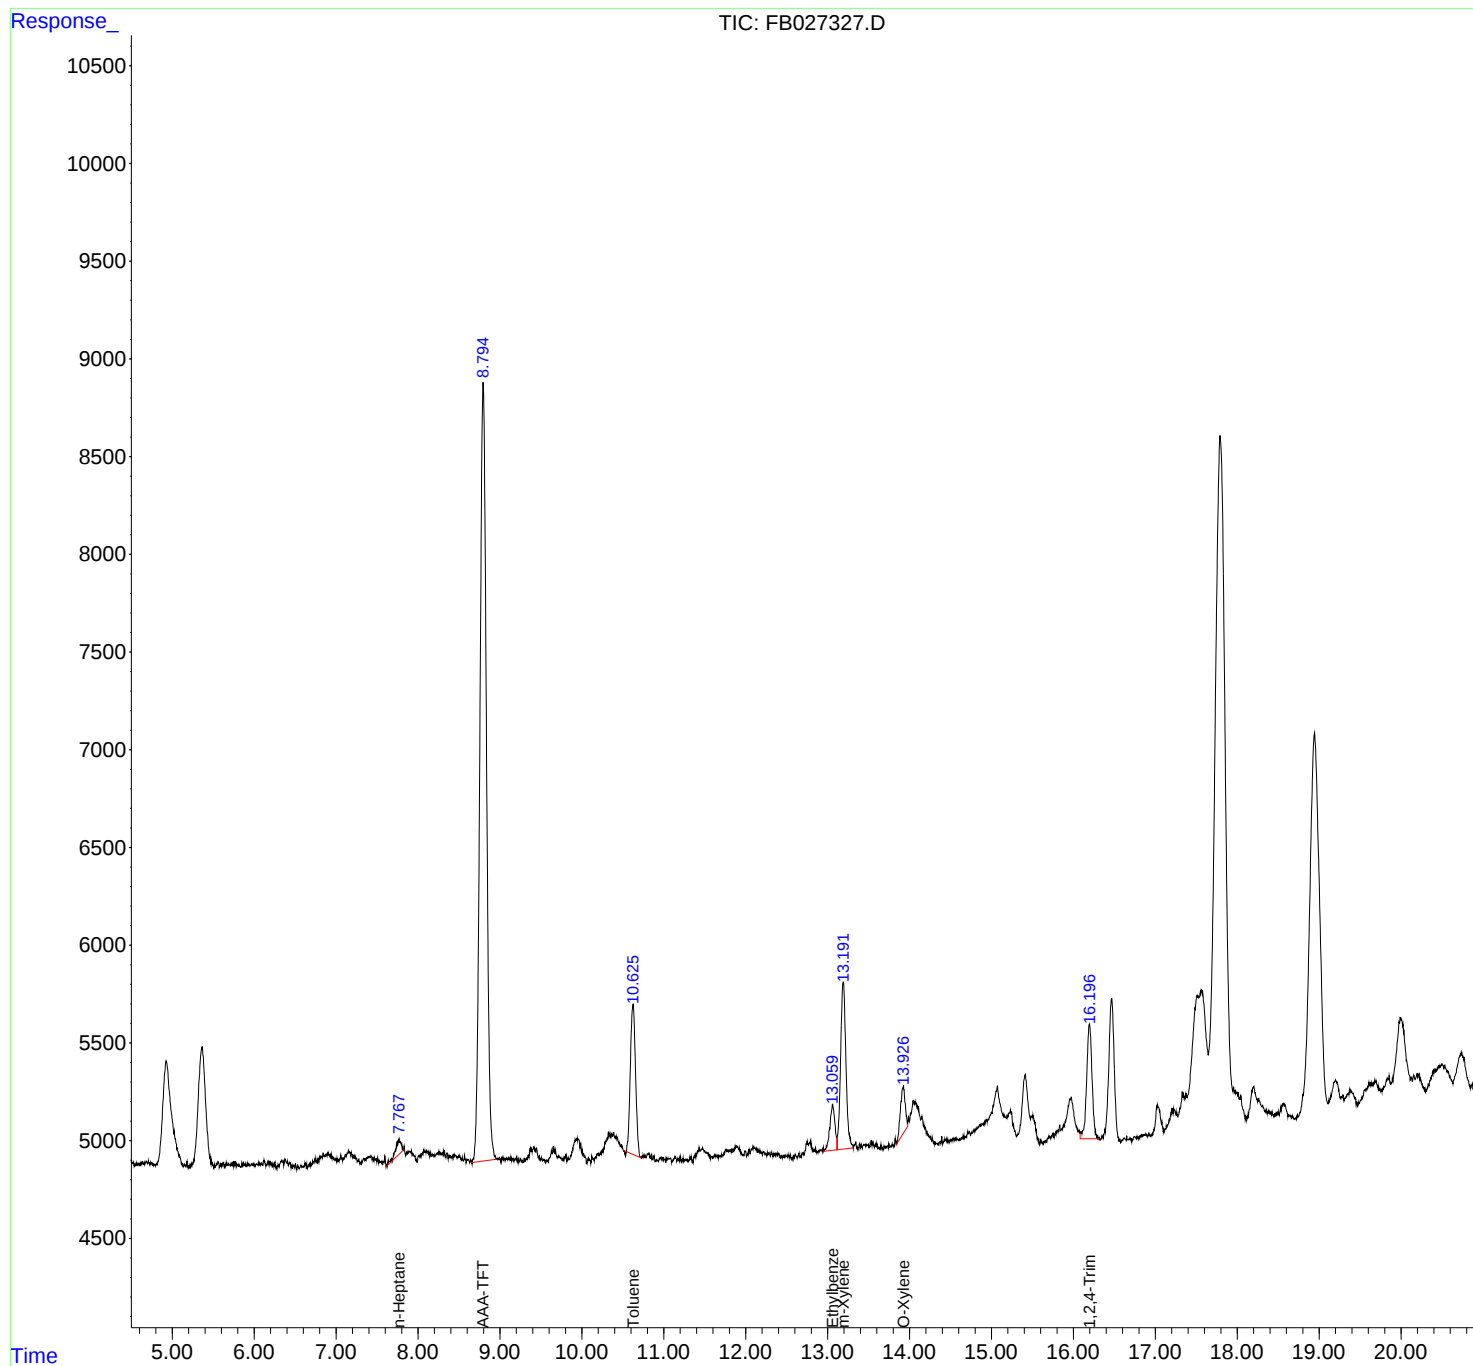


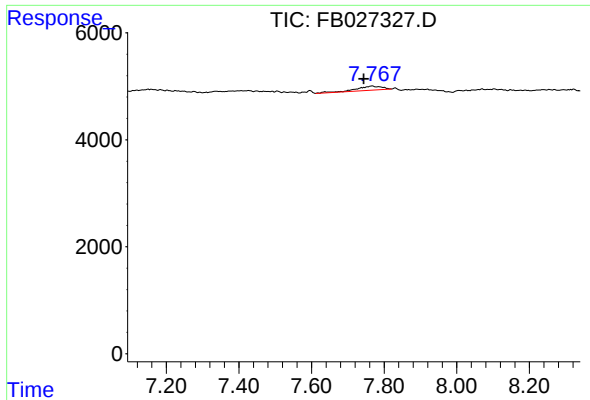

#3 n-Heptane


R.T.: 7.768 min
Delta R.T.: 0.024 min
Response: 3624
Conc: 0.22 ng/ml

Instrument :
FID_B
ClientSampleId :

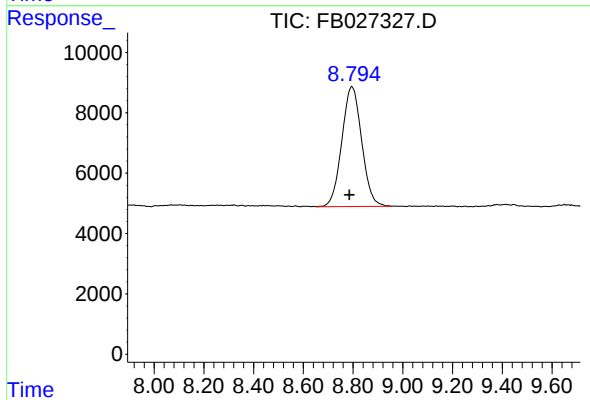


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: 0.010 min
Response: 220203
Conc: 20.98 ng/ml

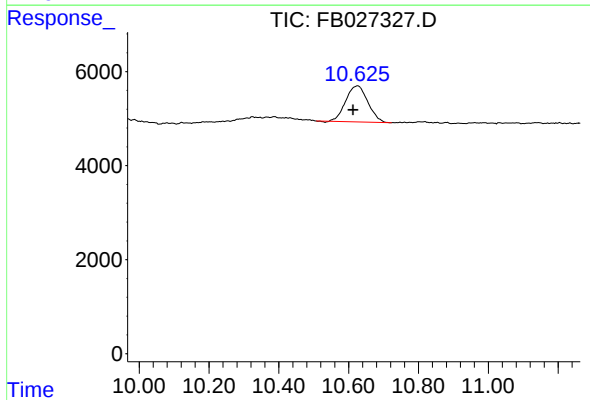


#6 Toluene

R.T.: 10.626 min
Delta R.T.: 0.013 min
Response: 33664
Conc: 1.90 ng/ml

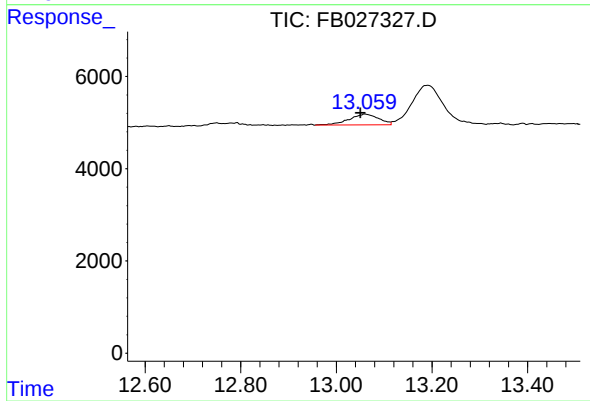

#7 Ethylbenzene


R.T.: 13.060 min
Delta R.T.: 0.010 min
Response: 9985
Conc: 0.60 ng/ml

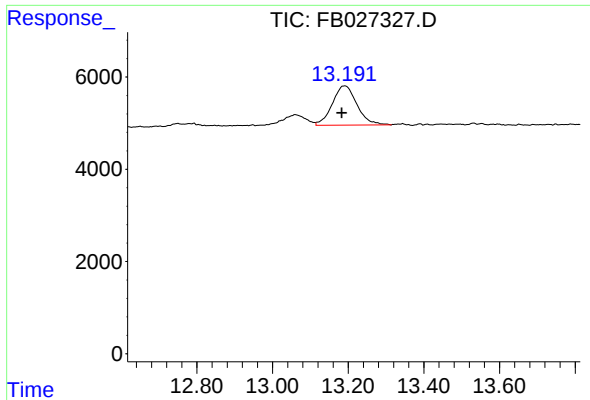

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: 0.009 min
Response: 38697
Conc: 2.35 ng/ml

Instrument :
FID_B
ClientSampleId :

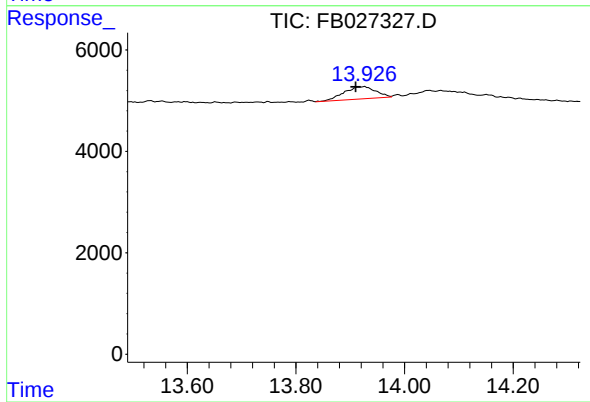

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: 0.017 min
Response: 9626
Conc: 0.59 ng/ml

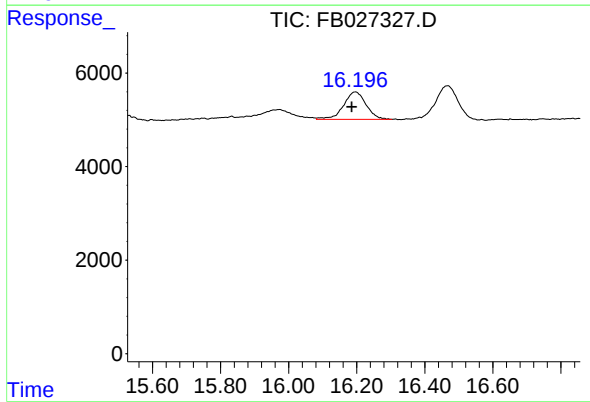

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.012 min
Response: 26895
Conc: 1.61 ng/ml