

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB053122\
Data File : FB027330.D
Signal(s) : FID2B.CH
Acq On : 31 May 2022 14:22
Operator : AJ/MA
Sample : I.BLK
Misc : 5.00G/5.00 ML MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 01 03:55:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
Quant Title :
QLast Update : Tue May 10 13:42:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	210228	20.027 ng/ml
Target Compounds			
6) t Toluene	10.619	10796	0.608 ng/ml
8) t m-Xylene	13.193	11153	0.678 ng/ml
9) t O-Xylene	13.922	2898	0.177 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	9021	0.540 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB053122\
Data File : FB027330.D
Signal(s) : FID2B.CH
Acq On : 31 May 2022 14:22
Operator : AJ/MA
Sample : I.BLK
Misc : 5.00G/5.00 ML MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 01 03:55:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
Quant Title :
QLast Update : Tue May 10 13:42:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

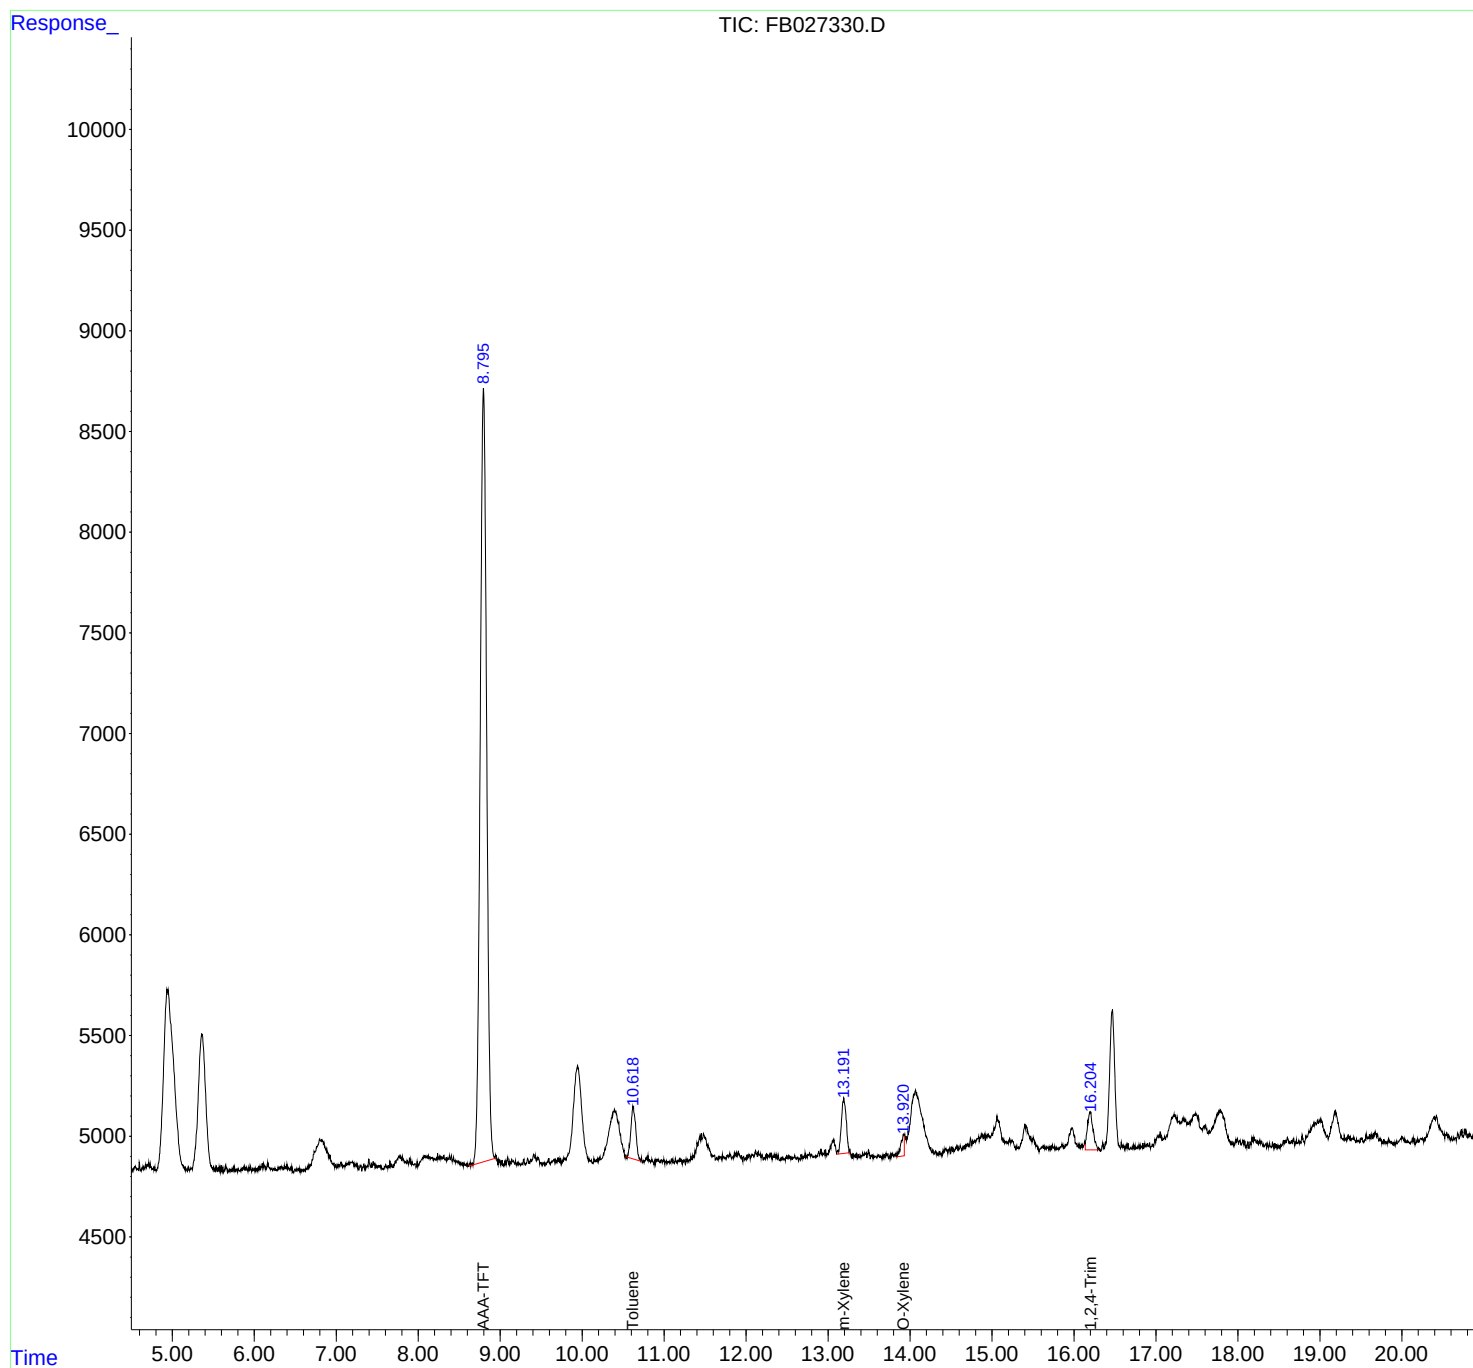


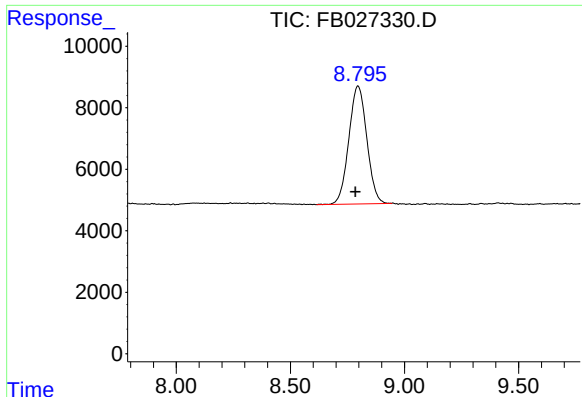

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: 0.011 min
Response: 210228
Conc: 20.03 ng/ml

Instrument :
FID_B
ClientSampleId :

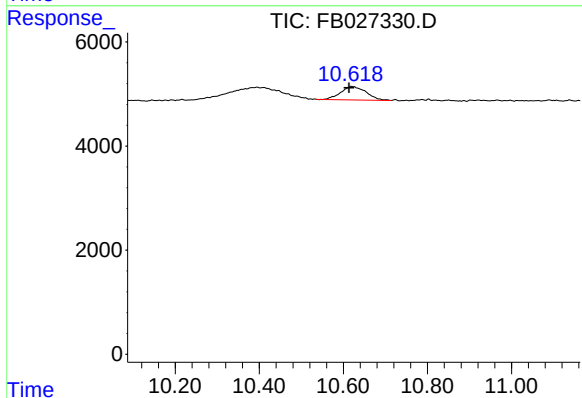


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.006 min
Response: 10796
Conc: 0.61 ng/ml

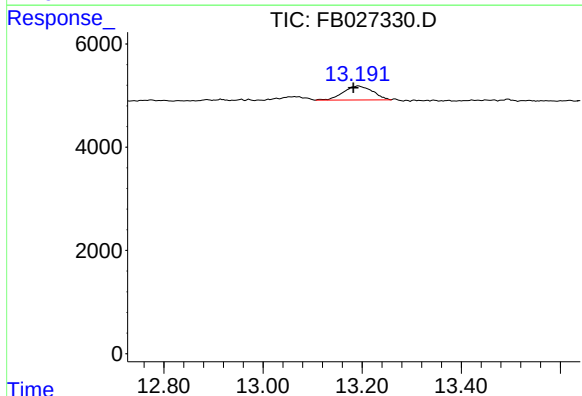


#8 m-Xylene

R.T.: 13.193 min
Delta R.T.: 0.010 min
Response: 11153
Conc: 0.68 ng/ml

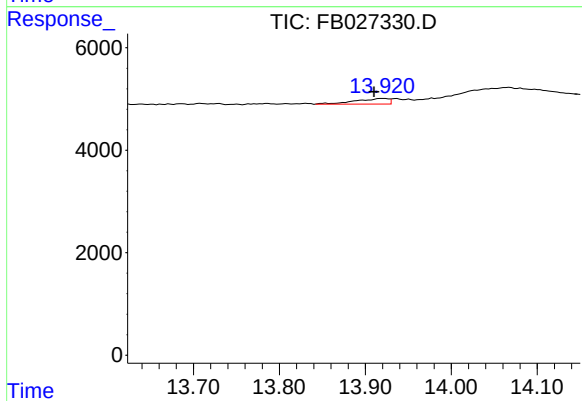

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.012 min
Response: 2898
Conc: 0.18 ng/ml

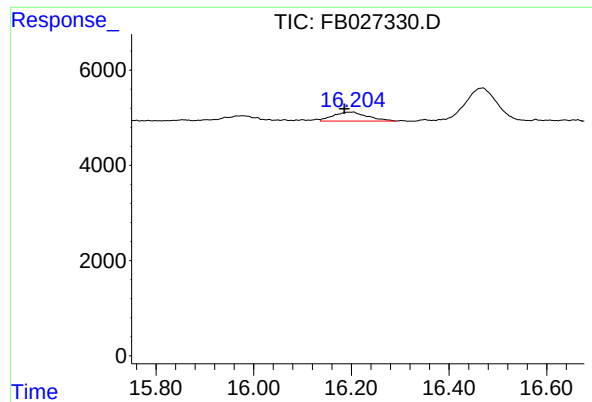

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: 0.019 min
Response: 9021
Conc: 0.54 ng/ml

Instrument :

FID_B

ClientSampleId :